

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051920\
 Data File : VV016121.D
 Acq On : 19 May 2020 14:44
 Operator : SY/MD
 Sample : L2711-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: May 20 02:29:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 20 01:20:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	147743	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	148432	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	66824	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35384	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.58	69	38400	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	2.13	63	57439	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.95	46	134159	58.68	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.36%
24) Chloroform-d	4.38	84	86941	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.06	65	51439	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.08	84	167700	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.10	67	54940	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.34	98	145020	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
45) trans-1,3-Dichloropropene-	7.65	79	17903	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
48) 2-Hexanone-d5	8.12	63	95874	51.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.16%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	40783	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	55840	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%


Target Compounds					Ovalue
25) Chloroform	4.41	83	5964	0.313 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV051920\
Data File : VV016121.D
Acq On : 19 May 2020 14:44
Operator : SY/MD
Sample : L2711-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: May 20 02:29:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 20 01:20:41 2020
Response via : Initial Calibration

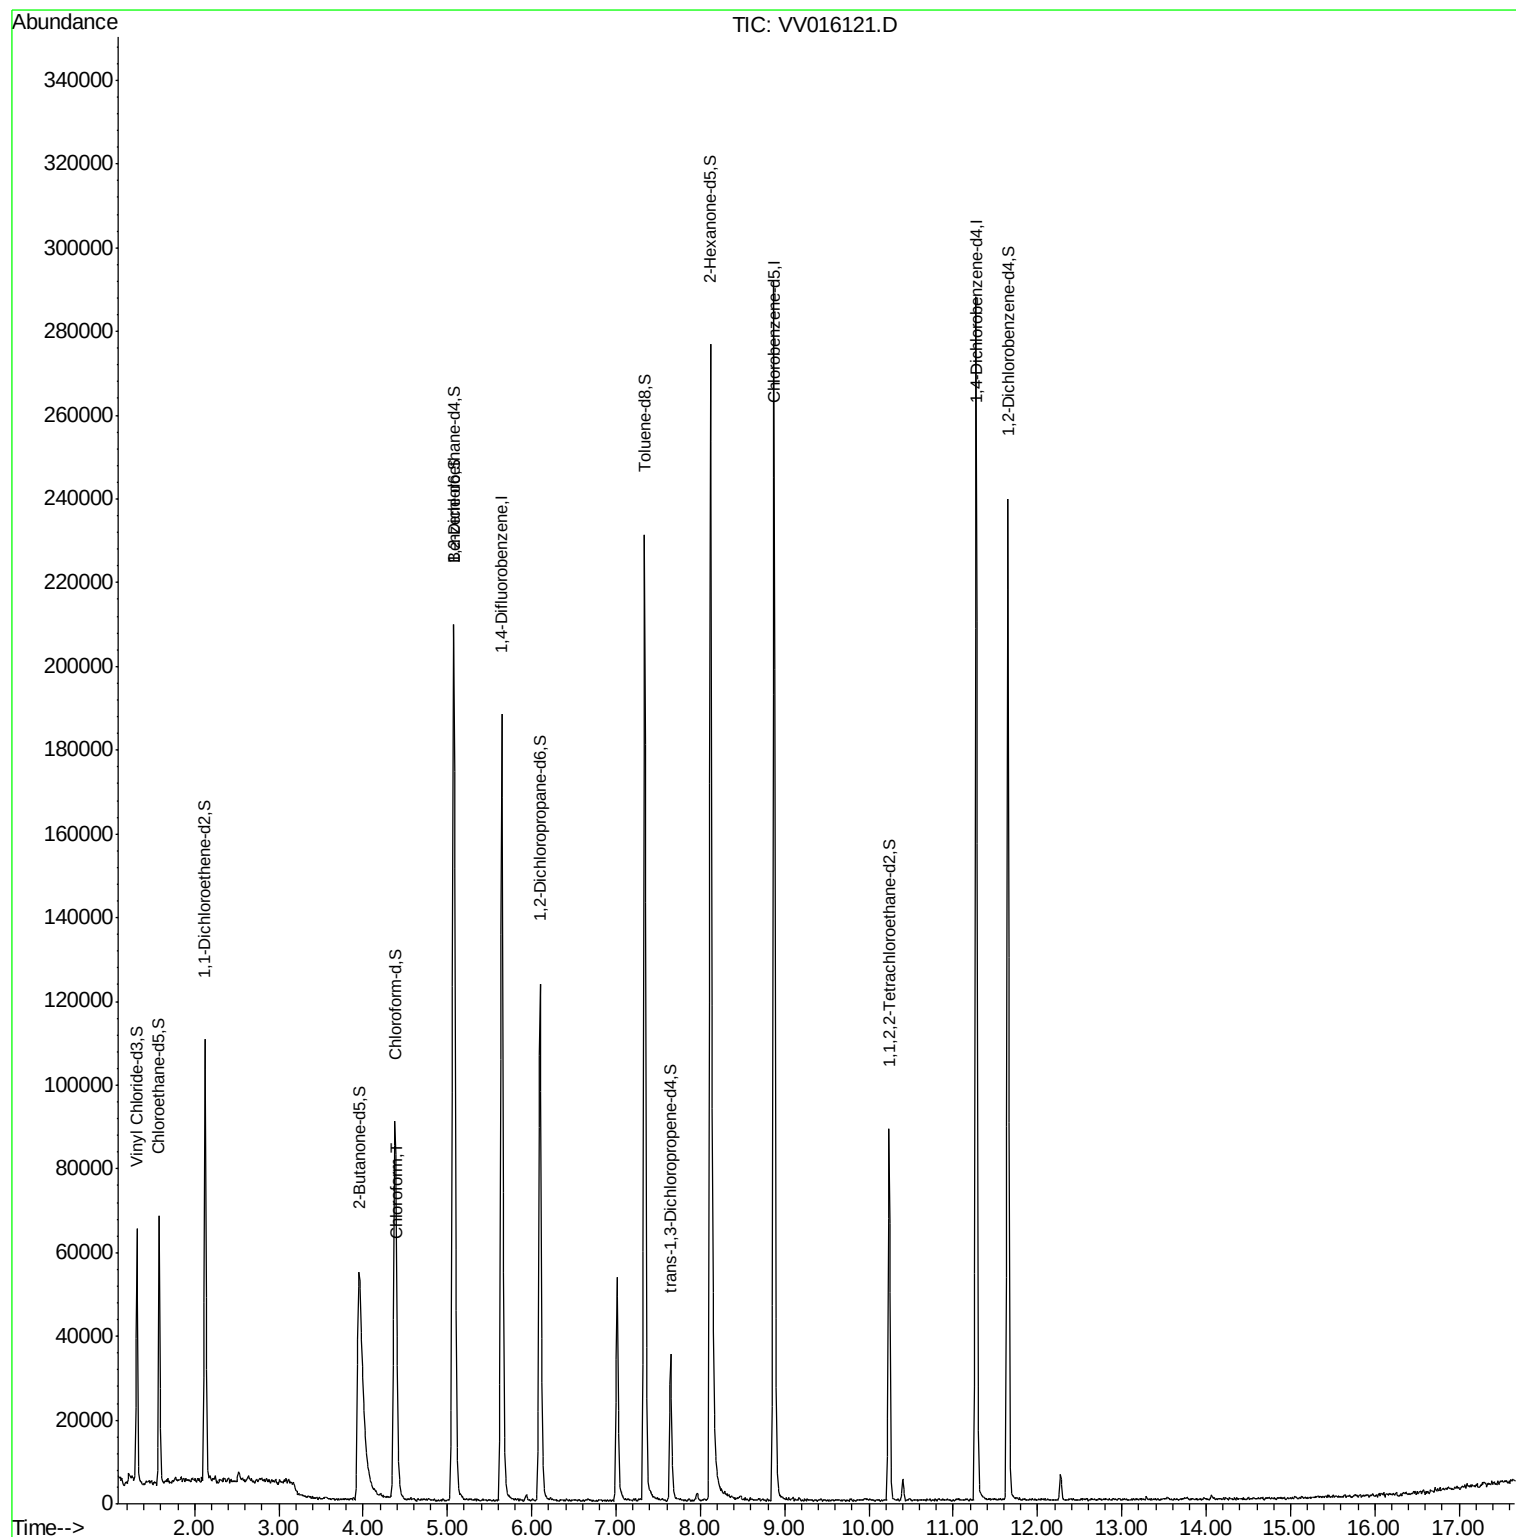

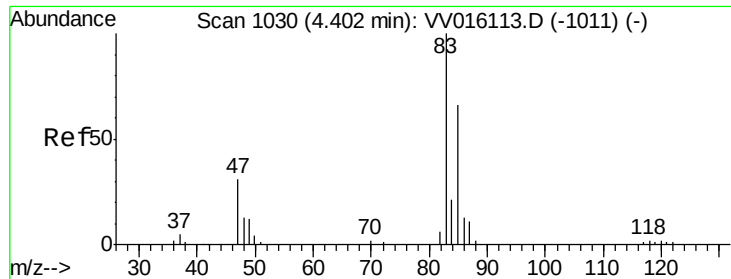

#25
 Chloroform
 Concen: 0.313 ug/L
 RT: 4.41 min Scan# 1032
 Delta R.T. 0.01 min
 Lab File: VV016121.D
 Acq: 19 May 2020 14:44

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 83 Resp: 5964
 Ion Ratio Lower Upper
 83 100
 85 69.7 45.7 84.9

