


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051920\
 Data File : VV016112.D
 Acq On : 19 May 2020 09:21
 Operator : SY/MD
 Sample : BFB59
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB59

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed May 20 01:20:41 2020

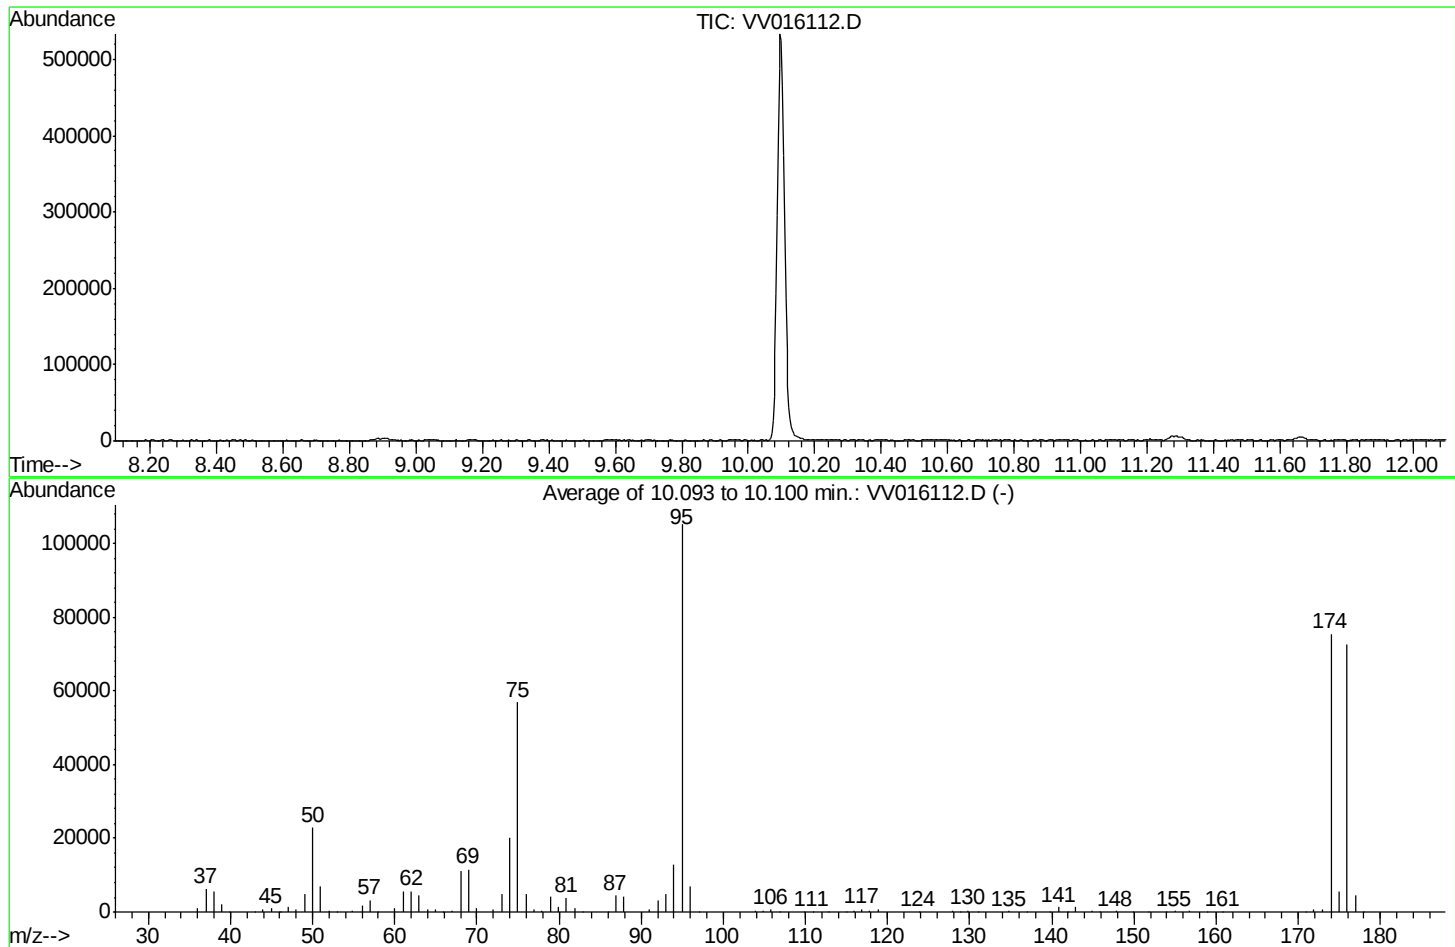

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	22810	PASS
75	95	30	80	54.0	56789	PASS
95	95	100	100	100.0	105170	PASS
96	95	5	9	6.7	7016	PASS
173	174	0.00	2	0.9	668	PASS
174	95	50	120	71.7	75394	PASS
175	174	5	9	7.5	5671	PASS
176	174	95	101	96.3	72576	PASS
177	176	5	9	6.5	4687	PASS

m/z	Abundance
36.00	1066.0
37.00	6247.0
38.00	5259.0
39.00	2122.0
39.90	449.0
43.10	123.0
44.00	1229.0
45.00	1035.0
46.20	190.0
47.00	1177.0
47.90	681.0
49.00	4628.0
50.00	21960.0
51.00	6548.0
52.00	270.0
52.90	189.0
54.90	334.0
56.00	1759.0
57.00	3136.0
57.90	156.0
60.00	1036.0
61.00	5571.0
62.00	5336.0
63.00	4124.0
63.90	580.0
65.00	730.0
65.90	174.0
66.90	350.0
68.00	10992.0
69.00	11142.0
70.00	923.0
72.00	620.0
73.00	4729.0
74.00	19424.0
75.00	54296.0
76.00	4533.0
76.90	638.0
78.00	335.0
78.90	4004.0
79.90	1220.0
80.90	3646.0
81.90	839.0
82.90	155.0
86.00	141.0
86.90	4297.0
87.90	4133.0
90.90	485.0
92.00	3115.0
93.00	4643.0
94.00	12401.0
95.00	98944.0
96.00	6691.0
97.00	181.0
103.90	501.0
104.90	196.0
105.80	606.0
106.80	163.0
109.80	108.0
110.90	110.0
112.80	143.0
114.90	141.0
115.80	430.0
116.80	737.0
117.80	439.0
118.90	578.0
123.80	107.0
127.90	394.0
128.90	155.0
129.80	429.0
131.00	162.0
134.80	172.0
137.00	187.0
140.90	1126.0
142.80	1197.0
144.90	258.0
145.90	154.0
147.90	272.0
149.90	145.0
151.80	101.0
153.90	120.0
155.00	195.0
156.80	212.0
158.90	129.0
160.90	128.0
170.90	102.0
171.80	842.0
173.00	927.0
174.00	69936.0
174.90	5362.0
175.90	67344.0
177.00	4372.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
36.00	1034.0
37.00	6707.0
38.00	5618.0
39.00	2281.0
39.90	401.0
43.00	131.0
44.00	1332.0
45.00	1081.0
46.10	175.0
47.00	1304.0
47.90	690.0
49.00	5077.0
50.00	23696.0
51.00	7066.0
52.00	287.0
52.90	182.0
54.90	360.0
56.00	1919.0
57.00	3474.0
57.90	172.0
60.00	1175.0
61.00	5867.0
62.00	5887.0
63.00	4601.0
63.90	567.0
65.00	772.0
65.90	150.0
67.00	347.0
68.00	11539.0
69.00	11875.0
70.00	1011.0
72.00	597.0
73.00	5192.0
74.00	21096.0
75.00	58664.0
76.00	4811.0
76.90	676.0
77.80	380.0
78.90	4307.0
79.90	1317.0
80.90	4060.0
81.90	928.0
82.90	169.0
86.10	152.0
86.90	4752.0
87.90	4354.0
90.90	598.0
92.00	3282.0
93.00	5089.0
94.00	13353.0
95.00	108808.0
96.00	7341.0
97.00	181.0
103.90	501.0
104.90	257.0
105.80	573.0
106.80	166.0
109.80	116.0
110.90	137.0
112.80	158.0
114.90	140.0
115.90	485.0
116.80	817.0
117.80	469.0
118.90	599.0
123.80	112.0
127.90	418.0
128.90	175.0
129.80	452.0
131.00	190.0
134.80	190.0
137.00	194.0
140.90	1363.0
142.00	134.0
142.80	1277.0
144.90	251.0
145.90	179.0
147.80	298.0
149.80	170.0
154.00	119.0
155.00	229.0
156.80	226.0
158.80	160.0
160.90	143.0
170.90	155.0
171.90	838.0
173.00	1077.0
173.90	77984.0
174.90	5835.0
175.90	74960.0
176.90	4762.0
177.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
36.00	945.0
37.00	6288.0
38.00	5486.0
39.00	2252.0
39.90	418.0
43.00	135.0
44.00	1295.0
45.00	1013.0
45.90	187.0
47.00	1269.0
47.90	651.0
49.00	4944.0
50.00	22776.0
51.00	6941.0
52.00	317.0
52.90	164.0
54.90	373.0
56.00	1850.0
57.00	3325.0
57.90	175.0
60.00	1215.0
61.00	5678.0
62.00	5988.0
63.00	4678.0
64.00	525.0
65.00	805.0
65.90	123.0
67.00	337.0
68.00	10974.0
69.00	11369.0
70.00	933.0
72.00	531.0
73.00	5205.0
74.00	20272.0
75.00	57408.0
76.00	4816.0
76.90	607.0
77.80	456.0
78.90	4100.0
79.90	1241.0
80.90	4159.0
81.90	945.0
82.90	141.0
86.10	171.0
86.90	4472.0
87.90	3996.0
90.90	600.0
92.00	3147.0
93.00	4978.0
94.00	12924.0
95.00	107760.0
96.00	7018.0
97.00	171.0
103.80	439.0
104.80	268.0
105.80	503.0
106.80	156.0
109.80	107.0
110.90	144.0
112.80	151.0
114.90	138.0
115.90	516.0
116.90	879.0
117.80	451.0
118.90	588.0
123.80	105.0
127.90	412.0
128.80	201.0
129.80	444.0
130.90	187.0
134.80	216.0
136.90	178.0
139.80	101.0
140.90	1441.0
142.00	138.0
142.80	1234.0
144.80	235.0
145.80	197.0
147.80	280.0
149.90	142.0
154.10	107.0
155.00	245.0
156.80	200.0
158.80	150.0
160.80	135.0
170.90	162.0
172.00	844.0
173.90	78264.0
175.00	5818.0
175.90	75424.0
176.90	4929.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

Scan 2788 (10.055 min): VV016112.D
BFB59

m/z	Abundance
39.90	261.0
42.80	117.0
43.90	538.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59