

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031104.D
 Acq On : 19 May 2023 14:05
 Operator : SY/MD
 Sample : VIBLK210
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	168654	186475	16.07%	2.110%
2	1.535	148	154	168	rVB	154667	178947	15.42%	2.025%
3	2.063	309	318	332	rBV	316667	460608	39.69%	5.212%
4	2.391	417	420	423	rBV4	1462	891	0.08%	0.010%
5	2.558	470	472	475	rBV4	1904	1374	0.12%	0.016%
6	2.683	508	511	514	rBV5	1577	1280	0.11%	0.014%
7	2.822	552	554	557	rBV4	1681	1142	0.10%	0.013%
8	2.857	563	565	570	rBV6	1639	1207	0.10%	0.014%
9	2.989	603	606	609	rVB4	1270	1045	0.09%	0.012%
10	3.008	609	612	615	rBV5	1497	1314	0.11%	0.015%
11	3.024	615	617	621	rVB5	1837	916	0.08%	0.010%
12	3.043	621	623	628	rBV5	1484	956	0.08%	0.011%
13	3.079	629	634	638	rBV8	1337	1712	0.15%	0.019%
14	3.275	692	695	698	rVB5	2399	1242	0.11%	0.014%
15	3.320	706	709	712	rBV5	1255	1004	0.09%	0.011%
16	3.346	715	717	721	rBV5	1515	980	0.08%	0.011%
17	3.371	721	725	728	rBV5	1928	1456	0.13%	0.016%
18	3.458	750	752	755	rVB3	1735	1128	0.10%	0.013%
19	3.542	776	778	782	rVV4	1581	1067	0.09%	0.012%
20	3.670	813	818	824	rBV9	2988	3285	0.28%	0.037%
21	3.802	848	859	892	rBV2	73014	237339	20.45%	2.686%
22	4.066	939	941	945	rVB5	2455	1146	0.10%	0.013%
23	4.259	986	1001	1022	rBV	186595	473107	40.77%	5.354%
24	4.548	1087	1091	1093	rBV5	1800	1622	0.14%	0.018%
25	4.609	1108	1110	1115	rBV6	1157	1077	0.09%	0.012%
26	4.876	1187	1193	1196	rBV7	2182	2321	0.20%	0.026%
27	4.963	1203	1220	1249	rBV2	436915	1160554	100.00%	13.133%
28	5.243	1306	1307	1311	rBV4	1507	899	0.08%	0.010%
29	5.542	1387	1400	1426	rBV	317533	666671	57.44%	7.544%
30	5.844	1484	1494	1509	rVV3	56565	116008	10.00%	1.313%
31	5.995	1530	1541	1562	rBV	253161	509823	43.93%	5.769%
32	6.423	1671	1674	1676	rBV4	1276	1032	0.09%	0.012%
33	6.532	1706	1708	1710	rVB3	2456	1076	0.09%	0.012%
34	6.551	1712	1714	1718	rVV4	1754	999	0.09%	0.011%
35	6.625	1734	1737	1743	rBV7	1314	1215	0.10%	0.014%
36	6.918	1819	1828	1851	rVV	132382	247883	21.36%	2.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031104.D
 Acq On : 19 May 2023 14:05
 Operator : SY/MD
 Sample : VIBLK210
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.249	1920	1931	1953	rBV	498217	872139	75.15%	9.870%
38	7.558	2018	2027	2046	rBV	96654	174782	15.06%	1.978%
39	7.882	2120	2128	2135	rBV2	11841	19467	1.68%	0.220%
40	7.979	2154	2158	2162	rBV7	1660	1552	0.13%	0.018%
41	8.034	2165	2175	2207	rVV	228351	467115	40.25%	5.286%
42	8.522	2325	2327	2330	rVB4	1954	1080	0.09%	0.012%
43	8.538	2330	2332	2337	rBV6	2322	1959	0.17%	0.022%
44	8.789	2398	2410	2430	rBV	490611	817795	70.47%	9.255%
45	9.062	2491	2495	2496	rBV3	2065	1367	0.12%	0.015%
46	9.153	2520	2523	2524	rBV3	1574	942	0.08%	0.011%
47	9.217	2539	2543	2545	rBV5	1461	1286	0.11%	0.015%
48	9.307	2568	2571	2577	rBV8	2351	2356	0.20%	0.027%
49	9.352	2583	2585	2588	rBV4	1781	1033	0.09%	0.012%
50	9.368	2588	2590	2594	rVV6	1771	1397	0.12%	0.016%
51	9.445	2611	2614	2616	rBV4	2385	1122	0.10%	0.013%
52	9.754	2706	2710	2711	rBV4	1474	1153	0.10%	0.013%
53	9.866	2741	2745	2747	rBV4	2185	1517	0.13%	0.017%
54	9.956	2770	2773	2776	rVB4	1370	896	0.08%	0.010%
55	9.976	2776	2779	2781	rBV3	2502	1424	0.12%	0.016%
56	10.159	2823	2836	2850	rBV	337805	541622	46.67%	6.129%
57	10.252	2863	2865	2867	rBV3	2236	1024	0.09%	0.012%
58	10.333	2881	2890	2899	rBV	21693	36623	3.16%	0.414%
59	10.413	2909	2915	2917	rBV6	1452	1724	0.15%	0.020%
60	10.474	2931	2934	2936	rBV4	2397	1406	0.12%	0.016%
61	10.529	2949	2951	2957	rBV6	2006	2074	0.18%	0.023%
62	10.564	2960	2962	2965	rBV4	1930	1412	0.12%	0.016%
63	10.844	3047	3049	3053	rBV5	1362	951	0.08%	0.011%
64	10.898	3063	3066	3068	rBV4	2128	1431	0.12%	0.016%
65	11.066	3115	3118	3120	rBV3	1574	1206	0.10%	0.014%
66	11.191	3146	3157	3175	rBV	470888	753379	64.92%	8.526%
67	11.455	3236	3239	3242	rBV5	2426	1279	0.11%	0.014%
68	11.567	3263	3274	3292	rBV	513679	799354	68.88%	9.046%
69	11.860	3364	3365	3372	rVB7	1964	1110	0.10%	0.013%
70	11.956	3392	3395	3398	rBV5	1229	971	0.08%	0.011%
71	12.033	3417	3419	3424	rVB6	1541	1113	0.10%	0.013%
72	12.101	3438	3440	3444	rBV5	2105	1396	0.12%	0.016%
73	12.156	3454	3457	3460	rBV5	1728	1348	0.12%	0.015%
74	12.281	3491	3496	3497	rBV5	1756	1143	0.10%	0.013%
75	12.480	3552	3558	3560	rBV7	2022	2242	0.19%	0.025%
76	12.525	3569	3572	3575	rVB5	1841	1567	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031104.D
 Acq On : 19 May 2023 14:05
 Operator : SY/MD
 Sample : VIBLK210
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.548	3575	3579	3581	rBV4	1496	1141	0.10%	0.013%
78	12.783	3649	3652	3655	rBV5	2056	1548	0.13%	0.018%
79	12.876	3678	3681	3683	rBV4	1809	1112	0.10%	0.013%
80	13.014	3722	3724	3726	rVB3	2469	971	0.08%	0.011%
81	13.091	3745	3748	3752	rBV5	2222	2132	0.18%	0.024%
82	13.156	3764	3768	3772	rBV7	1761	1562	0.13%	0.018%
83	13.175	3772	3774	3777	rBV4	2002	1303	0.11%	0.015%
84	13.246	3793	3796	3798	rVB4	1628	984	0.08%	0.011%
85	13.262	3798	3801	3802	rBV3	1916	1081	0.09%	0.012%
86	13.313	3811	3817	3818	rBV5	1895	1672	0.14%	0.019%
87	13.603	3900	3907	3909	rBV8	2323	2277	0.20%	0.026%
88	13.648	3916	3921	3924	rBV7	2204	1916	0.17%	0.022%
89	13.673	3924	3929	3930	rBV5	2842	2231	0.19%	0.025%
90	13.802	3964	3969	3970	rBV5	1254	999	0.09%	0.011%
91	14.162	4078	4081	4082	rVV3	1985	1108	0.10%	0.013%
92	14.236	4100	4104	4106	rVB5	2364	1533	0.13%	0.017%
93	14.249	4106	4108	4112	rBV5	2106	1436	0.12%	0.016%
94	14.374	4144	4147	4150	rVB5	2388	1595	0.14%	0.018%
95	14.397	4150	4154	4158	rBV7	2757	2873	0.25%	0.033%
96	14.496	4180	4185	4190	rBV8	2059	2393	0.21%	0.027%
97	14.631	4224	4227	4232	rBV6	3079	2870	0.25%	0.032%
98	14.702	4245	4249	4253	rBV6	2766	2511	0.22%	0.028%
99	15.139	4382	4385	4387	rBV4	2532	1539	0.13%	0.017%
100	15.757	4573	4577	4579	rBV5	2612	2301	0.20%	0.026%




Sum of corrected areas: 8836646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031104.D
Acq On : 19 May 2023 14:05
Operator : SY/MD
Sample : VIBLK210
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

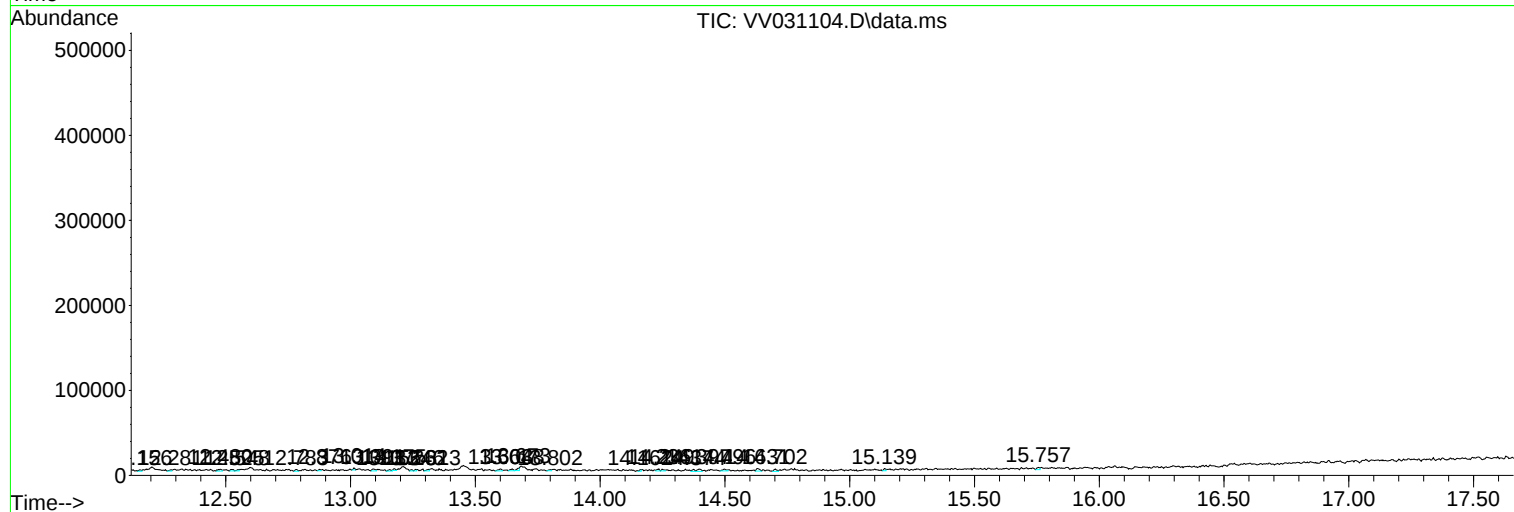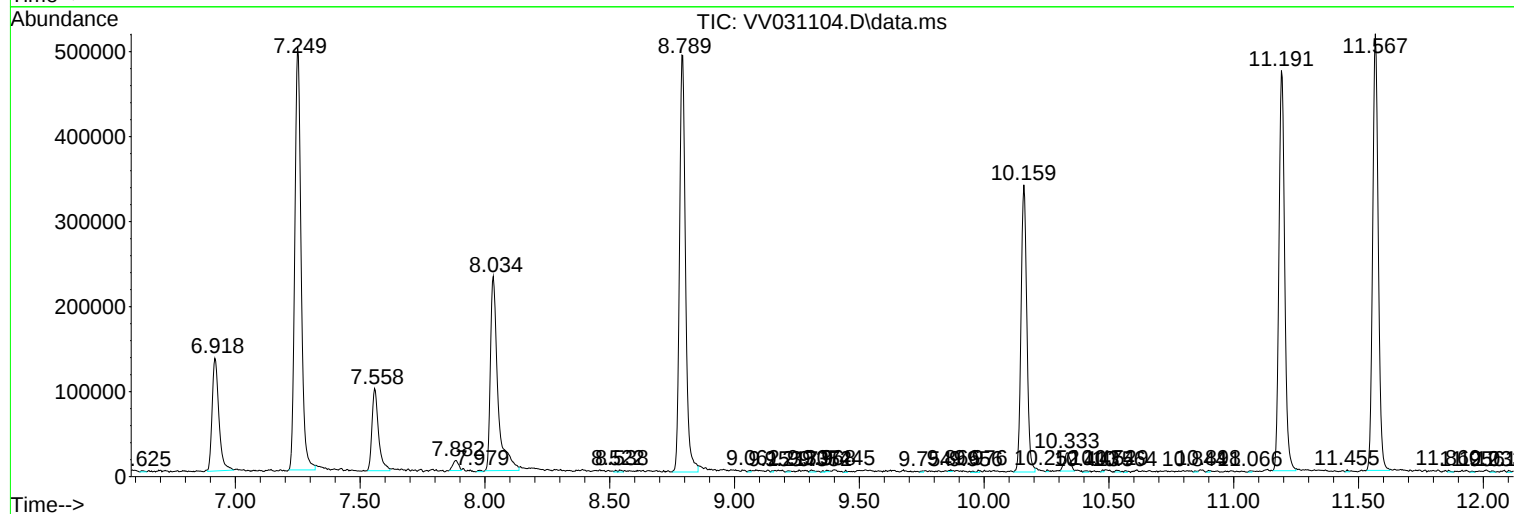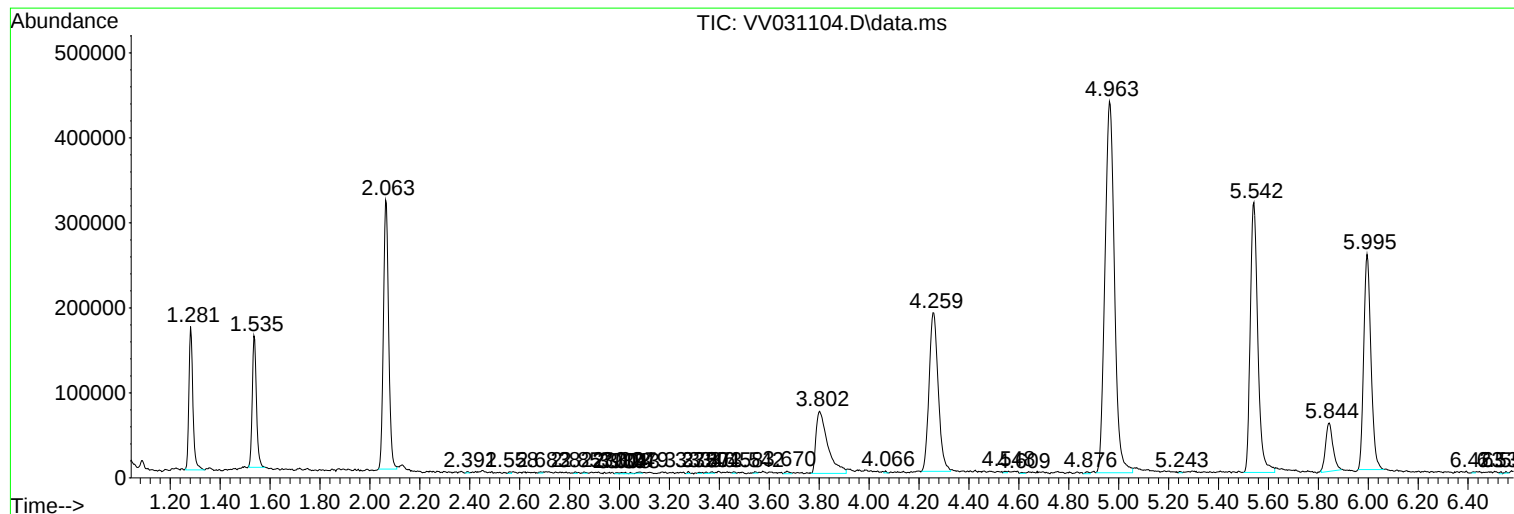

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031104.D
Acq On : 19 May 2023 14:05
Operator : SY/MD
Sample : VIBLK210
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031104.D
Acq On : 19 May 2023 14:05
Operator : SY/MD
Sample : VIBLK210
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------