

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031105.D
 Acq On : 19 May 2023 14:29
 Operator : SY/MD
 Sample : 02866-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	166173	179300	15.86%	2.035%
2	1.535	148	154	170	rVB	149593	179239	15.85%	2.034%
3	2.066	309	319	332	rBV	301572	442297	39.11%	5.020%
4	2.484	446	449	452	rBV4	1933	1486	0.13%	0.017%
5	2.693	510	514	517	rBV5	2990	3103	0.27%	0.035%
6	2.773	536	539	540	rBV3	1033	604	0.05%	0.007%
7	2.805	548	549	552	rBV3	1363	655	0.06%	0.007%
8	2.847	560	562	565	rBV3	1469	729	0.06%	0.008%
9	2.937	588	590	591	rBV2	1057	497	0.04%	0.006%
10	3.011	611	613	615	rBV3	1172	584	0.05%	0.007%
11	3.201	668	672	675	rBV6	2681	2605	0.23%	0.030%
12	3.236	681	683	686	rBV3	2701	1813	0.16%	0.021%
13	3.281	694	697	699	rBV4	2471	1183	0.10%	0.013%
14	3.352	716	719	722	rVB5	1781	1124	0.10%	0.013%
15	3.368	722	724	728	rBV4	1242	555	0.05%	0.006%
16	3.400	732	734	738	rVB5	1753	1003	0.09%	0.011%
17	3.423	738	741	744	rBV5	1832	1402	0.12%	0.016%
18	3.465	751	754	756	rBV4	1845	1048	0.09%	0.012%
19	3.522	769	772	773	rBV3	1316	768	0.07%	0.009%
20	3.539	773	777	778	rBV4	1491	974	0.09%	0.011%
21	3.587	789	792	794	rBV4	1681	1056	0.09%	0.012%
22	3.648	809	811	813	rBV3	1539	810	0.07%	0.009%
23	3.706	827	829	832	rVB4	1499	832	0.07%	0.009%
24	3.802	849	859	879	rBV	69778	198641	17.57%	2.254%
25	4.159	968	970	971	rBV2	1232	510	0.05%	0.006%
26	4.256	988	1000	1021	rVB2	180516	445473	39.39%	5.056%
27	4.493	1071	1074	1077	rBV5	2683	2066	0.18%	0.023%
28	4.696	1134	1137	1138	rBV3	1723	921	0.08%	0.010%
29	4.844	1177	1183	1186	rBV6	3457	2991	0.26%	0.034%
30	4.860	1186	1188	1191	rBV4	2108	1485	0.13%	0.017%
31	4.892	1196	1198	1199	rBV2	1494	684	0.06%	0.008%
32	4.963	1204	1220	1247	rBV2	431072	1130839	100.00%	12.834%
33	5.284	1319	1320	1323	rBV3	1392	664	0.06%	0.008%
34	5.381	1347	1350	1353	rBV4	2393	1510	0.13%	0.017%
35	5.487	1381	1383	1386	rBV4	1582	979	0.09%	0.011%
36	5.542	1388	1400	1421	rVV	306064	634271	56.09%	7.198%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031105.D
 Acq On : 19 May 2023 14:29
 Operator : SY/MD
 Sample : 02866-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.841	1482	1493	1513	rBV	235070	458982	40.59%	5.209%
38	5.995	1530	1541	1561	rBV	247326	503351	44.51%	5.712%
39	6.429	1674	1676	1678	rBV3	1645	806	0.07%	0.009%
40	6.776	1781	1784	1786	rBV4	2136	1590	0.14%	0.018%
41	6.815	1793	1796	1800	rVB4	2701	2098	0.19%	0.024%
42	6.841	1800	1804	1806	rBV4	1870	1427	0.13%	0.016%
43	6.876	1813	1815	1816	rBV2	1945	618	0.05%	0.007%
44	6.918	1819	1828	1847	rVV2	128731	239011	21.14%	2.712%
45	7.117	1888	1890	1892	rBV3	2186	1183	0.10%	0.013%
46	7.249	1920	1931	1956	rBV	481958	867001	76.67%	9.839%
47	7.558	2019	2027	2043	rBV	95757	162775	14.39%	1.847%
48	7.960	2150	2152	2157	rBV5	1433	985	0.09%	0.011%
49	8.034	2163	2175	2191	rBV	229762	438876	38.81%	4.981%
50	8.670	2370	2373	2375	rBV4	1658	1246	0.11%	0.014%
51	8.738	2390	2394	2395	rBV4	1721	1174	0.10%	0.013%
52	8.789	2399	2410	2427	rBV	471595	785686	69.48%	8.917%
53	9.136	2514	2518	2520	rVB5	2417	1630	0.14%	0.018%
54	9.294	2565	2567	2570	rVB3	1877	914	0.08%	0.010%
55	9.339	2579	2581	2585	rVB5	1882	806	0.07%	0.009%
56	9.940	2765	2768	2770	rBV4	1898	1225	0.11%	0.014%
57	10.159	2824	2836	2855	rBV	339271	537156	47.50%	6.096%
58	10.413	2913	2915	2917	rBV3	1607	967	0.09%	0.011%
59	10.455	2926	2928	2931	rBV5	2389	1496	0.13%	0.017%
60	10.529	2949	2951	2954	rBV4	1129	598	0.05%	0.007%
61	10.664	2991	2993	2995	rBV3	1350	870	0.08%	0.010%
62	10.763	3022	3024	3027	rBV4	1195	753	0.07%	0.009%
63	10.779	3027	3029	3031	rBV3	1219	693	0.06%	0.008%
64	10.969	3083	3088	3092	rBV6	1856	2471	0.22%	0.028%
65	11.066	3115	3118	3120	rBV4	2079	1417	0.13%	0.016%
66	11.191	3146	3157	3177	rBV	458325	723892	64.01%	8.215%
67	11.567	3264	3274	3290	rVB	492449	779604	68.94%	8.848%
68	11.734	3323	3326	3327	rBV3	1722	717	0.06%	0.008%
69	11.776	3336	3339	3341	rBV4	1879	1046	0.09%	0.012%
70	11.898	3375	3377	3379	rBV3	1909	891	0.08%	0.010%
71	11.937	3388	3389	3391	rBV2	2025	738	0.07%	0.008%
72	12.024	3413	3416	3419	rVB4	2269	1632	0.14%	0.019%
73	12.043	3419	3422	3425	rBV5	2297	1766	0.16%	0.020%
74	12.104	3438	3441	3445	rBV5	1424	1324	0.12%	0.015%
75	12.149	3453	3455	3457	rBV3	1938	902	0.08%	0.010%
76	12.249	3483	3486	3489	rBV4	2263	1687	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031105.D
 Acq On : 19 May 2023 14:29
 Operator : SY/MD
 Sample : 02866-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.342	3513	3515	3519	rBV5	1624	1064	0.09%	0.012%
78	12.374	3521	3525	3526	rBV4	1781	1368	0.12%	0.016%
79	12.484	3557	3559	3562	rBV3	1266	681	0.06%	0.008%
80	12.506	3562	3566	3568	rBV5	2200	1500	0.13%	0.017%
81	12.590	3590	3592	3595	rBV4	2343	1373	0.12%	0.016%
82	12.664	3611	3615	3616	rBV4	1864	1134	0.10%	0.013%
83	12.702	3625	3627	3629	rBV3	2297	1157	0.10%	0.013%
84	12.750	3638	3642	3643	rBV3	2387	1757	0.16%	0.020%
85	12.815	3660	3662	3666	rVB4	1881	1095	0.10%	0.012%
86	13.014	3722	3724	3725	rBV2	1214	601	0.05%	0.007%
87	13.024	3725	3727	3731	rVV5	2634	1780	0.16%	0.020%
88	13.094	3746	3749	3750	rBV3	1336	553	0.05%	0.006%
89	13.165	3769	3771	3774	rVB4	1057	512	0.05%	0.006%
90	13.194	3774	3780	3781	rBV5	3532	3515	0.31%	0.040%
91	13.413	3845	3848	3852	rBV6	1754	1420	0.13%	0.016%
92	13.548	3887	3890	3892	rBV4	2284	1551	0.14%	0.018%
93	13.602	3906	3907	3910	rBV3	1291	757	0.07%	0.009%
94	13.734	3945	3948	3951	rVB5	1554	998	0.09%	0.011%
95	14.226	4097	4101	4103	rBV4	1535	1158	0.10%	0.013%
96	14.406	4152	4157	4158	rBV4	1860	1543	0.14%	0.018%
97	14.590	4211	4214	4216	rBV3	1928	1393	0.12%	0.016%
98	14.773	4268	4271	4272	rBV3	1822	782	0.07%	0.009%
99	14.863	4293	4299	4305	rBV3	2750	4513	0.40%	0.051%
100	14.927	4315	4319	4322	rBV6	2577	2557	0.23%	0.029%



Sum of corrected areas: 8811467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031105.D
Acq On : 19 May 2023 14:29
Operator : SY/MD
Sample : 02866-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

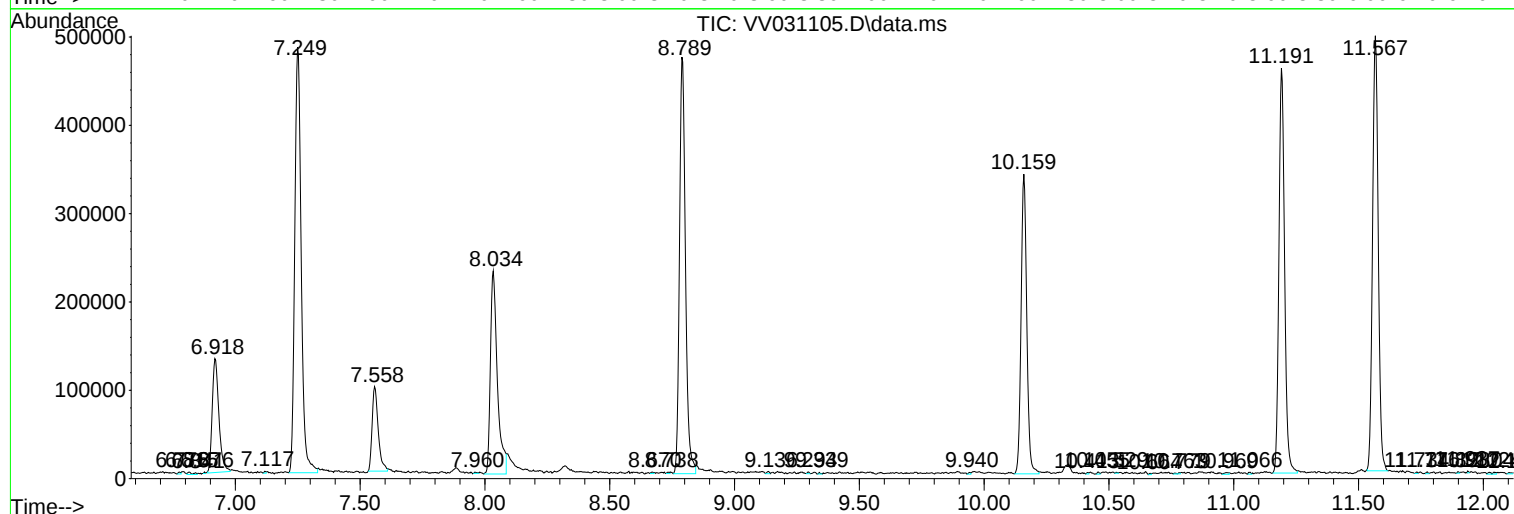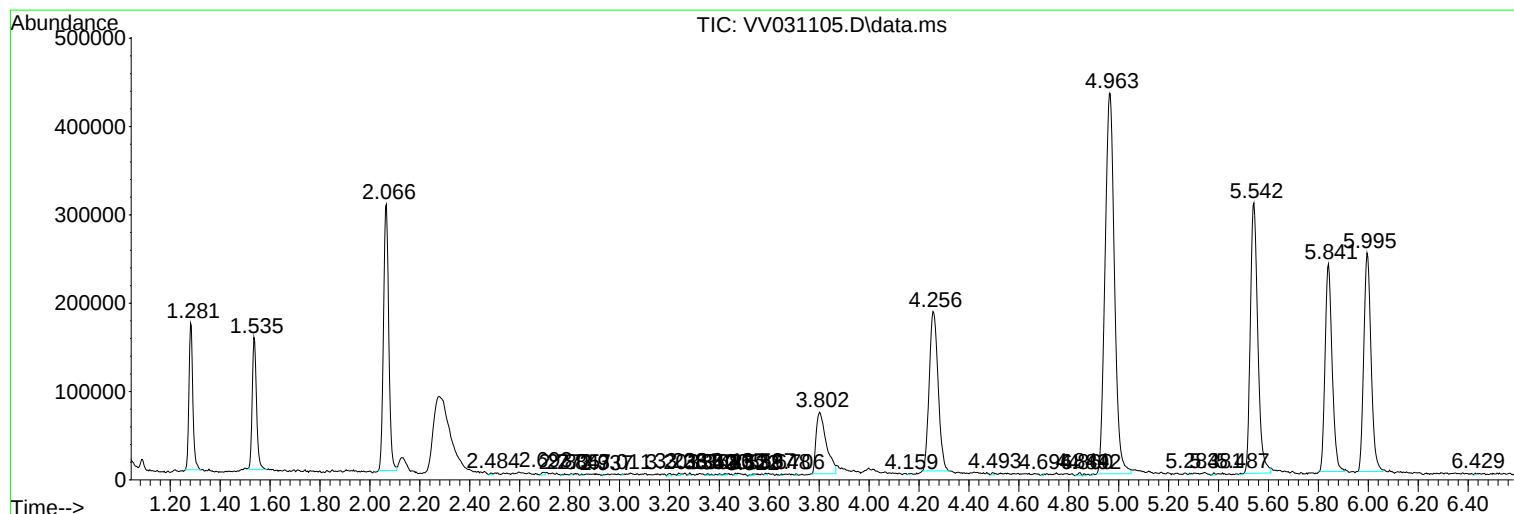

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031105.D
Acq On : 19 May 2023 14:29
Operator : SY/MD
Sample : 02866-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031105.D
Acq On : 19 May 2023 14:29
Operator : SY/MD
Sample : 02866-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------