

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031106.D
 Acq On : 19 May 2023 14:56
 Operator : SY/MD
 Sample : VIBLK211
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rBV	149748	162745	15.20%	2.000%
2	1.539	148	155	170	rVB	126205	161740	15.11%	1.988%
3	2.063	310	318	332	rVB	281834	406375	37.96%	4.995%
4	2.532	460	464	466	rBV5	2266	1905	0.18%	0.023%
5	2.593	481	483	486	rVB4	1577	680	0.06%	0.008%
6	2.658	499	503	504	rBV3	1918	1414	0.13%	0.017%
7	2.973	599	601	603	rBV3	1361	952	0.09%	0.012%
8	3.005	606	611	612	rBV5	1841	1643	0.15%	0.020%
9	3.092	635	638	640	rBV3	1680	1114	0.10%	0.014%
10	3.133	646	651	653	rBV6	1304	1046	0.10%	0.013%
11	3.185	665	667	671	rBV4	1391	962	0.09%	0.012%
12	3.291	696	700	701	rBV4	2078	1070	0.10%	0.013%
13	3.310	701	706	707	rVV5	1805	1186	0.11%	0.015%
14	3.532	771	775	777	rBV4	2207	1627	0.15%	0.020%
15	3.686	821	823	824	rBV2	1595	607	0.06%	0.007%
16	3.805	849	860	891	rBV	66222	207460	19.38%	2.550%
17	4.256	987	1000	1028	rVB	176566	450254	42.05%	5.534%
18	4.503	1071	1077	1078	rBV6	1965	2044	0.19%	0.025%
19	4.963	1204	1220	1245	rBV2	407127	1070657	100.00%	13.160%
20	5.310	1324	1328	1329	rBV4	2263	1405	0.13%	0.017%
21	5.490	1379	1384	1385	rBV5	2300	1656	0.15%	0.020%
22	5.539	1387	1399	1424	rVV	311079	652241	60.92%	8.017%
23	5.995	1530	1541	1563	rVB	239864	482484	45.06%	5.930%
24	6.410	1666	1670	1671	rBV4	1991	1245	0.12%	0.015%
25	6.432	1675	1677	1680	rBV3	1301	942	0.09%	0.012%
26	6.490	1692	1695	1700	rBV6	1838	1265	0.12%	0.016%
27	6.860	1808	1810	1815	rBV6	2168	1237	0.12%	0.015%
28	6.918	1817	1828	1847	rBV2	124127	236159	22.06%	2.903%
29	7.249	1919	1931	1951	rBV	457824	805989	75.28%	9.907%
30	7.558	2018	2027	2045	rBV	89269	158235	14.78%	1.945%
31	7.786	2094	2098	2100	rBV5	2437	1691	0.16%	0.021%
32	7.879	2122	2127	2130	rBV7	2141	2062	0.19%	0.025%
33	8.034	2166	2175	2214	rVV	212315	450135	42.04%	5.533%
34	8.368	2277	2279	2282	rVB4	2148	949	0.09%	0.012%
35	8.452	2303	2305	2308	rVB4	1900	1034	0.10%	0.013%
36	8.474	2308	2312	2316	rVB7	1614	1043	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031106.D
 Acq On : 19 May 2023 14:56
 Operator : SY/MD
 Sample : VIBLK211
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	8.497	2316	2319	2323	rBV5	1844	1796	0.17%	0.022%
38	8.583	2344	2346	2349	rVB4	2036	1005	0.09%	0.012%
39	8.599	2349	2351	2353	rBV2	1519	690	0.06%	0.008%
40	8.622	2353	2358	2362	rVB8	3181	2660	0.25%	0.033%
41	8.661	2366	2370	2373	rBV5	1664	1751	0.16%	0.022%
42	8.792	2399	2411	2433	rBV	449979	769068	71.83%	9.453%
43	9.001	2472	2476	2477	rBV4	2683	1662	0.16%	0.020%
44	9.043	2487	2489	2491	rBV3	1264	661	0.06%	0.008%
45	9.181	2530	2532	2535	rVB3	1753	786	0.07%	0.010%
46	9.198	2535	2537	2540	rBV4	1213	861	0.08%	0.011%
47	9.275	2559	2561	2565	rBV5	1578	560	0.05%	0.007%
48	9.294	2565	2567	2569	rVB4	2219	846	0.08%	0.010%
49	9.378	2590	2593	2598	rVB7	1093	1041	0.10%	0.013%
50	9.397	2598	2599	2604	rVB4	1215	856	0.08%	0.011%
51	9.423	2604	2607	2610	rBV5	1306	1033	0.10%	0.013%
52	9.452	2614	2616	2617	rBV2	1433	636	0.06%	0.008%
53	9.529	2635	2640	2642	rBV5	1728	1615	0.15%	0.020%
54	9.574	2650	2654	2657	rBV5	1367	1126	0.11%	0.014%
55	9.718	2698	2699	2703	rVB3	1537	973	0.09%	0.012%
56	9.789	2719	2721	2726	rVB6	1374	1124	0.10%	0.014%
57	9.812	2726	2728	2729	rBV2	1346	583	0.05%	0.007%
58	9.821	2729	2731	2733	rVV3	2173	1093	0.10%	0.013%
59	9.844	2735	2738	2744	rBV6	2804	3195	0.30%	0.039%
60	9.879	2744	2749	2753	rVV7	2151	2541	0.24%	0.031%
61	9.918	2757	2761	2765	rBV6	1408	1447	0.14%	0.018%
62	9.956	2769	2773	2776	rBV5	1397	1302	0.12%	0.016%
63	10.027	2792	2795	2800	rBV6	2755	1921	0.18%	0.024%
64	10.159	2824	2836	2854	rVV	322449	524452	48.98%	6.446%
65	10.590	2969	2970	2973	rBV3	1384	758	0.07%	0.009%
66	10.622	2976	2980	2982	rBV4	2947	2335	0.22%	0.029%
67	10.725	3008	3012	3014	rBV5	2353	2252	0.21%	0.028%
68	10.754	3019	3021	3023	rBV2	1456	600	0.06%	0.007%
69	10.834	3044	3046	3049	rBV4	1736	847	0.08%	0.010%
70	10.921	3070	3073	3075	rBV3	1356	727	0.07%	0.009%
71	10.943	3078	3080	3082	rBV3	1478	733	0.07%	0.009%
72	11.033	3104	3108	3110	rBV5	1483	1225	0.11%	0.015%
73	11.130	3133	3138	3140	rBV5	2506	2217	0.21%	0.027%
74	11.191	3146	3157	3174	rBV	468527	743712	69.46%	9.141%
75	11.284	3184	3186	3191	rBV6	2085	1591	0.15%	0.020%
76	11.349	3203	3206	3207	rBV3	1681	901	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031106.D
 Acq On : 19 May 2023 14:56
 Operator : SY/MD
 Sample : VIBLK211
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3288	rBV	468974	745079	69.59%	9.158%
78	11.956	3393	3395	3399	rBV5	2139	1370	0.13%	0.017%
79	12.143	3451	3453	3454	rBV3	1637	794	0.07%	0.010%
80	12.223	3475	3478	3480	rBV4	1806	1053	0.10%	0.013%
81	12.268	3490	3492	3494	rBV3	1670	818	0.08%	0.010%
82	12.323	3503	3509	3513	rBV7	2110	2665	0.25%	0.033%
83	12.390	3528	3530	3534	rBV5	1245	1006	0.09%	0.012%
84	12.458	3548	3551	3554	rBV5	2863	1759	0.16%	0.022%
85	12.484	3556	3559	3563	rVV6	2297	1344	0.13%	0.017%
86	12.657	3609	3613	3617	rBV7	2853	2843	0.27%	0.035%
87	12.792	3653	3655	3659	rBV5	1725	1288	0.12%	0.016%
88	12.895	3683	3687	3691	rBV6	1963	2046	0.19%	0.025%
89	12.943	3699	3702	3705	rBV4	1775	934	0.09%	0.011%
90	12.959	3705	3707	3711	rBV6	1566	1195	0.11%	0.015%
91	13.027	3725	3728	3730	rBV4	1865	1127	0.11%	0.014%
92	13.059	3736	3738	3739	rBV2	1445	693	0.06%	0.009%
93	13.172	3771	3773	3775	rVB3	1513	665	0.06%	0.008%
94	13.188	3775	3778	3779	rBV3	2101	1045	0.10%	0.013%
95	13.348	3826	3828	3832	rBV5	1710	1360	0.13%	0.017%
96	13.422	3849	3851	3855	rBV5	1771	1018	0.10%	0.013%
97	13.676	3928	3930	3931	rBV2	1962	818	0.08%	0.010%
98	13.805	3966	3970	3972	rVB4	2602	1433	0.13%	0.018%
99	14.043	4039	4044	4045	rBV5	2793	2412	0.23%	0.030%
100	14.844	4291	4293	4295	rBV3	1605	685	0.06%	0.008%




Sum of corrected areas: 8135885

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031106.D
Acq On : 19 May 2023 14:56
Operator : SY/MD
Sample : VIBLK211
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

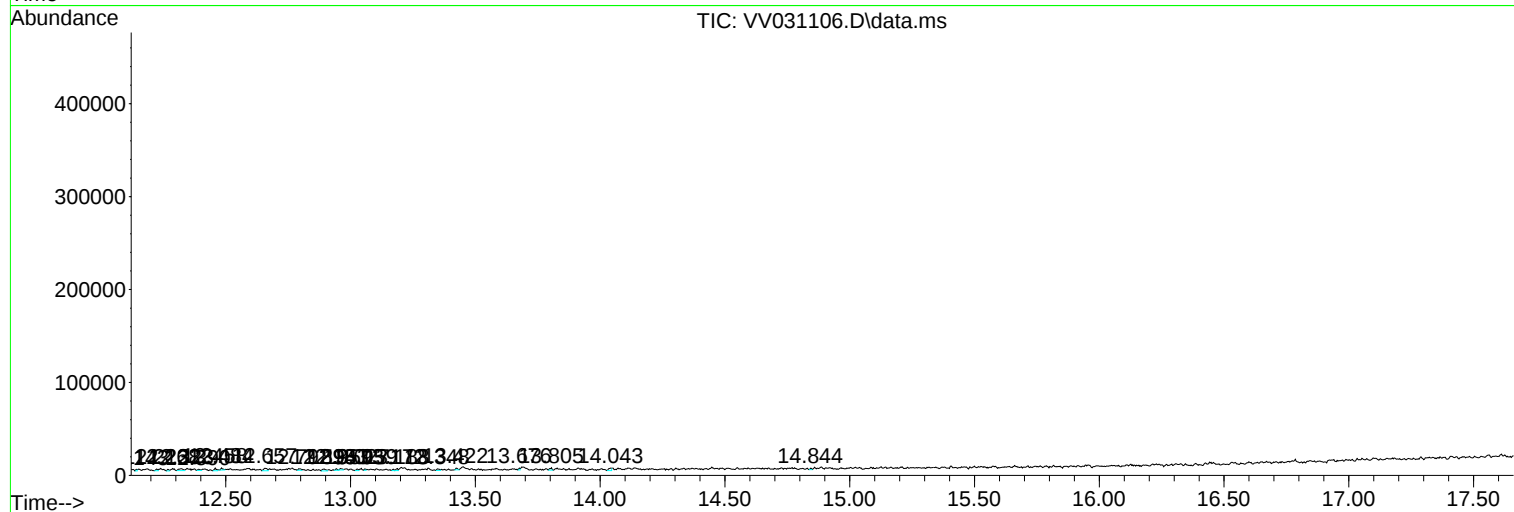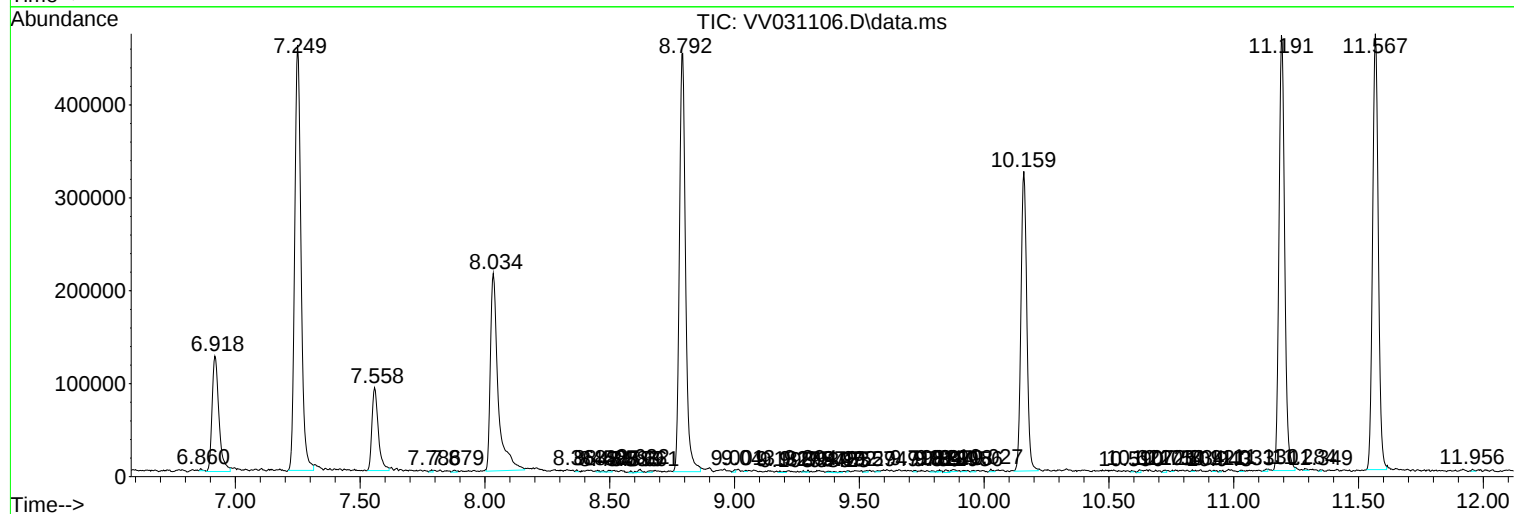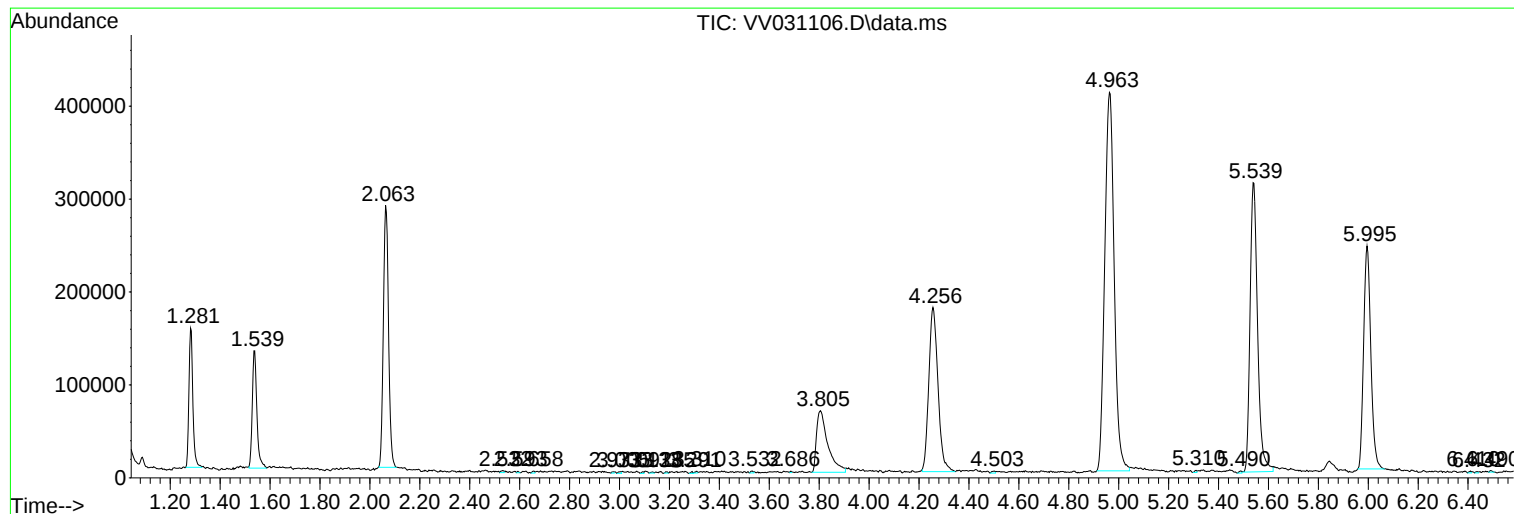

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031106.D
Acq On : 19 May 2023 14:56
Operator : SY/MD
Sample : VIBLK211
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031106.D
Acq On : 19 May 2023 14:56
Operator : SY/MD
Sample : VIBLK211
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------