

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031108.D
 Acq On : 19 May 2023 15:45
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	154576	169841	16.28%	2.038%
2	1.536	148	154	170	rVB	142410	167530	16.06%	2.010%
3	2.063	309	318	331	rBV	284720	411319	39.43%	4.935%
4	2.497	449	453	454	rBV3	1733	1014	0.10%	0.012%
5	2.609	485	488	491	rBV5	1339	1049	0.10%	0.013%
6	2.706	516	518	523	rBV5	1435	881	0.08%	0.011%
7	2.728	523	525	527	rVB3	2320	940	0.09%	0.011%
8	2.928	585	587	590	rBV5	1714	1035	0.10%	0.012%
9	2.992	604	607	613	rVB7	2243	2047	0.20%	0.025%
10	3.034	613	620	624	rBV9	2364	2966	0.28%	0.036%
11	3.105	638	642	646	rBV6	2018	2095	0.20%	0.025%
12	3.201	667	672	674	rBV6	1650	1617	0.16%	0.019%
13	3.240	681	684	688	rBV6	1616	1428	0.14%	0.017%
14	3.278	694	696	699	rBV4	1429	988	0.09%	0.012%
15	3.330	708	712	714	rBV5	1864	1491	0.14%	0.018%
16	3.397	729	733	737	rBV7	1800	1910	0.18%	0.023%
17	3.696	822	826	828	rBV5	962	704	0.07%	0.008%
18	3.802	850	859	885	rVV	66033	189423	18.16%	2.273%
19	4.124	955	959	962	rBV6	2686	2111	0.20%	0.025%
20	4.195	979	981	982	rBV2	2169	955	0.09%	0.011%
21	4.259	988	1001	1022	rVB	182584	434607	41.67%	5.214%
22	4.580	1098	1101	1102	rBV3	1760	954	0.09%	0.011%
23	4.690	1132	1135	1137	rBV4	1424	949	0.09%	0.011%
24	4.725	1144	1146	1149	rBV4	1392	872	0.08%	0.010%
25	4.783	1162	1164	1168	rVB5	1771	986	0.09%	0.012%
26	4.806	1168	1171	1174	rBV4	1963	1743	0.17%	0.021%
27	4.963	1204	1220	1246	rBV3	397835	1043090	100.00%	12.514%
28	5.259	1310	1312	1314	rBV2	2357	1392	0.13%	0.017%
29	5.542	1388	1400	1424	rBV	319468	663325	63.59%	7.958%
30	5.841	1482	1493	1512	rBV	141825	282881	27.12%	3.394%
31	5.995	1530	1541	1561	rVB	238043	471565	45.21%	5.657%
32	6.436	1675	1678	1681	rBV3	1988	1348	0.13%	0.016%
33	6.468	1687	1688	1691	rBV3	1314	875	0.08%	0.010%
34	6.728	1766	1769	1772	rBV4	1572	811	0.08%	0.010%
35	6.744	1772	1774	1776	rBV3	1689	846	0.08%	0.010%
36	6.876	1811	1815	1817	rBV5	2044	1393	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031108.D
 Acq On : 19 May 2023 15:45
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.918	1819	1828	1842	rVV	116342	212405	20.36%	2.548%
38	7.249	1920	1931	1952	rBV	447430	785735	75.33%	9.427%
39	7.558	2018	2027	2049	rBV2	86263	157427	15.09%	1.889%
40	7.767	2090	2092	2094	rBV3	1747	729	0.07%	0.009%
41	7.812	2104	2106	2111	rBV6	1447	1073	0.10%	0.013%
42	7.844	2113	2116	2117	rBV3	1660	905	0.09%	0.011%
43	8.034	2165	2175	2207	rBV	222871	459858	44.09%	5.517%
44	8.233	2235	2237	2241	rBV4	2015	1696	0.16%	0.020%
45	8.339	2268	2270	2272	rBV3	2118	847	0.08%	0.010%
46	8.561	2337	2339	2341	rBV3	1565	967	0.09%	0.012%
47	8.748	2393	2397	2398	rBV4	1376	884	0.08%	0.011%
48	8.789	2400	2410	2430	rVV	480110	800185	76.71%	9.600%
49	9.127	2513	2515	2517	rBV3	1487	770	0.07%	0.009%
50	9.243	2549	2551	2552	rBV2	2151	795	0.08%	0.010%
51	9.471	2617	2622	2624	rBV6	2293	1926	0.18%	0.023%
52	9.638	2670	2674	2677	rBV6	1597	1226	0.12%	0.015%
53	9.677	2684	2686	2689	rVB4	2093	892	0.09%	0.011%
54	9.735	2702	2704	2708	rVB5	1411	891	0.09%	0.011%
55	9.831	2732	2734	2737	rBV4	1544	730	0.07%	0.009%
56	9.921	2759	2762	2764	rBV4	1544	1118	0.11%	0.013%
57	10.159	2825	2836	2859	rVB	317042	503351	48.26%	6.039%
58	10.381	2903	2905	2906	rBV2	2459	1129	0.11%	0.014%
59	10.468	2928	2932	2934	rBV5	2853	2595	0.25%	0.031%
60	10.564	2959	2962	2967	rVB7	2549	1632	0.16%	0.020%
61	10.603	2970	2974	2975	rBV4	1144	832	0.08%	0.010%
62	11.191	3146	3157	3179	rBV	476770	750260	71.93%	9.001%
63	11.310	3191	3194	3196	rBV4	2121	1554	0.15%	0.019%
64	11.345	3203	3205	3208	rBV4	1542	878	0.08%	0.011%
65	11.567	3263	3274	3288	rBV	459230	719360	68.96%	8.630%
66	11.831	3354	3356	3359	rVB3	1683	717	0.07%	0.009%
67	11.944	3389	3391	3395	rBV5	1380	1101	0.11%	0.013%
68	12.172	3460	3462	3464	rBV3	1762	1006	0.10%	0.012%
69	12.452	3545	3549	3552	rBV5	2046	1916	0.18%	0.023%
70	12.477	3553	3557	3563	rVV8	2059	2610	0.25%	0.031%
71	12.583	3586	3590	3591	rBV3	1649	1151	0.11%	0.014%
72	12.628	3601	3604	3609	rBV7	1639	1256	0.12%	0.015%
73	12.683	3619	3621	3624	rBV4	1674	832	0.08%	0.010%
74	12.747	3639	3641	3646	rVB6	1933	1095	0.10%	0.013%
75	12.783	3649	3652	3659	rVB7	2211	2118	0.20%	0.025%
76	12.818	3659	3663	3666	rBV6	1840	1342	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031108.D
 Acq On : 19 May 2023 15:45
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.898	3682	3688	3690	rBV7	1731	1829	0.18%	0.022%
78	12.943	3699	3702	3706	rBV6	2005	1592	0.15%	0.019%
79	12.995	3716	3718	3724	rBV7	1900	1947	0.19%	0.023%
80	13.027	3724	3728	3730	rBV4	2246	1880	0.18%	0.023%
81	13.207	3779	3784	3788	rBV7	2079	2761	0.26%	0.033%
82	13.246	3794	3796	3799	rBV4	1548	803	0.08%	0.010%
83	13.297	3810	3812	3816	rBV5	1784	802	0.08%	0.010%
84	13.442	3853	3857	3858	rBV4	2194	1417	0.14%	0.017%
85	13.525	3880	3883	3888	rBV7	2103	1657	0.16%	0.020%
86	13.603	3904	3907	3910	rVB4	1170	718	0.07%	0.009%
87	13.628	3910	3915	3917	rBV6	2271	2048	0.20%	0.025%
88	13.664	3921	3926	3927	rBV5	2442	1790	0.17%	0.021%
89	13.776	3958	3961	3963	rBV4	1053	825	0.08%	0.010%
90	13.937	4009	4011	4015	rBV4	1574	1163	0.11%	0.014%
91	14.082	4049	4056	4057	rBV7	1975	1603	0.15%	0.019%
92	14.214	4094	4097	4098	rBV3	1846	886	0.08%	0.011%
93	14.316	4126	4129	4133	rVB5	1640	1401	0.13%	0.017%
94	14.342	4133	4137	4144	rBV9	2460	3109	0.30%	0.037%
95	14.384	4146	4150	4154	rBV6	2103	2457	0.24%	0.029%
96	14.487	4178	4182	4186	rBV7	2359	1831	0.18%	0.022%
97	14.689	4242	4245	4249	rBV5	2183	2287	0.22%	0.027%
98	14.760	4265	4267	4270	rBV4	2235	1366	0.13%	0.016%
99	14.847	4290	4294	4295	rBV4	1763	1180	0.11%	0.014%
100	15.384	4458	4461	4462	rBV3	1859	1141	0.11%	0.014%


Sum of corrected areas: 8335268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031108.D
Acq On : 19 May 2023 15:45
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

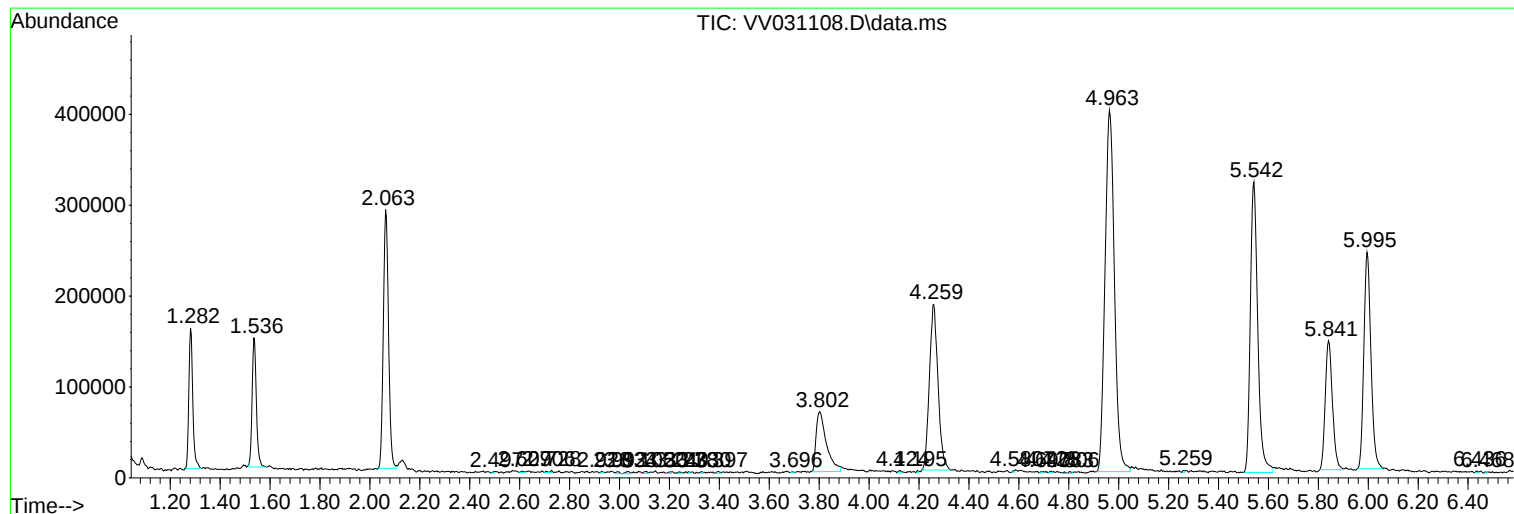

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031108.D
Acq On : 19 May 2023 15:45
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031108.D
Acq On : 19 May 2023 15:45
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc