

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031112.D
 Acq On : 19 May 2023 17:22
 Operator : SY/MD
 Sample : 02866-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	145317	157393	1.84%	0.954%
2	1.535	148	154	180	rVB	177965	234818	2.75%	1.423%
3	2.063	309	318	335	rBV	283060	414454	4.85%	2.511%
4	2.423	428	430	432	rVB2	2221	694	0.01%	0.004%
5	2.812	548	551	553	rBV4	1263	866	0.01%	0.005%
6	2.940	589	591	594	rVB4	1724	1048	0.01%	0.006%
7	2.960	594	597	598	rBV3	1333	642	0.01%	0.004%
8	3.098	637	640	642	rBV3	1299	801	0.01%	0.005%
9	3.194	668	670	671	rBV	1408	576	0.01%	0.003%
10	3.214	674	676	679	rBV4	1067	655	0.01%	0.004%
11	3.294	698	701	702	rBV3	1037	500	0.01%	0.003%
12	3.468	752	755	756	rBV3	1155	644	0.01%	0.004%
13	3.519	768	771	774	rBV5	1845	1481	0.02%	0.009%
14	3.561	782	784	785	rBV2	1831	930	0.01%	0.006%
15	3.603	795	797	800	rBV4	1374	704	0.01%	0.004%
16	3.619	800	802	803	rBV2	1189	599	0.01%	0.004%
17	3.664	813	816	818	rBV5	1050	710	0.01%	0.004%
18	3.722	831	834	835	rBV3	1288	648	0.01%	0.004%
19	3.812	849	862	888	rBV3	88173	303208	3.55%	1.837%
20	4.259	986	1001	1022	rBV	172558	438596	5.13%	2.658%
21	4.757	1155	1156	1157	rBV	1345	399	0.00%	0.002%
22	4.828	1175	1178	1180	rBV3	2281	1184	0.01%	0.007%
23	4.963	1204	1220	1241	rBV2	394239	1035563	12.11%	6.275%
24	5.542	1387	1400	1423	rBV	307707	646429	7.56%	3.917%
25	5.837	1478	1492	1523	rBV	4522385	8548271	100.00%	51.796%
26	5.995	1533	1541	1562	rVB	238767	480114	5.62%	2.909%
27	6.844	1800	1805	1807	rBV5	3004	2572	0.03%	0.016%
28	6.918	1818	1828	1850	rBV	115818	221374	2.59%	1.341%
29	7.249	1920	1931	1953	rBV	433863	774019	9.05%	4.690%
30	7.558	2019	2027	2042	rBV	84281	149549	1.75%	0.906%
31	8.034	2166	2175	2209	rBV	213206	433038	5.07%	2.624%
32	8.407	2287	2291	2292	rBV4	1819	1220	0.01%	0.007%
33	8.497	2314	2319	2321	rBV6	2192	1821	0.02%	0.011%
34	8.587	2345	2347	2351	rBV5	1888	1212	0.01%	0.007%
35	8.792	2400	2411	2432	rBV	469860	779948	9.12%	4.726%
36	9.705	2693	2695	2698	rBV4	1654	878	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031112.D
 Acq On : 19 May 2023 17:22
 Operator : SY/MD
 Sample : 02866-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.869	2743	2746	2748	rBV4	1557	848	0.01%	0.005%
38	9.908	2756	2758	2764	rVB6	2257	1596	0.02%	0.010%
39	9.937	2764	2767	2768	rBV3	1459	961	0.01%	0.006%
40	9.982	2778	2781	2784	rBV5	1553	1117	0.01%	0.007%
41	10.159	2819	2836	2854	rBV	296520	477748	5.59%	2.895%
42	10.294	2877	2878	2881	rBV3	1402	823	0.01%	0.005%
43	10.371	2899	2902	2904	rBV4	1552	991	0.01%	0.006%
44	10.413	2912	2915	2916	rBV3	1111	524	0.01%	0.003%
45	10.442	2922	2924	2926	rBV3	892	506	0.01%	0.003%
46	10.522	2943	2949	2950	rBV5	2354	1696	0.02%	0.010%
47	10.635	2982	2984	2987	rBV4	1206	860	0.01%	0.005%
48	10.680	2996	2998	3000	rBV3	1315	559	0.01%	0.003%
49	10.696	3001	3003	3005	rVB2	1389	498	0.01%	0.003%
50	10.728	3010	3013	3017	rBV4	1445	1191	0.01%	0.007%
51	10.747	3017	3019	3021	rBV3	1124	491	0.01%	0.003%
52	10.853	3050	3052	3057	rVB6	1487	886	0.01%	0.005%
53	10.905	3064	3068	3070	rBV5	2333	1326	0.02%	0.008%
54	11.059	3112	3116	3118	rBV5	1853	976	0.01%	0.006%
55	11.075	3118	3121	3125	rBV5	1730	1368	0.02%	0.008%
56	11.127	3134	3137	3140	rBV4	2230	1540	0.02%	0.009%
57	11.191	3147	3157	3176	rBV	418290	662352	7.75%	4.013%
58	11.458	3238	3240	3242	rBV3	1171	700	0.01%	0.004%
59	11.567	3263	3274	3292	rVB	420686	665401	7.78%	4.032%
60	11.699	3313	3315	3318	rBV4	1811	910	0.01%	0.006%
61	11.844	3357	3360	3363	rBV5	1534	1166	0.01%	0.007%
62	11.969	3396	3399	3405	rVB8	2482	2377	0.03%	0.014%
63	12.001	3405	3409	3412	rBV5	2895	2427	0.03%	0.015%
64	12.117	3442	3445	3446	rBV3	672	330	0.00%	0.002%
65	12.149	3452	3455	3457	rBV4	1476	796	0.01%	0.005%
66	12.204	3468	3472	3476	rBV7	1484	1568	0.02%	0.010%
67	12.226	3476	3479	3481	rVB3	1133	691	0.01%	0.004%
68	12.242	3481	3484	3485	rBV3	1625	802	0.01%	0.005%
69	12.252	3485	3487	3489	rVB3	1192	569	0.01%	0.003%
70	12.265	3489	3491	3493	rBV3	1406	628	0.01%	0.004%
71	12.281	3494	3496	3499	rBV4	861	558	0.01%	0.003%
72	12.329	3508	3511	3514	rBV5	1478	1164	0.01%	0.007%
73	12.413	3534	3537	3540	rBV5	1241	1003	0.01%	0.006%
74	12.438	3540	3545	3546	rVB5	1544	1125	0.01%	0.007%
75	12.467	3551	3554	3557	rBV4	1514	960	0.01%	0.006%
76	12.496	3560	3563	3564	rBV3	1709	1040	0.01%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031112.D
 Acq On : 19 May 2023 17:22
 Operator : SY/MD
 Sample : 02866-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.545	3577	3578	3581	rVV3	1666	813	0.01%	0.005%
78	12.557	3581	3582	3584	rVB2	1655	417	0.00%	0.003%
79	12.586	3587	3591	3593	rBV5	2045	1473	0.02%	0.009%
80	12.599	3593	3595	3600	rVB6	1711	1044	0.01%	0.006%
81	12.628	3602	3604	3606	rBV2	1059	566	0.01%	0.003%
82	12.673	3617	3618	3621	rVB3	1224	454	0.01%	0.003%
83	12.705	3627	3628	3630	rBV2	1000	484	0.01%	0.003%
84	12.734	3636	3637	3638	rBV	1132	339	0.00%	0.002%
85	12.757	3642	3644	3646	rVB3	1614	655	0.01%	0.004%
86	12.795	3654	3656	3660	rVB4	1648	1087	0.01%	0.007%
87	12.828	3663	3666	3667	rBV3	1233	747	0.01%	0.005%
88	12.834	3667	3668	3670	rBV	1480	460	0.01%	0.003%
89	12.863	3675	3677	3679	rBV3	645	386	0.00%	0.002%
90	12.930	3696	3698	3700	rBV4	1251	566	0.01%	0.003%
91	12.953	3703	3705	3707	rBV3	1327	852	0.01%	0.005%
92	13.024	3725	3727	3728	rBV2	1659	756	0.01%	0.005%
93	13.056	3735	3737	3740	rVB4	1713	946	0.01%	0.006%
94	13.201	3780	3782	3787	rBV6	2845	2182	0.03%	0.013%
95	13.303	3812	3814	3816	rBV3	1942	1037	0.01%	0.006%
96	13.342	3824	3826	3828	rBV3	1224	503	0.01%	0.003%
97	13.416	3847	3849	3852	rBV4	1757	1012	0.01%	0.006%
98	13.795	3964	3967	3968	rBV3	2080	1169	0.01%	0.007%
99	14.708	4249	4251	4253	rBV3	2690	1603	0.02%	0.010%
100	14.927	4314	4319	4322	rBV7	2835	3430	0.04%	0.021%




Sum of corrected areas: 16503611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031112.D
Acq On : 19 May 2023 17:22
Operator : SY/MD
Sample : 02866-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

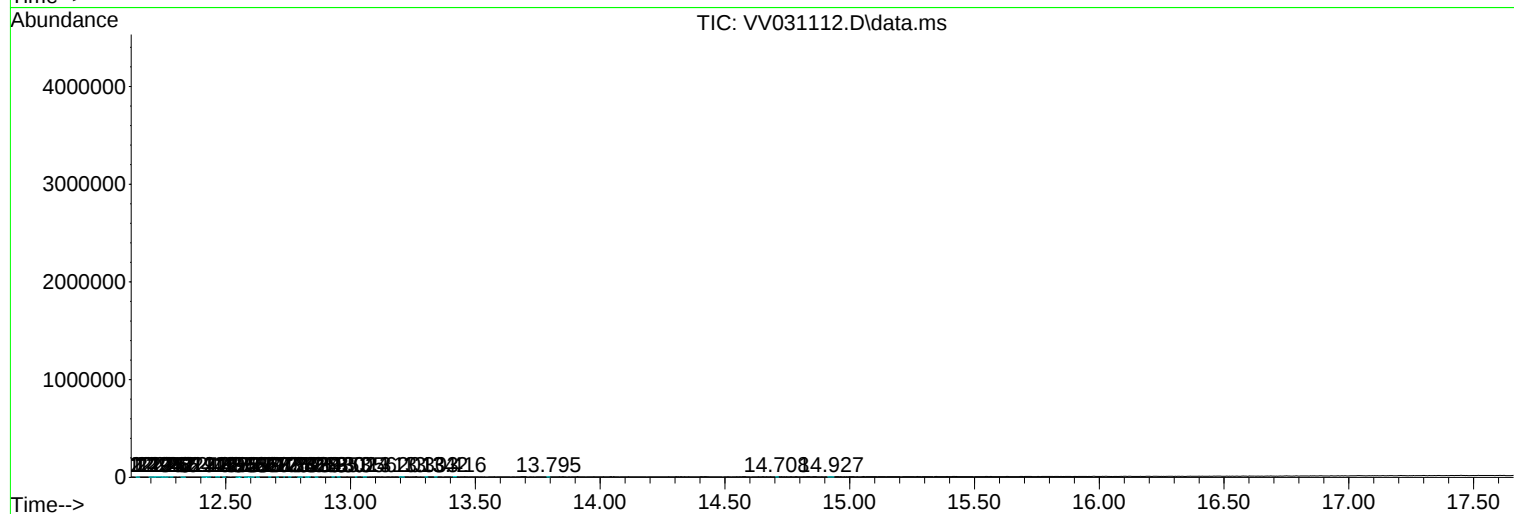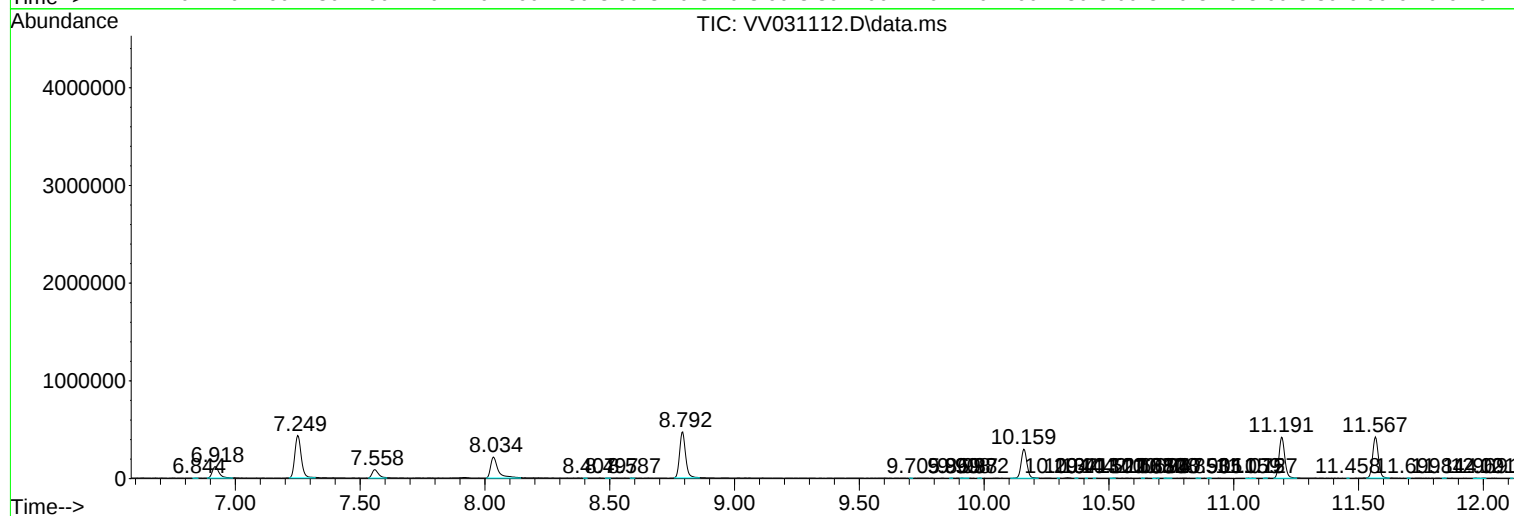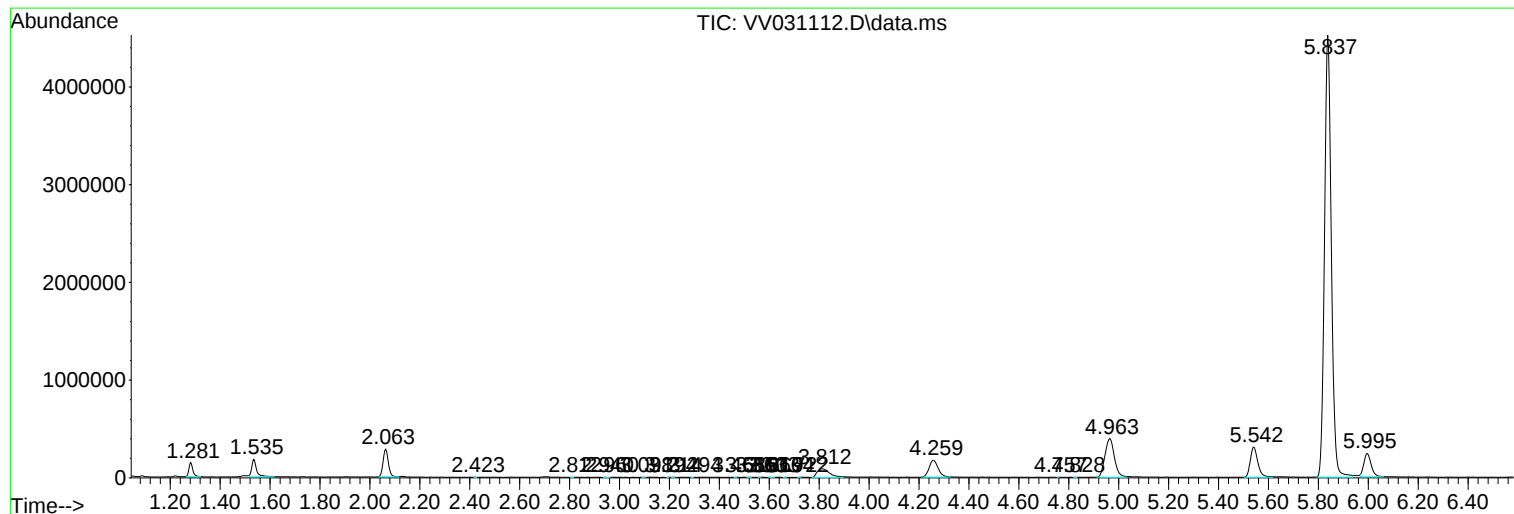

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031112.D
Acq On : 19 May 2023 17:22
Operator : SY/MD
Sample : 02866-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031112.D
Acq On : 19 May 2023 17:22
Operator : SY/MD
Sample : 02866-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------