

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031113.D
 Acq On : 19 May 2023 17:46
 Operator : SY/MD
 Sample : 02866-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rVB	152757	162001	6.58%	1.528%
2	1.536	148	154	170	rVB	166822	200997	8.16%	1.896%
3	2.063	310	318	330	rVB	282447	405528	16.47%	3.825%
4	2.327	398	400	402	rBV2	1751	759	0.03%	0.007%
5	2.429	430	432	434	rBV3	1798	1087	0.04%	0.010%
6	2.516	455	459	461	rBV4	1746	1363	0.06%	0.013%
7	2.822	551	554	556	rBV4	1777	1357	0.06%	0.013%
8	2.918	582	584	588	rBV5	1696	1104	0.04%	0.010%
9	2.953	593	595	598	rBV4	1904	1269	0.05%	0.012%
10	2.986	602	605	606	rBV3	1439	811	0.03%	0.008%
11	3.233	680	682	685	rBV4	1989	1164	0.05%	0.011%
12	3.253	685	688	690	rBV4	1728	1217	0.05%	0.011%
13	3.346	713	717	718	rBV3	1793	1275	0.05%	0.012%
14	3.371	723	725	729	rBV5	2431	1939	0.08%	0.018%
15	3.410	734	737	738	rBV3	2766	1467	0.06%	0.014%
16	3.497	762	764	765	rVB2	1965	650	0.03%	0.006%
17	3.545	777	779	781	rBV2	1388	656	0.03%	0.006%
18	3.687	821	823	824	rBV2	825	335	0.01%	0.003%
19	3.757	841	845	848	rBV6	1653	1455	0.06%	0.014%
20	3.815	849	863	889	rVV2	99462	341484	13.87%	3.221%
21	4.101	950	952	954	rBV3	1726	882	0.04%	0.008%
22	4.140	962	964	966	rVB3	2573	1026	0.04%	0.010%
23	4.256	986	1000	1024	rBV	176292	444890	18.07%	4.197%
24	4.806	1168	1171	1172	rBV3	1531	927	0.04%	0.009%
25	4.896	1195	1199	1201	rBV5	1984	1649	0.07%	0.016%
26	4.963	1205	1220	1248	rVV2	395354	1058721	43.00%	9.987%
27	5.281	1317	1319	1323	rVB6	2235	1231	0.05%	0.012%
28	5.474	1376	1379	1380	rBV3	2177	1070	0.04%	0.010%
29	5.542	1386	1400	1424	rBV	313131	658826	26.76%	6.215%
30	5.838	1479	1492	1517	rBV	1255256	2461996	100.00%	23.225%
31	5.995	1531	1541	1561	rVB	240608	488803	19.85%	4.611%
32	6.567	1717	1719	1721	rBV3	1605	835	0.03%	0.008%
33	6.696	1757	1759	1764	rBV5	2440	2323	0.09%	0.022%
34	6.918	1813	1828	1846	rBV	121802	233220	9.47%	2.200%
35	7.063	1869	1873	1875	rBV5	2534	1839	0.07%	0.017%
36	7.249	1920	1931	1950	rBV	447350	793834	32.24%	7.489%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031113.D
 Acq On : 19 May 2023 17:46
 Operator : SY/MD
 Sample : 02866-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.558	2019	2027	2042	rBV	87545	147917	6.01%	1.395%
38	8.034	2166	2175	2202	rBV	213460	429522	17.45%	4.052%
39	8.567	2340	2341	2343	rBV2	1560	713	0.03%	0.007%
40	8.792	2400	2411	2438	rBV	474453	793579	32.23%	7.486%
41	9.265	2554	2558	2561	rBV6	2089	1653	0.07%	0.016%
42	9.358	2585	2587	2588	rBV2	1241	416	0.02%	0.004%
43	9.391	2595	2597	2600	rBV4	1692	993	0.04%	0.009%
44	9.535	2640	2642	2644	rBV3	1766	1040	0.04%	0.010%
45	9.680	2682	2687	2690	rBV7	2412	2206	0.09%	0.021%
46	9.889	2750	2752	2755	rBV4	1797	984	0.04%	0.009%
47	9.934	2763	2766	2768	rBV3	1842	927	0.04%	0.009%
48	10.114	2820	2822	2824	rBV3	2027	1160	0.05%	0.011%
49	10.159	2825	2836	2854	rVV	322007	510182	20.72%	4.813%
50	10.513	2943	2946	2947	rBV3	1813	1045	0.04%	0.010%
51	10.667	2993	2994	2995	rBV	1096	227	0.01%	0.002%
52	10.931	3073	3076	3078	rBV4	1539	1096	0.04%	0.010%
53	10.950	3078	3082	3085	rVV5	1580	1677	0.07%	0.016%
54	10.985	3089	3093	3095	rBV5	2053	1353	0.05%	0.013%
55	11.098	3123	3128	3131	rBV7	2630	2818	0.11%	0.027%
56	11.191	3147	3157	3178	rVB	428544	687033	27.91%	6.481%
57	11.426	3228	3230	3235	rBV5	2125	1801	0.07%	0.017%
58	11.567	3264	3274	3290	rVB	435217	692316	28.12%	6.531%
59	11.747	3328	3330	3332	rBV2	1862	694	0.03%	0.007%
60	11.831	3354	3356	3358	rBV3	2190	1042	0.04%	0.010%
61	12.406	3532	3535	3538	rBV4	1474	958	0.04%	0.009%
62	12.423	3538	3540	3541	rBV2	1128	584	0.02%	0.006%
63	12.461	3549	3552	3555	rBV6	1304	878	0.04%	0.008%
64	12.493	3559	3562	3563	rBV3	1595	790	0.03%	0.007%
65	12.632	3603	3605	3610	rVB5	2152	1378	0.06%	0.013%
66	12.657	3610	3613	3615	rBV4	1807	866	0.04%	0.008%
67	12.673	3615	3618	3619	rBV3	1721	882	0.04%	0.008%
68	12.715	3628	3631	3632	rBV3	975	443	0.02%	0.004%
69	12.738	3637	3638	3640	rBV2	1521	708	0.03%	0.007%
70	12.751	3640	3642	3643	rBV2	1292	355	0.01%	0.003%
71	12.779	3648	3651	3652	rBV3	1091	454	0.02%	0.004%
72	12.799	3652	3657	3659	rBV6	1712	1569	0.06%	0.015%
73	12.898	3684	3688	3689	rBV4	1390	820	0.03%	0.008%
74	12.943	3699	3702	3703	rBV3	1227	762	0.03%	0.007%
75	12.956	3704	3706	3716	rVB3	2762	2563	0.10%	0.024%
76	12.998	3716	3719	3724	rBV6	2396	2249	0.09%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031113.D
 Acq On : 19 May 2023 17:46
 Operator : SY/MD
 Sample : 02866-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	13.021	3724	3726	3728	rBV3	719	392	0.02%	0.004%
78	13.098	3748	3750	3753	rVB4	1193	758	0.03%	0.007%
79	13.178	3773	3775	3779	rBV5	1344	894	0.04%	0.008%
80	13.204	3779	3783	3784	rBV4	1169	727	0.03%	0.007%
81	13.262	3798	3801	3803	rBV3	1746	838	0.03%	0.008%
82	13.310	3812	3816	3817	rBV3	1064	633	0.03%	0.006%
83	13.323	3818	3820	3822	rVV3	1263	624	0.03%	0.006%
84	13.342	3825	3826	3827	rBV	821	241	0.01%	0.002%
85	13.355	3827	3830	3836	rVB6	2591	1945	0.08%	0.018%
86	13.400	3842	3844	3845	rVB2	873	287	0.01%	0.003%
87	13.413	3845	3848	3850	rBV4	1486	1074	0.04%	0.010%
88	13.577	3896	3899	3902	rBV5	1909	1321	0.05%	0.012%
89	13.619	3910	3912	3915	rBV4	1074	446	0.02%	0.004%
90	13.635	3915	3917	3923	rVB6	1865	1225	0.05%	0.012%
91	13.664	3923	3926	3929	rBV4	1257	1119	0.05%	0.011%
92	13.689	3932	3934	3938	rVB5	1814	1205	0.05%	0.011%
93	13.770	3957	3959	3961	rBV3	1323	598	0.02%	0.006%
94	13.789	3964	3965	3966	rBV	1691	451	0.02%	0.004%
95	13.882	3992	3994	3996	rBV2	2197	1183	0.05%	0.011%
96	14.027	4036	4039	4041	rBV4	1596	954	0.04%	0.009%
97	14.374	4145	4147	4148	rBV2	1706	868	0.04%	0.008%
98	14.403	4154	4156	4160	rBV4	2022	1105	0.04%	0.010%
99	14.422	4160	4162	4166	rBV5	1915	1593	0.06%	0.015%
100	14.709	4250	4251	4255	rVB4	2708	1563	0.06%	0.015%




Sum of corrected areas: 10600687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031113.D
Acq On : 19 May 2023 17:46
Operator : SY/MD
Sample : 02866-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

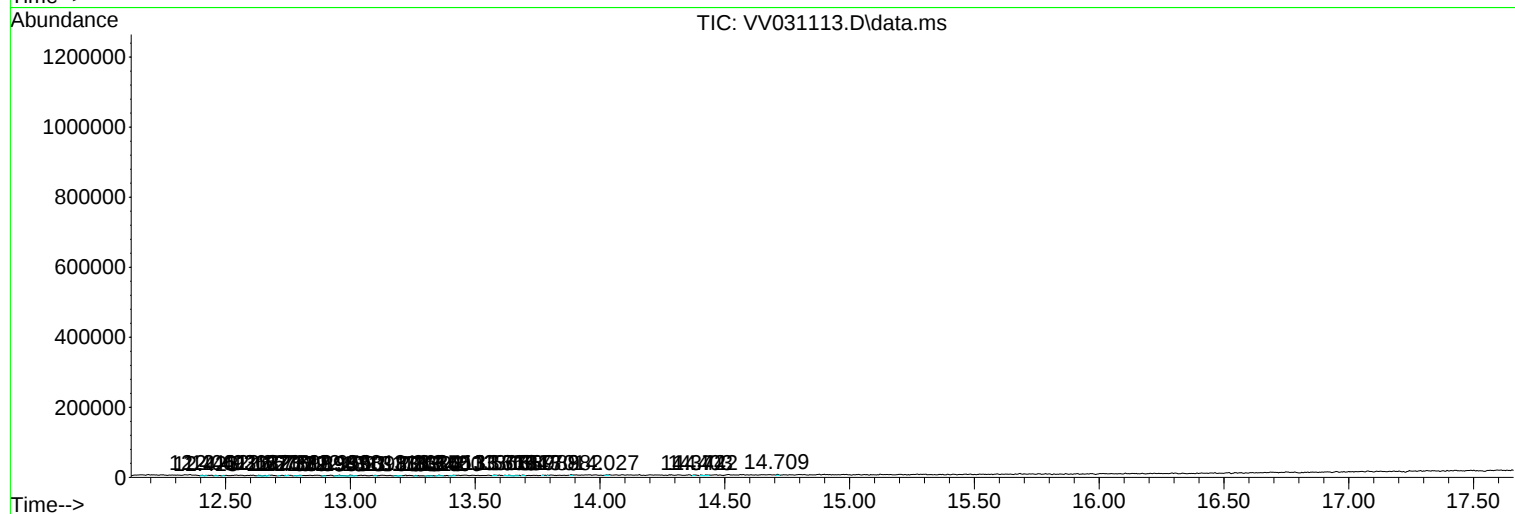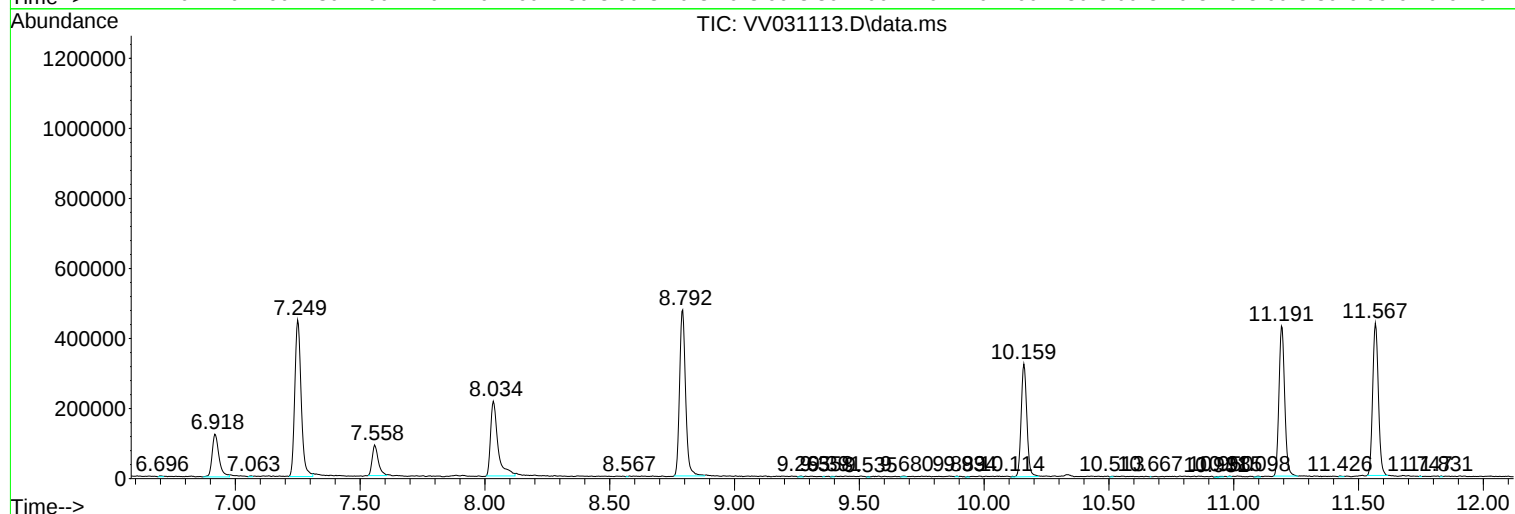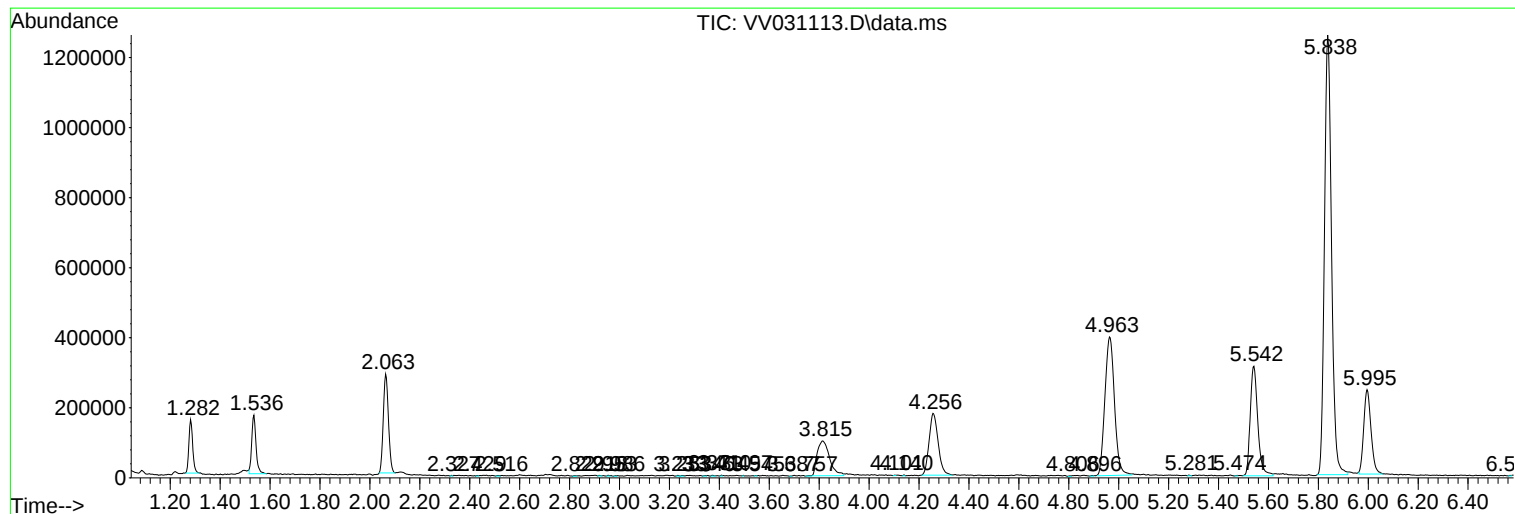

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031113.D
Acq On : 19 May 2023 17:46
Operator : SY/MD
Sample : 02866-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031113.D
Acq On : 19 May 2023 17:46
Operator : SY/MD
Sample : 02866-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc