

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031114.D
 Acq On : 19 May 2023 18:11
 Operator : SY/MD
 Sample : 02866-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rVB	146940	155427	6.24%	1.509%
2	1.536	148	154	170	rVB	155975	190350	7.64%	1.848%
3	2.063	309	318	332	rBV	282232	414190	16.62%	4.022%
4	2.301	390	392	396	rVB5	2895	1450	0.06%	0.014%
5	2.336	400	403	404	rBV2	2575	1473	0.06%	0.014%
6	2.372	412	414	415	rBV2	1228	463	0.02%	0.004%
7	2.671	505	507	508	rBV2	1725	901	0.04%	0.009%
8	3.233	680	682	685	rBV4	1726	1254	0.05%	0.012%
9	3.282	693	697	700	rBV5	2331	2060	0.08%	0.020%
10	3.343	713	716	718	rBV4	1679	1269	0.05%	0.012%
11	3.474	753	757	759	rBV5	2238	1760	0.07%	0.017%
12	3.571	785	787	789	rBV2	1451	601	0.02%	0.006%
13	3.609	797	799	801	rBV3	1334	795	0.03%	0.008%
14	3.818	849	864	886	rBV3	92563	318075	12.76%	3.089%
15	4.114	952	956	960	rBV7	2080	1927	0.08%	0.019%
16	4.256	988	1000	1023	rVB	167957	422308	16.94%	4.101%
17	4.873	1190	1192	1194	rBV3	1141	313	0.01%	0.003%
18	4.963	1204	1220	1252	rBV2	386797	1041657	41.79%	10.115%
19	5.542	1388	1400	1422	rBV	313662	641268	25.73%	6.227%
20	5.838	1479	1492	1520	rBV	1259751	2492432	100.00%	24.202%
21	5.995	1531	1541	1562	rVB	234913	471318	18.91%	4.577%
22	6.918	1819	1828	1850	rBV	116957	218795	8.78%	2.125%
23	7.249	1917	1931	1949	rBV	429187	773017	31.01%	7.506%
24	7.558	2019	2027	2043	rBV2	83721	148032	5.94%	1.437%
25	8.034	2166	2175	2208	rBV	203030	433086	17.38%	4.205%
26	8.789	2400	2410	2429	rBV	473213	783729	31.44%	7.610%
27	9.117	2508	2512	2515	rBV6	2261	1901	0.08%	0.018%
28	9.448	2611	2615	2618	rBV5	1458	1176	0.05%	0.011%
29	9.577	2653	2655	2656	rBV2	1376	526	0.02%	0.005%
30	9.625	2666	2670	2673	rBV5	2139	1939	0.08%	0.019%
31	9.641	2673	2675	2678	rVB4	1564	687	0.03%	0.007%
32	9.715	2696	2698	2699	rBV2	2607	1004	0.04%	0.010%
33	9.738	2703	2705	2706	rBV2	1478	676	0.03%	0.007%
34	9.748	2706	2708	2712	rVB5	1511	794	0.03%	0.008%
35	9.767	2712	2714	2715	rVB2	902	291	0.01%	0.003%
36	9.780	2715	2718	2720	rBV3	2110	1439	0.06%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031114.D
 Acq On : 19 May 2023 18:11
 Operator : SY/MD
 Sample : 02866-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.793	2720	2722	2726	rVV4	2263	1260	0.05%	0.012%
38	9.825	2730	2732	2734	rVB3	1458	538	0.02%	0.005%
39	9.844	2734	2738	2743	rBV8	1383	1392	0.06%	0.014%
40	9.873	2743	2747	2750	rBV6	1949	1591	0.06%	0.015%
41	9.950	2769	2771	2772	rBV2	1211	380	0.02%	0.004%
42	9.989	2782	2783	2786	rVB3	587	207	0.01%	0.002%
43	10.159	2825	2836	2856	rBV	298017	477526	19.16%	4.637%
44	10.252	2864	2865	2868	rBV2	1284	753	0.03%	0.007%
45	10.368	2899	2901	2902	rBV2	1554	813	0.03%	0.008%
46	10.420	2914	2917	2919	rBV3	1415	1122	0.05%	0.011%
47	10.529	2949	2951	2953	rBV3	1562	722	0.03%	0.007%
48	10.648	2987	2988	2990	rBV2	771	360	0.01%	0.003%
49	10.712	3005	3008	3009	rBV3	1436	618	0.02%	0.006%
50	10.722	3009	3011	3013	rVV3	848	288	0.01%	0.003%
51	10.754	3015	3021	3023	rVV5	1535	1548	0.06%	0.015%
52	10.789	3029	3032	3034	rBV4	1744	1227	0.05%	0.012%
53	10.831	3040	3045	3046	rBV5	1113	1000	0.04%	0.010%
54	10.860	3053	3054	3056	rBV2	1335	500	0.02%	0.005%
55	10.873	3056	3058	3061	rVB3	1898	837	0.03%	0.008%
56	10.960	3082	3085	3087	rBV4	1649	857	0.03%	0.008%
57	11.050	3112	3113	3115	rVB2	1432	446	0.02%	0.004%
58	11.063	3115	3117	3119	rBV3	1589	543	0.02%	0.005%
59	11.101	3127	3129	3130	rVB2	973	337	0.01%	0.003%
60	11.120	3130	3135	3137	rBV6	1593	1436	0.06%	0.014%
61	11.191	3144	3157	3174	rBV	394253	626278	25.13%	6.081%
62	11.349	3204	3206	3211	rBV6	1464	1082	0.04%	0.011%
63	11.426	3228	3230	3231	rBV2	1037	389	0.02%	0.004%
64	11.500	3248	3253	3255	rBV6	1816	1783	0.07%	0.017%
65	11.567	3263	3274	3295	rVB	387635	622335	24.97%	6.043%
66	11.702	3312	3316	3319	rBV6	1829	2003	0.08%	0.019%
67	11.773	3335	3338	3340	rVB4	2094	1160	0.05%	0.011%
68	11.796	3341	3345	3347	rBV6	806	610	0.02%	0.006%
69	11.950	3391	3393	3394	rBV2	1360	617	0.02%	0.006%
70	11.960	3394	3396	3397	rVV2	955	314	0.01%	0.003%
71	12.030	3413	3418	3420	rBV7	1691	1483	0.06%	0.014%
72	12.043	3420	3422	3427	rVB6	2300	1670	0.07%	0.016%
73	12.066	3427	3429	3430	rBV2	1772	780	0.03%	0.008%
74	12.162	3454	3459	3460	rBV6	1517	1264	0.05%	0.012%
75	12.188	3464	3467	3468	rBV3	963	641	0.03%	0.006%
76	12.220	3475	3477	3478	rBV2	1483	580	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031114.D
 Acq On : 19 May 2023 18:11
 Operator : SY/MD
 Sample : 02866-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	12.294	3498	3500	3502	rBV3	1123	597	0.02%	0.006%
78	12.345	3514	3516	3518	rBV3	933	524	0.02%	0.005%
79	12.403	3532	3534	3540	rBV6	1412	1114	0.04%	0.011%
80	12.458	3548	3551	3552	rBV3	1600	841	0.03%	0.008%
81	12.680	3618	3620	3623	rBV4	1495	740	0.03%	0.007%
82	12.773	3646	3649	3650	rBV3	1945	1053	0.04%	0.010%
83	12.950	3699	3704	3706	rBV6	2300	2151	0.09%	0.021%
84	13.124	3756	3758	3759	rBV2	1807	642	0.03%	0.006%
85	13.571	3895	3897	3899	rBV3	1753	766	0.03%	0.007%
86	13.947	4012	4014	4016	rBV4	2096	1250	0.05%	0.012%
87	14.429	4160	4164	4165	rBV4	2272	1282	0.05%	0.012%




Sum of corrected areas: 10298633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031114.D
Acq On : 19 May 2023 18:11
Operator : SY/MD
Sample : 02866-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

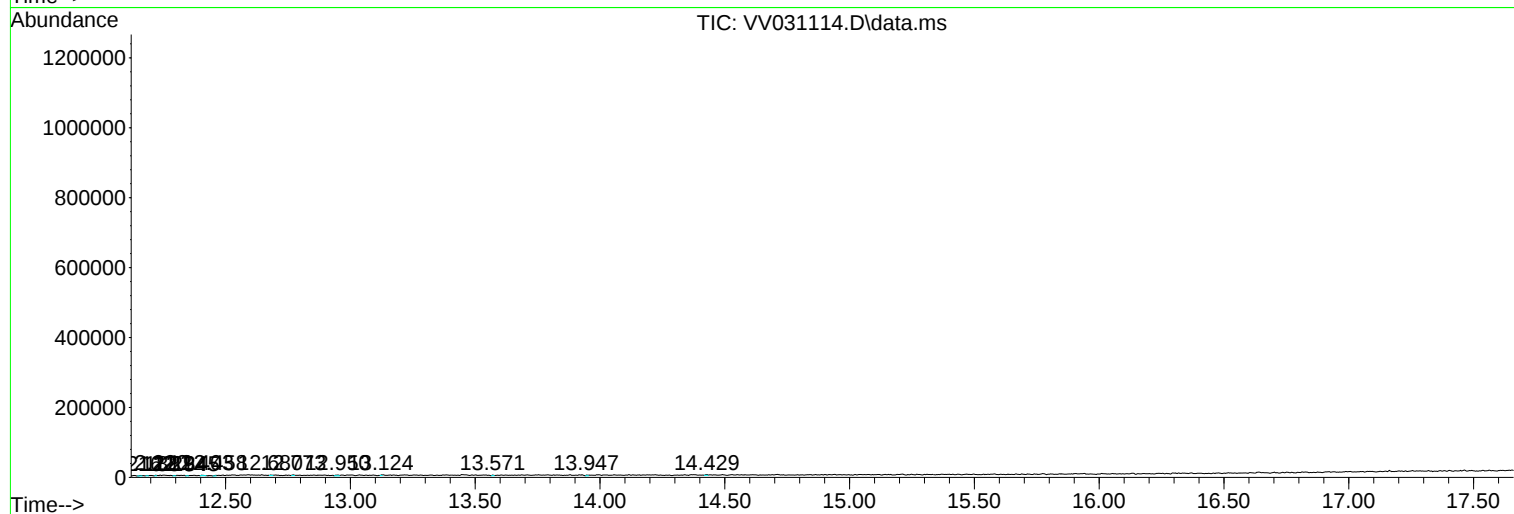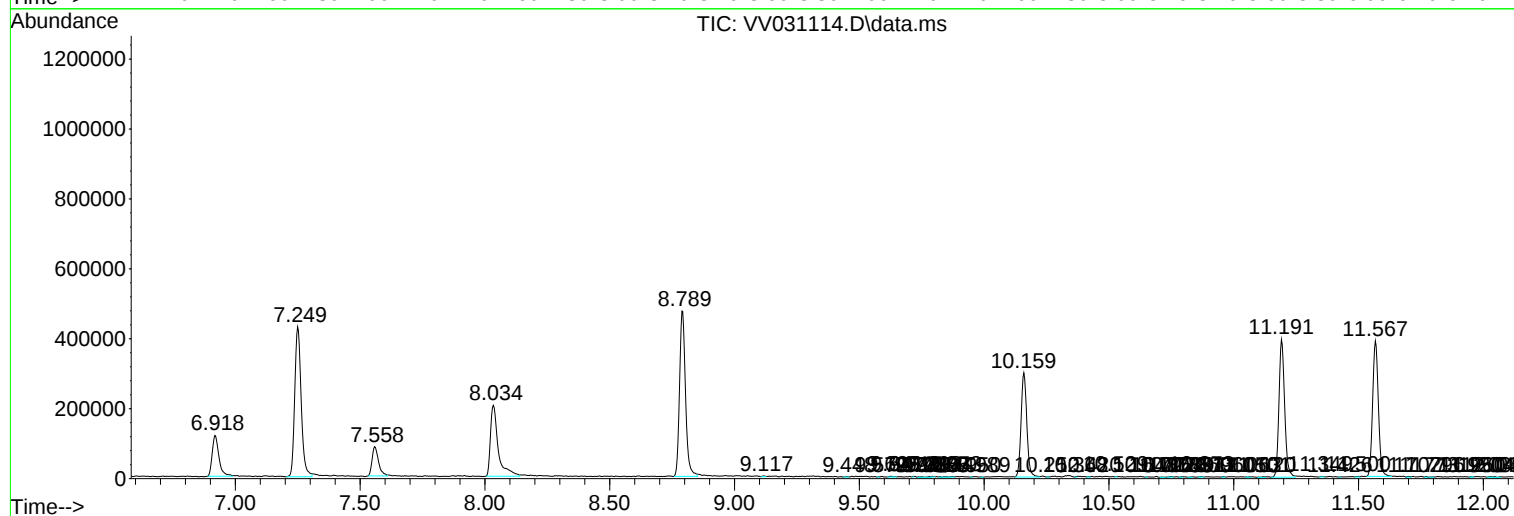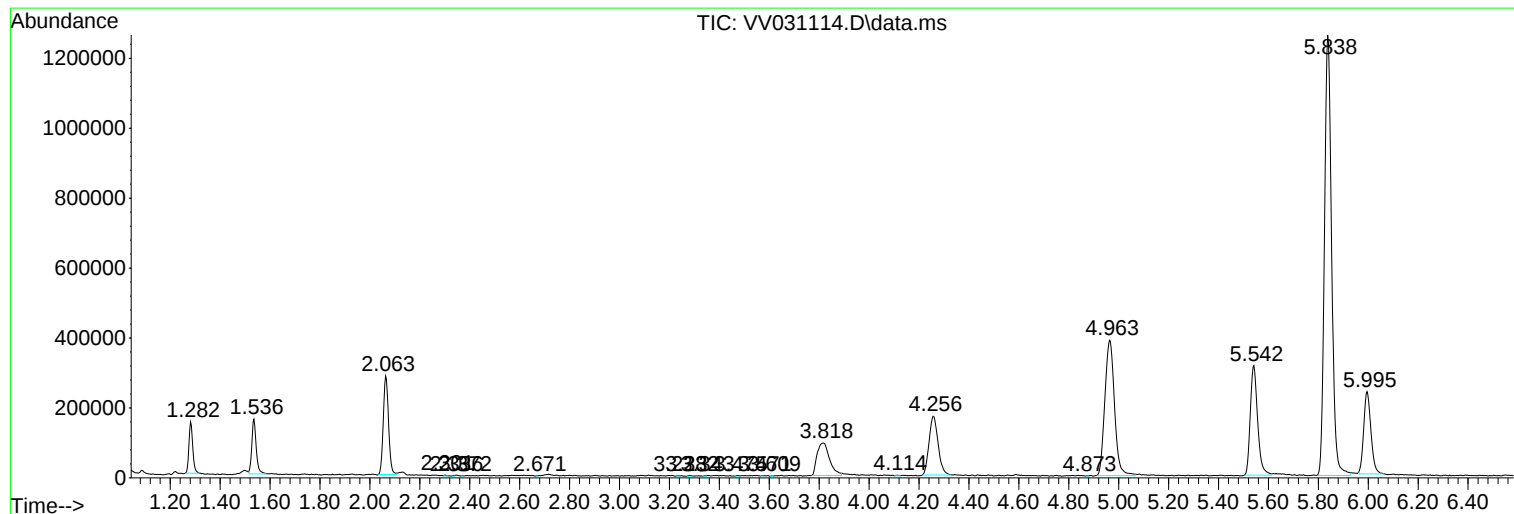

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031114.D
Acq On : 19 May 2023 18:11
Operator : SY/MD
Sample : 02866-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031114.D
Acq On : 19 May 2023 18:11
Operator : SY/MD
Sample : 02866-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc