

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031115.D
 Acq On : 19 May 2023 18:35
 Operator : SY/MD
 Sample : 02866-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	149852	165503	6.86%	1.631%
2	1.532	148	153	165	rVB	170139	201560	8.35%	1.986%
3	2.063	309	318	332	rBV	271477	397258	16.46%	3.914%
4	2.387	417	419	421	rBV2	1339	811	0.03%	0.008%
5	2.545	466	468	470	rBV3	1225	762	0.03%	0.008%
6	2.834	556	558	561	rBV4	1988	902	0.04%	0.009%
7	2.937	588	590	592	rBV3	1806	843	0.03%	0.008%
8	3.262	685	691	692	rBV6	1835	1806	0.07%	0.018%
9	3.272	692	694	696	rVV3	2122	800	0.03%	0.008%
10	3.503	764	766	767	rBV2	1452	656	0.03%	0.006%
11	3.551	778	781	782	rBV3	1245	769	0.03%	0.008%
12	3.638	806	808	810	rVB3	1600	866	0.04%	0.009%
13	3.654	810	813	815	rBV3	1077	738	0.03%	0.007%
14	3.667	815	817	818	rBV2	1169	384	0.02%	0.004%
15	3.818	849	864	889	rBV3	106164	350796	14.53%	3.456%
16	4.256	988	1000	1023	rVB	165432	412266	17.08%	4.062%
17	4.850	1182	1185	1188	rBV5	1783	1513	0.06%	0.015%
18	4.963	1205	1220	1245	rBV2	379517	1000034	41.43%	9.853%
19	5.538	1387	1399	1421	rBV	310686	647966	26.85%	6.384%
20	5.838	1479	1492	1513	rBV	1232653	2413528	100.00%	23.780%
21	5.995	1532	1541	1560	rVB2	229560	457749	18.97%	4.510%
22	6.236	1615	1616	1617	rBV	1850	500	0.02%	0.005%
23	6.918	1820	1828	1849	rVB	109424	202700	8.40%	1.997%
24	7.249	1921	1931	1952	rBV	428079	740869	30.70%	7.300%
25	7.558	2018	2027	2047	rBV	81656	151630	6.28%	1.494%
26	8.034	2166	2175	2206	rBV	203732	418735	17.35%	4.126%
27	8.554	2336	2337	2338	rBV	1473	501	0.02%	0.005%
28	8.638	2361	2363	2365	rBV3	1031	497	0.02%	0.005%
29	8.792	2400	2411	2432	rBV	471011	781947	32.40%	7.704%
30	9.075	2497	2499	2501	rBV3	1754	1145	0.05%	0.011%
31	9.416	2603	2605	2606	rBV2	1503	551	0.02%	0.005%
32	9.542	2640	2644	2646	rBV4	1711	1147	0.05%	0.011%
33	9.577	2652	2655	2657	rBV4	1646	1236	0.05%	0.012%
34	9.638	2672	2674	2675	rBV2	1378	413	0.02%	0.004%
35	9.715	2696	2698	2700	rBV3	1619	472	0.02%	0.005%
36	9.921	2760	2762	2764	rBV3	1488	968	0.04%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031115.D
 Acq On : 19 May 2023 18:35
 Operator : SY/MD
 Sample : 02866-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.159	2826	2836	2854	rBV	302549	472686	19.58%	4.657%
38	10.423	2914	2918	2921	rBV6	2073	1582	0.07%	0.016%
39	10.455	2924	2928	2930	rBV5	1615	1146	0.05%	0.011%
40	10.522	2947	2949	2952	rBV4	1419	946	0.04%	0.009%
41	10.538	2952	2954	2958	rVB4	2258	1314	0.05%	0.013%
42	10.677	2996	2997	2998	rBV	1111	340	0.01%	0.003%
43	10.725	3009	3012	3015	rBV4	1693	1472	0.06%	0.015%
44	10.789	3029	3032	3034	rBV4	1503	937	0.04%	0.009%
45	10.824	3041	3043	3045	rVB3	1633	625	0.03%	0.006%
46	10.837	3045	3047	3050	rVB4	948	301	0.01%	0.003%
47	10.982	3089	3092	3094	rBV3	1191	792	0.03%	0.008%
48	11.014	3100	3102	3104	rVB2	1667	767	0.03%	0.008%
49	11.082	3122	3123	3124	rBV	901	297	0.01%	0.003%
50	11.191	3145	3157	3180	rBV	410913	655095	27.14%	6.455%
51	11.500	3248	3253	3256	rBV7	3945	4510	0.19%	0.044%
52	11.567	3263	3274	3290	rBV	384804	613024	25.40%	6.040%
53	11.840	3357	3359	3362	rVB4	1001	509	0.02%	0.005%
54	11.857	3362	3364	3366	rBV3	1469	630	0.03%	0.006%
55	11.988	3402	3405	3408	rBV5	1617	1027	0.04%	0.010%
56	12.037	3419	3420	3423	rBV3	1082	505	0.02%	0.005%
57	12.062	3426	3428	3433	rVB4	2185	1256	0.05%	0.012%
58	12.091	3433	3437	3438	rBV4	1579	801	0.03%	0.008%
59	12.249	3485	3486	3489	rBV3	1514	712	0.03%	0.007%
60	12.297	3496	3501	3503	rBV6	1517	1314	0.05%	0.013%
61	12.374	3523	3525	3530	rBV6	1526	1355	0.06%	0.013%
62	12.416	3536	3538	3540	rBV3	702	260	0.01%	0.003%
63	12.442	3545	3546	3549	rBV3	1325	783	0.03%	0.008%
64	12.484	3557	3559	3562	rVB3	1393	592	0.02%	0.006%
65	12.503	3562	3565	3568	rBV4	2394	1641	0.07%	0.016%
66	12.603	3594	3596	3599	rBV4	1165	662	0.03%	0.007%
67	12.641	3607	3608	3610	rBV2	1195	604	0.03%	0.006%
68	12.689	3621	3623	3625	rBV3	1644	876	0.04%	0.009%
69	12.725	3632	3634	3636	rVB3	1401	654	0.03%	0.006%
70	12.744	3636	3640	3641	rBV3	1399	472	0.02%	0.005%
71	12.757	3641	3644	3645	rBV3	1550	808	0.03%	0.008%
72	12.786	3651	3653	3656	rVB4	1100	555	0.02%	0.005%
73	12.837	3665	3669	3672	rBV6	1700	1374	0.06%	0.014%
74	12.869	3677	3679	3683	rVV5	1804	1361	0.06%	0.013%
75	12.898	3687	3688	3689	rBV	1326	296	0.01%	0.003%
76	12.930	3694	3698	3699	rBV4	1643	1202	0.05%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031115.D
 Acq On : 19 May 2023 18:35
 Operator : SY/MD
 Sample : 02866-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	12.992	3715	3717	3718	rBV2	1447	604	0.03%	0.006%
78	13.111	3750	3754	3755	rBV3	1835	1127	0.05%	0.011%
79	13.384	3837	3839	3840	rBV	1302	470	0.02%	0.005%
80	13.503	3872	3876	3877	rBV4	1666	1137	0.05%	0.011%
81	13.615	3908	3911	3912	rBV3	1864	1122	0.05%	0.011%
82	13.664	3921	3926	3928	rBV5	2460	2177	0.09%	0.021%
83	13.754	3951	3954	3957	rBV5	2810	2476	0.10%	0.024%
84	13.869	3988	3990	3994	rBV5	1560	899	0.04%	0.009%
85	13.943	4010	4013	4016	rBV5	2341	1823	0.08%	0.018%
86	14.156	4077	4079	4080	rBV2	1457	531	0.02%	0.005%




Sum of corrected areas: 10149270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031115.D
Acq On : 19 May 2023 18:35
Operator : SY/MD
Sample : 02866-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

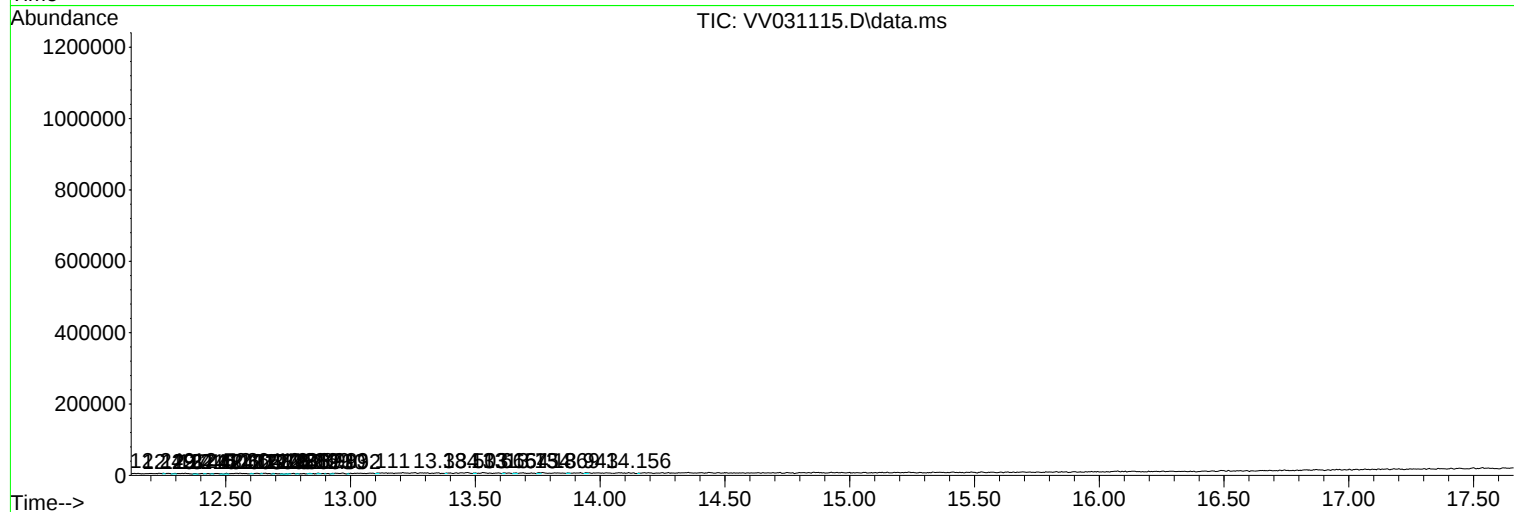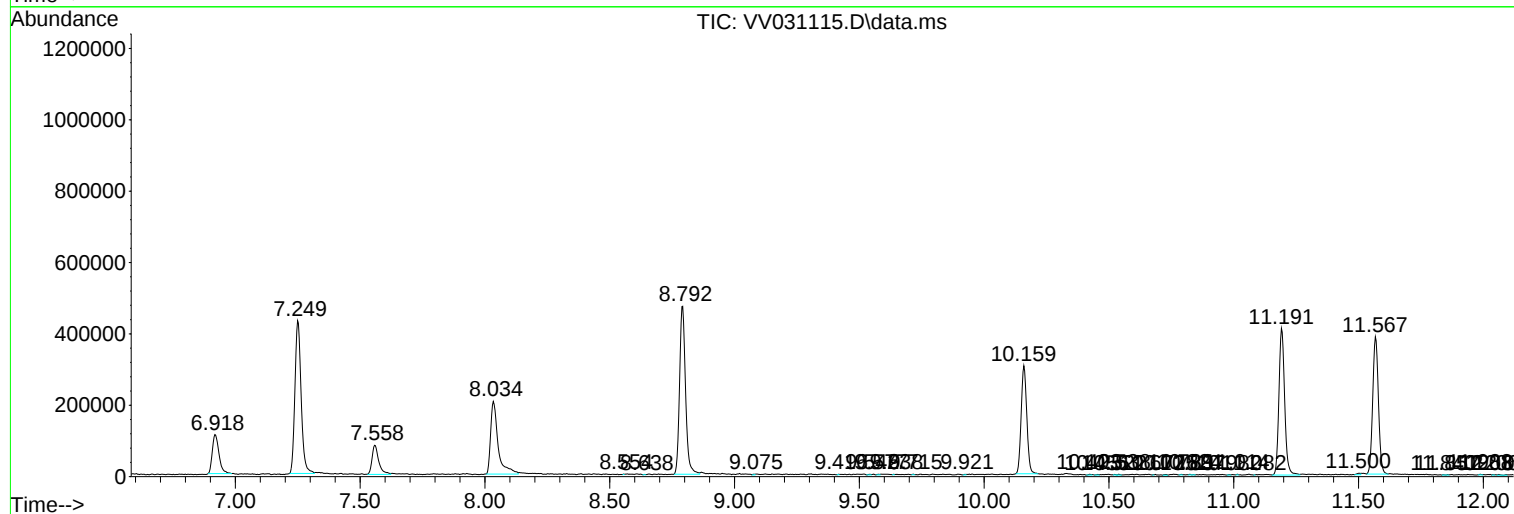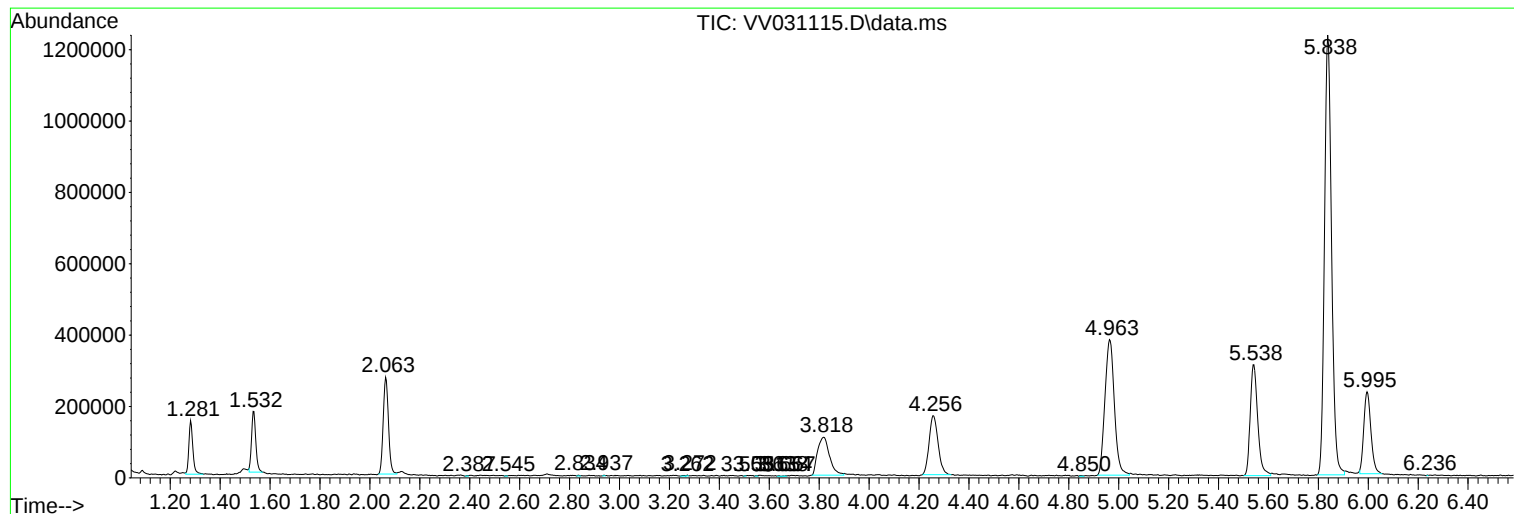

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031115.D
Acq On : 19 May 2023 18:35
Operator : SY/MD
Sample : 02866-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031115.D
Acq On : 19 May 2023 18:35
Operator : SY/MD
Sample : 02866-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------