

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031117.D
 Acq On : 19 May 2023 19:24
 Operator : SY/MD
 Sample : 02866-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	95	rVB	151057	173233	2.11%	1.140%
2	1.535	148	154	169	rVB	171940	211383	2.58%	1.391%
3	2.063	310	318	330	rVB	280678	405006	4.94%	2.665%
4	2.391	418	420	422	rBV2	2064	831	0.01%	0.005%
5	2.519	458	460	463	rBV3	1868	1288	0.02%	0.008%
6	2.690	511	513	516	rBV4	1757	1388	0.02%	0.009%
7	2.767	536	537	539	rBV2	1102	632	0.01%	0.004%
8	2.831	555	557	558	rBV2	1201	463	0.01%	0.003%
9	3.047	622	624	626	rBV2	1179	482	0.01%	0.003%
10	3.059	626	628	630	rBV3	1159	587	0.01%	0.004%
11	3.195	668	670	672	rVB3	1242	393	0.00%	0.003%
12	3.217	674	677	681	rVB5	2408	1652	0.02%	0.011%
13	3.236	681	683	685	rBV3	1501	840	0.01%	0.006%
14	3.288	696	699	700	rBV3	1742	1261	0.02%	0.008%
15	3.397	731	733	736	rBV4	2519	1421	0.02%	0.009%
16	3.661	812	815	816	rBV3	1267	683	0.01%	0.004%
17	3.802	849	859	889	rBV2	68650	230344	2.81%	1.516%
18	4.963	1204	1220	1249	rBV2	394216	1051386	12.83%	6.919%
19	5.542	1389	1400	1422	rBV	304528	626699	7.65%	4.124%
20	5.838	1478	1492	1522	rBV	4278596	8191758	100.00%	53.910%
21	6.918	1819	1828	1845	rBV	116515	211186	2.58%	1.390%
22	7.249	1920	1931	1954	rBV	446853	791764	9.67%	5.211%
23	7.558	2018	2027	2047	rBV	90794	159771	1.95%	1.051%
24	8.034	2166	2175	2204	rBV	204400	421539	5.15%	2.774%
25	8.728	2389	2391	2395	rVB5	2899	2021	0.02%	0.013%
26	8.789	2399	2410	2431	rBV	467595	790848	9.65%	5.205%
27	9.345	2581	2583	2586	rBV3	2197	1364	0.02%	0.009%
28	9.439	2610	2612	2617	rBV6	1630	1953	0.02%	0.013%
29	9.693	2690	2691	2693	rBV2	1198	579	0.01%	0.004%
30	9.892	2748	2753	2756	rBV7	2323	2389	0.03%	0.016%
31	9.953	2771	2772	2775	rBV4	1489	720	0.01%	0.005%
32	10.001	2784	2787	2789	rBV4	2529	1735	0.02%	0.011%
33	10.085	2811	2813	2815	rBV2	1325	820	0.01%	0.005%
34	10.159	2825	2836	2853	rBV	311779	499731	6.10%	3.289%
35	10.429	2918	2920	2922	rVB3	1902	802	0.01%	0.005%
36	10.574	2961	2965	2968	rBV6	1991	1793	0.02%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031117.D
 Acq On : 19 May 2023 19:24
 Operator : SY/MD
 Sample : 02866-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.628	2977	2982	2983	rBV5	1698	1425	0.02%	0.009%
38	10.689	2999	3001	3004	rVB5	1797	821	0.01%	0.005%
39	10.828	3042	3044	3045	rBV2	1441	637	0.01%	0.004%
40	11.027	3104	3106	3107	rBV2	1024	382	0.00%	0.003%
41	11.191	3147	3157	3174	rBV	432264	679792	8.30%	4.474%
42	11.567	3264	3274	3292	rVB	436362	684342	8.35%	4.504%
43	11.821	3349	3353	3355	rBV4	3157	2457	0.03%	0.016%
44	11.853	3361	3363	3368	rBV6	1678	1249	0.02%	0.008%
45	11.969	3397	3399	3402	rVB4	1706	588	0.01%	0.004%
46	11.988	3402	3405	3407	rBV3	1481	816	0.01%	0.005%
47	12.075	3430	3432	3433	rBV2	1155	408	0.00%	0.003%
48	12.249	3484	3486	3487	rBV3	1242	529	0.01%	0.003%
49	12.381	3523	3527	3529	rBV4	1920	1519	0.02%	0.010%
50	12.435	3542	3544	3549	rVB5	1516	1085	0.01%	0.007%
51	12.464	3551	3553	3556	rVV4	1253	877	0.01%	0.006%
52	12.496	3560	3563	3565	rBV4	1696	860	0.01%	0.006%
53	12.512	3565	3568	3570	rBV4	1409	862	0.01%	0.006%
54	12.567	3583	3585	3587	rBV2	1514	574	0.01%	0.004%
55	12.580	3587	3589	3594	rBV6	1172	1086	0.01%	0.007%
56	12.648	3607	3610	3612	rBV4	1711	1331	0.02%	0.009%
57	12.728	3633	3635	3638	rBV3	2131	1491	0.02%	0.010%
58	12.760	3643	3645	3647	rBV3	1551	873	0.01%	0.006%
59	12.895	3685	3687	3691	rBV5	1639	1185	0.01%	0.008%
60	12.921	3693	3695	3698	rVB4	1343	731	0.01%	0.005%
61	12.950	3700	3704	3708	rVV7	1081	1007	0.01%	0.007%
62	13.001	3717	3720	3721	rBV3	1195	547	0.01%	0.004%
63	13.014	3721	3724	3728	rBV6	1596	1530	0.02%	0.010%
64	13.069	3737	3741	3742	rBV4	1309	1074	0.01%	0.007%
65	13.117	3751	3756	3758	rBV5	1874	1683	0.02%	0.011%
66	13.133	3758	3761	3768	rVB8	1739	1570	0.02%	0.010%
67	13.159	3768	3769	3772	rBV2	880	446	0.01%	0.003%
68	13.181	3774	3776	3777	rBV2	935	419	0.01%	0.003%
69	13.207	3782	3784	3786	rVV3	1156	609	0.01%	0.004%
70	13.297	3807	3812	3815	rBV7	2310	2375	0.03%	0.016%
71	13.358	3828	3831	3833	rBV4	1566	1208	0.01%	0.008%
72	13.496	3873	3874	3876	rBV2	771	249	0.00%	0.002%
73	13.516	3878	3880	3884	rVB4	1141	644	0.01%	0.004%
74	13.538	3884	3887	3891	rBV5	2380	2225	0.03%	0.015%
75	13.567	3894	3896	3898	rVB3	3081	1199	0.01%	0.008%
76	13.580	3898	3900	3902	rBV3	1846	986	0.01%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031117.D
Acq On : 19 May 2023 19:24
Operator : SY/MD
Sample : 02866-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis

77	14.130	4070	4071	4075	rVB4	1507	716	0.01%	0.005%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 15195152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031117.D
Acq On : 19 May 2023 19:24
Operator : SY/MD
Sample : 02866-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

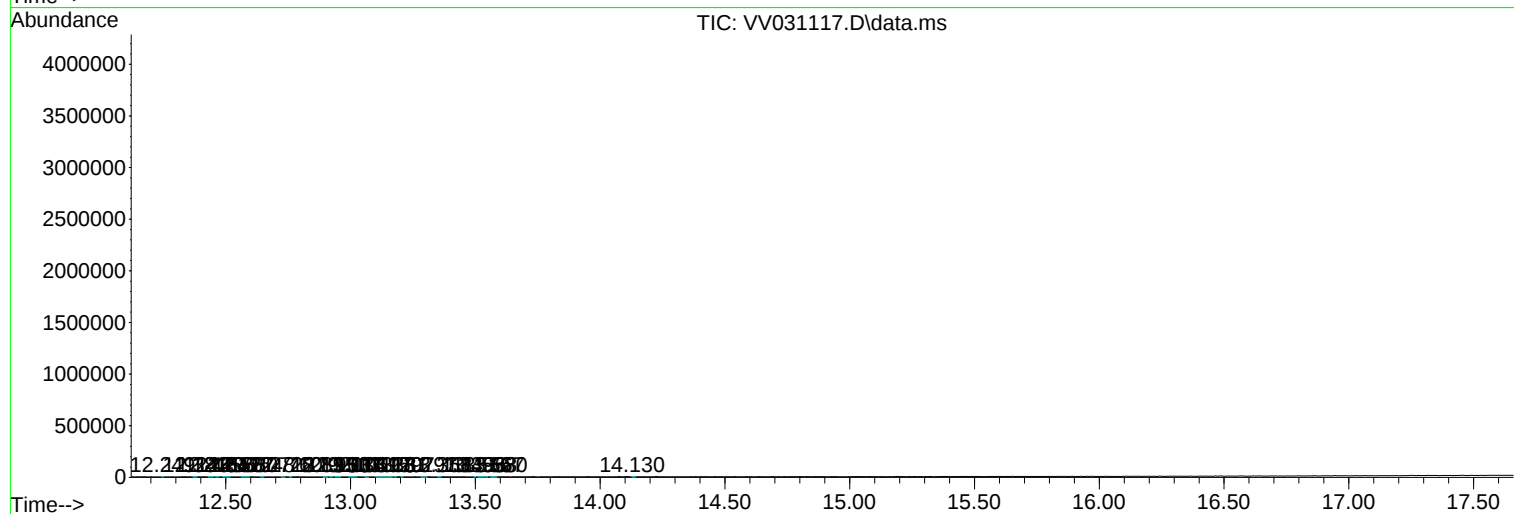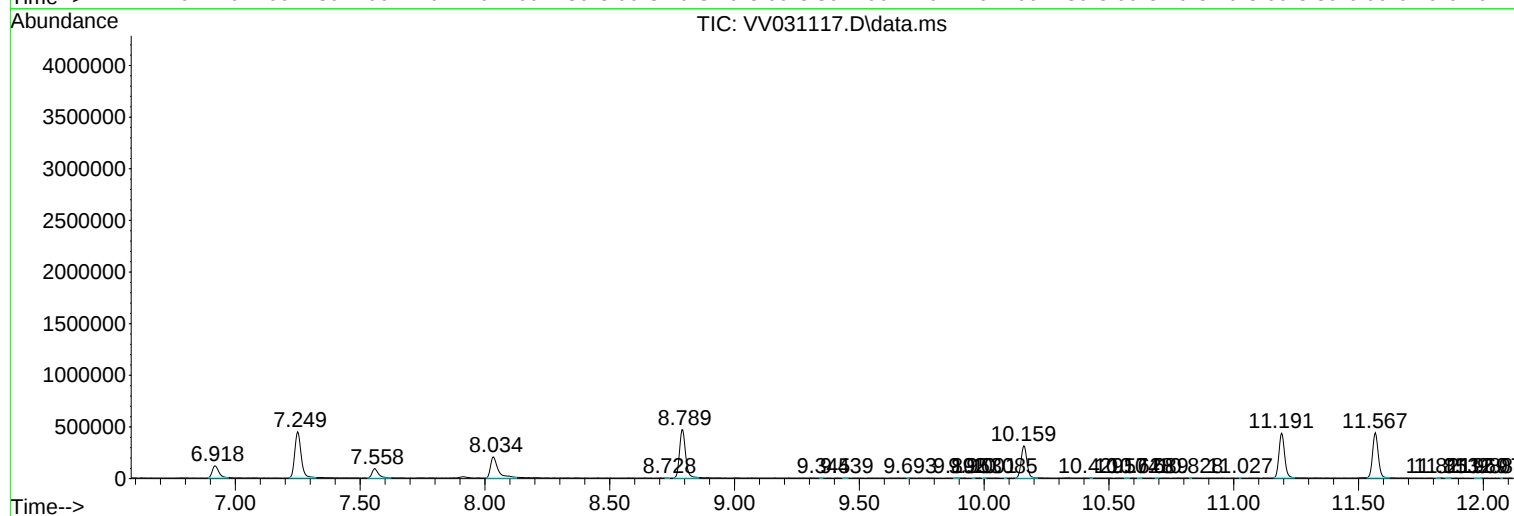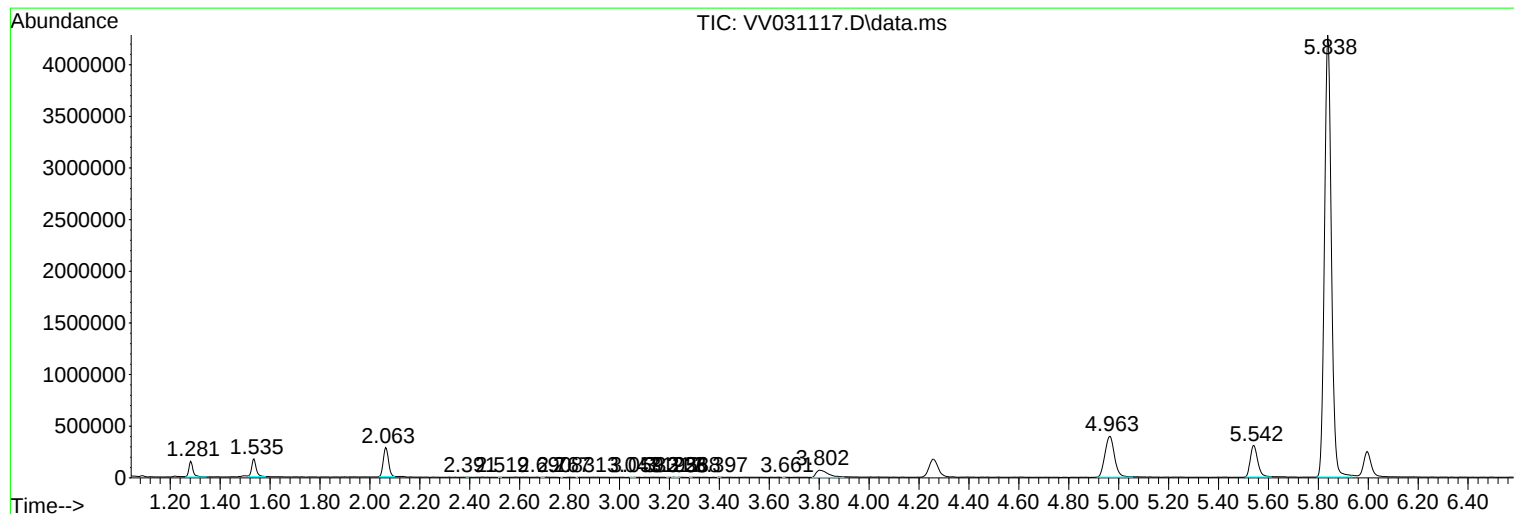

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031117.D
Acq On : 19 May 2023 19:24
Operator : SY/MD
Sample : 02866-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031117.D
Acq On : 19 May 2023 19:24
Operator : SY/MD
Sample : 02866-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------