

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031118.D
 Acq On : 19 May 2023 19:49
 Operator : SY/MD
 Sample : 02866-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	93	rVB	151695	170232	2.15%	1.119%
2	1.536	148	154	171	rVB	163068	203689	2.57%	1.338%
3	2.063	309	318	332	rBV	281099	407515	5.15%	2.678%
4	2.237	370	372	377	rBV5	1441	1080	0.01%	0.007%
5	2.494	447	452	458	rBV10	1928	2574	0.03%	0.017%
6	2.574	473	477	478	rBV3	1564	1017	0.01%	0.007%
7	2.896	575	577	578	rBV2	1489	560	0.01%	0.004%
8	2.979	601	603	606	rVB4	1640	666	0.01%	0.004%
9	3.195	668	670	673	rBV4	1298	776	0.01%	0.005%
10	3.343	713	716	717	rBV3	1584	778	0.01%	0.005%
11	3.449	747	749	752	rVB4	1837	666	0.01%	0.004%
12	3.529	772	774	777	rBV4	1536	730	0.01%	0.005%
13	3.606	793	798	800	rBV5	1548	1498	0.02%	0.010%
14	3.802	849	859	881	rBV2	64251	204091	2.58%	1.341%
15	4.175	972	975	976	rBV3	1616	761	0.01%	0.005%
16	4.256	987	1000	1024	rVB3	169266	428338	5.41%	2.814%
17	4.876	1187	1193	1194	rBV4	1604	1381	0.02%	0.009%
18	4.963	1202	1220	1247	rBV2	394719	1057360	13.36%	6.947%
19	5.542	1388	1400	1423	rBV	303119	641165	8.10%	4.213%
20	5.838	1478	1492	1524	rBV	4150966	7916096	100.00%	52.013%
21	6.735	1766	1771	1772	rBV5	1733	1393	0.02%	0.009%
22	6.921	1819	1829	1844	rBV2	116483	212061	2.68%	1.393%
23	7.114	1887	1889	1892	rBV3	2681	1628	0.02%	0.011%
24	7.249	1920	1931	1949	rBV	440047	779902	9.85%	5.124%
25	7.558	2019	2027	2046	rVB	81523	145664	1.84%	0.957%
26	8.034	2165	2175	2201	rBV	205647	427460	5.40%	2.809%
27	8.712	2384	2386	2388	rBV3	1549	704	0.01%	0.005%
28	8.793	2399	2411	2431	rBV	462624	778372	9.83%	5.114%
29	8.950	2457	2460	2462	rBV3	2208	1659	0.02%	0.011%
30	9.207	2536	2540	2542	rBV5	1548	1338	0.02%	0.009%
31	9.506	2632	2633	2635	rBV2	1331	479	0.01%	0.003%
32	9.555	2644	2648	2652	rVB5	1945	1574	0.02%	0.010%
33	9.577	2652	2655	2657	rBV3	1809	1067	0.01%	0.007%
34	9.629	2666	2671	2674	rBV7	2431	2008	0.03%	0.013%
35	9.664	2679	2682	2684	rBV4	1016	609	0.01%	0.004%
36	9.789	2718	2721	2724	rBV5	1266	671	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031118.D
 Acq On : 19 May 2023 19:49
 Operator : SY/MD
 Sample : 02866-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.802	2724	2725	2727	rVV2	1061	537	0.01%	0.004%
38	9.831	2731	2734	2736	rBV4	988	567	0.01%	0.004%
39	9.892	2751	2753	2757	rVB5	2178	1330	0.02%	0.009%
40	9.912	2757	2759	2761	rBV3	2001	935	0.01%	0.006%
41	9.931	2761	2765	2767	rVV4	1707	1480	0.02%	0.010%
42	9.950	2769	2771	2775	rVB4	1450	813	0.01%	0.005%
43	9.969	2775	2777	2780	rBV4	1575	1074	0.01%	0.007%
44	9.992	2782	2784	2786	rVB3	2104	1006	0.01%	0.007%
45	10.008	2786	2789	2792	rBV5	1445	534	0.01%	0.004%
46	10.034	2794	2797	2799	rBV4	1738	1014	0.01%	0.007%
47	10.056	2802	2804	2807	rBV4	959	488	0.01%	0.003%
48	10.114	2818	2822	2824	rBV5	1560	1214	0.02%	0.008%
49	10.159	2825	2836	2858	rVB	287018	460500	5.82%	3.026%
50	10.442	2921	2924	2926	rBV4	1218	672	0.01%	0.004%
51	10.477	2932	2935	2939	rBV5	1795	1419	0.02%	0.009%
52	10.522	2947	2949	2953	rBV5	1296	865	0.01%	0.006%
53	10.545	2953	2956	2957	rBV3	1297	633	0.01%	0.004%
54	10.577	2963	2966	2968	rBV4	1309	905	0.01%	0.006%
55	10.616	2973	2978	2980	rBV6	1918	1393	0.02%	0.009%
56	10.632	2980	2983	2988	rBV6	1268	1339	0.02%	0.009%
57	10.686	2998	3000	3002	rVB3	1224	547	0.01%	0.004%
58	10.706	3002	3006	3008	rBV5	1229	875	0.01%	0.006%
59	10.773	3025	3027	3028	rBV	1854	736	0.01%	0.005%
60	10.873	3055	3058	3061	rVB5	1037	500	0.01%	0.003%
61	10.892	3061	3064	3066	rBV4	1333	810	0.01%	0.005%
62	10.953	3081	3083	3084	rBV2	1170	560	0.01%	0.004%
63	11.014	3100	3102	3105	rVB4	1477	952	0.01%	0.006%
64	11.088	3124	3125	3128	rBV3	1772	1095	0.01%	0.007%
65	11.127	3135	3137	3139	rBV3	1667	1073	0.01%	0.007%
66	11.191	3145	3157	3176	rBV	393757	633402	8.00%	4.162%
67	11.465	3239	3242	3243	rBV3	779	476	0.01%	0.003%
68	11.490	3246	3250	3251	rBV4	1779	1210	0.02%	0.008%
69	11.567	3261	3274	3290	rBV	414091	663056	8.38%	4.357%
70	11.674	3305	3307	3311	rBV5	1878	1264	0.02%	0.008%
71	11.796	3343	3345	3350	rBV6	1446	962	0.01%	0.006%
72	11.902	3375	3378	3383	rVB6	2188	1897	0.02%	0.012%
73	11.931	3383	3387	3393	rVB8	2191	2240	0.03%	0.015%
74	12.008	3407	3411	3413	rBV3	1347	1134	0.01%	0.007%
75	12.120	3442	3446	3450	rBV7	2005	1576	0.02%	0.010%
76	12.140	3450	3452	3456	rVV5	893	742	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031118.D
 Acq On : 19 May 2023 19:49
 Operator : SY/MD
 Sample : 02866-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.265	3489	3491	3494	rVB4	1542	768	0.01%	0.005%
78	12.281	3494	3496	3499	rBV4	882	583	0.01%	0.004%
79	12.304	3499	3503	3510	rVB7	2250	1978	0.02%	0.013%
80	12.365	3518	3522	3528	rBV8	2385	2351	0.03%	0.015%
81	12.423	3538	3540	3541	rBV3	1454	659	0.01%	0.004%
82	12.500	3561	3564	3565	rBV3	1002	518	0.01%	0.003%
83	12.535	3572	3575	3576	rBV3	1239	777	0.01%	0.005%
84	12.590	3589	3592	3593	rBV2	980	612	0.01%	0.004%
85	12.667	3613	3616	3619	rBV5	1990	1621	0.02%	0.011%
86	12.889	3683	3685	3689	rBV4	1400	984	0.01%	0.006%
87	12.985	3709	3715	3722	rBV4	1896	2856	0.04%	0.019%
88	13.111	3751	3754	3756	rBV4	1686	1277	0.02%	0.008%
89	13.307	3813	3815	3816	rBV	970	499	0.01%	0.003%
90	13.326	3818	3821	3824	rBV5	2218	1742	0.02%	0.011%
91	13.403	3843	3845	3846	rBV2	1626	636	0.01%	0.004%
92	13.429	3850	3853	3857	rBV6	1579	1603	0.02%	0.011%
93	13.509	3876	3878	3882	rBV5	1893	1402	0.02%	0.009%
94	13.564	3893	3895	3898	rBV4	2349	1327	0.02%	0.009%
95	13.808	3969	3971	3976	rVB6	1929	1017	0.01%	0.007%
96	14.201	4090	4093	4096	rBV5	1931	1153	0.01%	0.008%
97	14.220	4097	4099	4100	rBV2	1956	694	0.01%	0.005%
98	14.259	4107	4111	4113	rBV5	2281	1813	0.02%	0.012%
99	14.484	4179	4181	4182	rBV3	1816	808	0.01%	0.005%
100	14.583	4210	4212	4213	rBV2	1331	477	0.01%	0.003%




Sum of corrected areas: 15219542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031118.D
Acq On : 19 May 2023 19:49
Operator : SY/MD
Sample : 02866-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

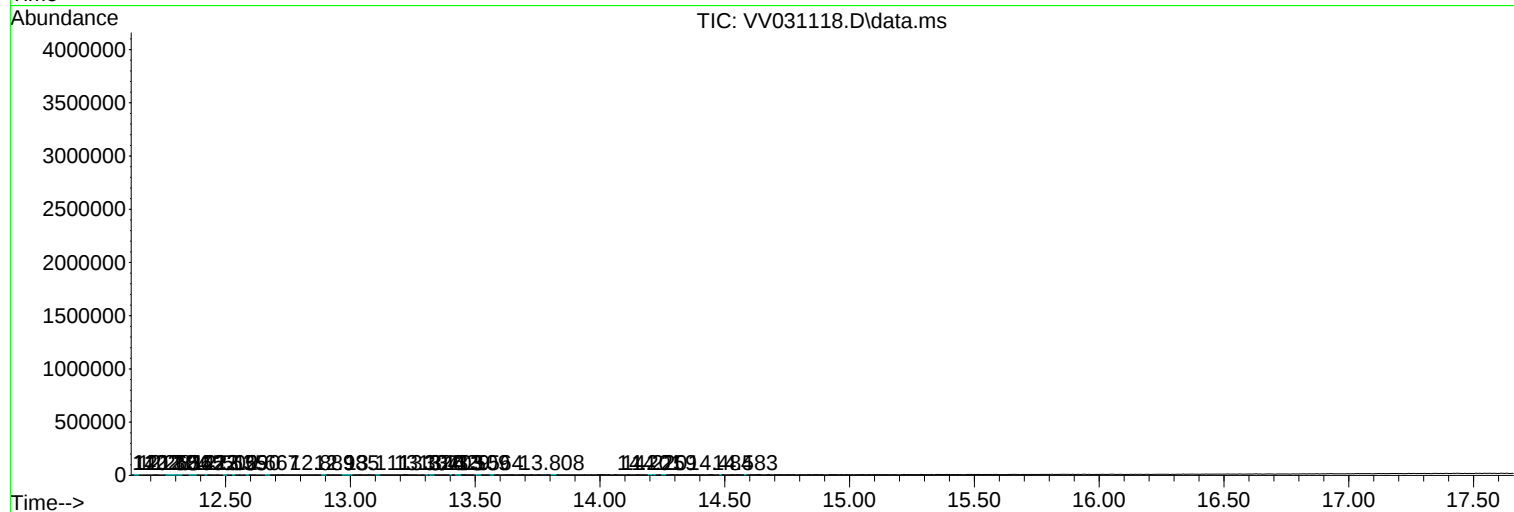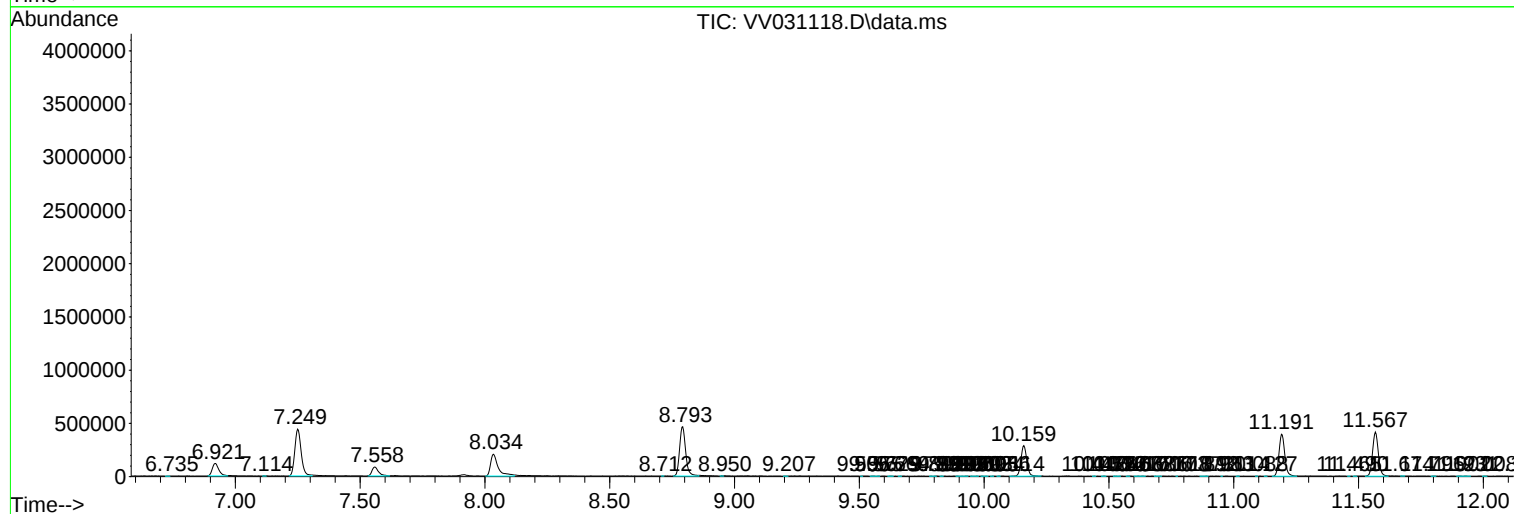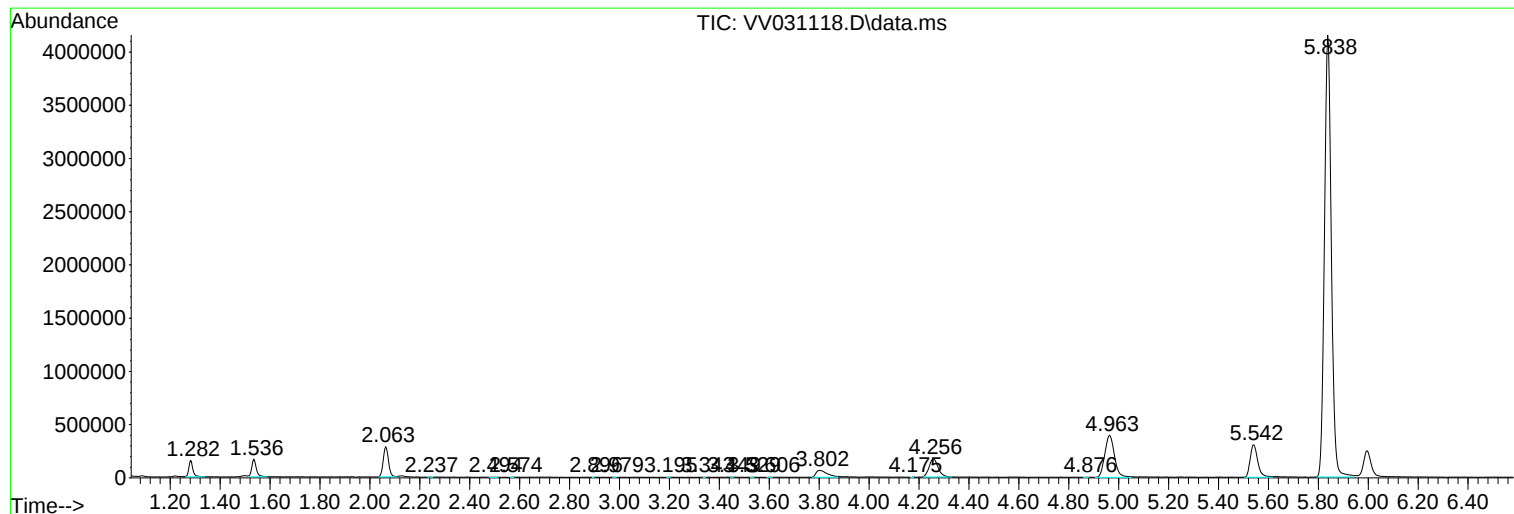

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031118.D
Acq On : 19 May 2023 19:49
Operator : SY/MD
Sample : 02866-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031118.D
Acq On : 19 May 2023 19:49
Operator : SY/MD
Sample : 02866-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc