

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031120.D
 Acq On : 19 May 2023 20:38
 Operator : SY/MD
 Sample : 02866-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	146400	161094	1.55%	0.912%
2	1.536	148	154	168	rVB	157186	188716	1.82%	1.068%
3	2.063	309	318	331	rBV	278502	412018	3.97%	2.332%
4	2.542	464	467	469	rBV4	1699	1258	0.01%	0.007%
5	2.812	547	551	555	rBV7	1759	1393	0.01%	0.008%
6	2.835	555	558	561	rBV5	2008	1558	0.02%	0.009%
7	2.989	603	606	608	rVV4	1243	772	0.01%	0.004%
8	3.021	614	616	621	rVB5	2295	1626	0.02%	0.009%
9	3.060	625	628	630	rBV3	1599	752	0.01%	0.004%
10	3.211	671	675	680	rBV7	1178	1114	0.01%	0.006%
11	3.275	691	695	699	rBV7	2501	2609	0.03%	0.015%
12	3.330	708	712	713	rBV3	1631	1085	0.01%	0.006%
13	3.429	737	743	745	rBV6	2406	2120	0.02%	0.012%
14	3.442	745	747	752	rVB6	2525	1595	0.02%	0.009%
15	3.513	765	769	770	rBV4	2293	1188	0.01%	0.007%
16	3.523	770	772	776	rVB5	2114	1120	0.01%	0.006%
17	3.622	801	803	806	rBV4	2046	1609	0.02%	0.009%
18	3.683	817	822	824	rBV6	1410	1140	0.01%	0.006%
19	3.748	837	842	846	rBV8	2230	2508	0.02%	0.014%
20	3.809	849	861	884	rBV3	66522	217785	2.10%	1.233%
21	4.256	987	1000	1025	rVB	170046	432428	4.17%	2.448%
22	4.783	1162	1164	1172	rVB8	1631	1240	0.01%	0.007%
23	4.963	1204	1220	1243	rBV3	395820	1044786	10.07%	5.914%
24	5.542	1387	1400	1422	rBV	297544	623871	6.01%	3.531%
25	5.838	1477	1492	1528	rBV	5434655	10379197	100.00%	58.747%
26	6.497	1695	1697	1700	rBV4	1845	851	0.01%	0.005%
27	6.699	1758	1760	1762	rBV3	1564	879	0.01%	0.005%
28	6.799	1787	1791	1795	rBV8	1807	1704	0.02%	0.010%
29	6.847	1804	1806	1809	rBV4	1582	964	0.01%	0.005%
30	6.918	1819	1828	1845	rBV	117896	215031	2.07%	1.217%
31	7.060	1868	1872	1874	rBV4	1559	1125	0.01%	0.006%
32	7.249	1920	1931	1955	rBV	440064	768211	7.40%	4.348%
33	7.561	2019	2028	2046	rBV	84343	150260	1.45%	0.850%
34	8.034	2166	2175	2191	rBV	194647	378314	3.64%	2.141%
35	8.413	2291	2293	2296	rBV4	1776	1262	0.01%	0.007%
36	8.455	2301	2306	2309	rBV6	2103	2238	0.02%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031120.D
 Acq On : 19 May 2023 20:38
 Operator : SY/MD
 Sample : 02866-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	8.600	2348	2351	2356	rVB7	1583	1271	0.01%	0.007%
38	8.632	2356	2361	2362	rBV5	1901	1568	0.02%	0.009%
39	8.754	2395	2399	2400	rBV3	2552	1892	0.02%	0.011%
40	8.789	2400	2410	2430	rVV	452361	750895	7.23%	4.250%
41	9.352	2582	2585	2587	rBV3	1646	1188	0.01%	0.007%
42	9.596	2659	2661	2663	rBV3	1865	962	0.01%	0.005%
43	9.744	2704	2707	2708	rBV3	1870	907	0.01%	0.005%
44	9.847	2737	2739	2740	rBV2	1717	747	0.01%	0.004%
45	9.895	2751	2754	2757	rBV4	1536	826	0.01%	0.005%
46	9.908	2757	2758	2761	rBV3	1369	942	0.01%	0.005%
47	10.024	2791	2794	2797	rBV4	1971	1306	0.01%	0.007%
48	10.104	2818	2819	2822	rBV3	1636	811	0.01%	0.005%
49	10.159	2824	2836	2851	rBV	311144	494143	4.76%	2.797%
50	10.243	2860	2862	2864	rBV3	1748	1004	0.01%	0.006%
51	10.603	2971	2974	2979	rVB6	1929	1403	0.01%	0.008%
52	10.645	2984	2987	2991	rVB5	1456	1277	0.01%	0.007%
53	10.683	2995	2999	3001	rVB4	1487	920	0.01%	0.005%
54	10.709	3001	3007	3010	rBV6	2138	2287	0.02%	0.013%
55	10.757	3020	3022	3026	rVB4	1785	1035	0.01%	0.006%
56	10.850	3048	3051	3055	rBV6	1594	1230	0.01%	0.007%
57	10.928	3071	3075	3076	rBV4	1921	1433	0.01%	0.008%
58	10.960	3081	3085	3086	rBV4	1577	1159	0.01%	0.007%
59	11.043	3107	3111	3113	rBV4	1464	1217	0.01%	0.007%
60	11.191	3146	3157	3178	rBV	414910	660835	6.37%	3.740%
61	11.442	3232	3235	3237	rBV3	1649	1046	0.01%	0.006%
62	11.567	3264	3274	3294	rVB	430479	680609	6.56%	3.852%
63	11.683	3308	3310	3312	rBV2	1858	997	0.01%	0.006%
64	11.947	3390	3392	3397	rBV6	1698	1385	0.01%	0.008%
65	11.982	3399	3403	3404	rBV3	2173	1556	0.01%	0.009%
66	12.037	3417	3420	3421	rBV3	1960	813	0.01%	0.005%
67	12.146	3450	3454	3458	rBV7	1899	2124	0.02%	0.012%
68	12.191	3465	3468	3471	rBV5	1982	1740	0.02%	0.010%
69	12.255	3486	3488	3493	rBV6	1892	1440	0.01%	0.008%
70	12.278	3493	3495	3497	rBV3	1822	972	0.01%	0.006%
71	12.390	3528	3530	3535	rBV5	1000	765	0.01%	0.004%
72	12.445	3545	3547	3551	rBV5	1492	917	0.01%	0.005%
73	12.526	3568	3572	3577	rVB7	1919	1902	0.02%	0.011%
74	12.551	3577	3580	3585	rBV6	2343	2457	0.02%	0.014%
75	12.815	3659	3662	3664	rBV4	1922	1158	0.01%	0.007%
76	12.873	3677	3680	3682	rBV3	2361	1307	0.01%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031120.D
 Acq On : 19 May 2023 20:38
 Operator : SY/MD
 Sample : 02866-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.902	3685	3689	3690	rBV4	1409	875	0.01%	0.005%
78	12.963	3707	3708	3711	rVB3	1714	758	0.01%	0.004%
79	12.985	3711	3715	3717	rBV4	2281	1710	0.02%	0.010%
80	13.079	3739	3744	3745	rBV5	2680	1800	0.02%	0.010%
81	13.114	3752	3755	3757	rBV4	2152	1399	0.01%	0.008%
82	13.146	3763	3765	3767	rBV2	1669	817	0.01%	0.005%
83	13.307	3810	3815	3819	rBV8	2477	2137	0.02%	0.012%
84	13.326	3819	3821	3824	rBV4	2066	1086	0.01%	0.006%
85	13.352	3828	3829	3831	rBV2	1721	743	0.01%	0.004%
86	13.394	3837	3842	3845	rBV6	1623	1680	0.02%	0.010%
87	13.458	3860	3862	3867	rBV6	1124	944	0.01%	0.005%
88	13.516	3877	3880	3883	rBV5	1468	1070	0.01%	0.006%
89	13.596	3903	3905	3907	rVB3	1925	760	0.01%	0.004%
90	13.657	3921	3924	3925	rBV3	1650	1030	0.01%	0.006%
91	13.821	3971	3975	3979	rBV6	2751	2921	0.03%	0.017%
92	13.995	4026	4029	4030	rBV3	1573	808	0.01%	0.005%
93	14.030	4038	4040	4042	rBV3	1590	725	0.01%	0.004%
94	14.043	4042	4044	4046	rBV3	1811	916	0.01%	0.005%
95	14.079	4052	4055	4057	rBV4	1851	925	0.01%	0.005%
96	14.252	4106	4109	4113	rBV5	1865	1257	0.01%	0.007%
97	14.291	4119	4121	4124	rBV4	1747	973	0.01%	0.006%
98	14.754	4261	4265	4267	rBV5	2068	1759	0.02%	0.010%
99	14.815	4282	4284	4286	rBV3	2013	800	0.01%	0.005%
100	15.268	4423	4425	4429	rBV4	2311	1862	0.02%	0.011%




Sum of corrected areas: 17667622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031120.D
Acq On : 19 May 2023 20:38
Operator : SY/MD
Sample : 02866-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

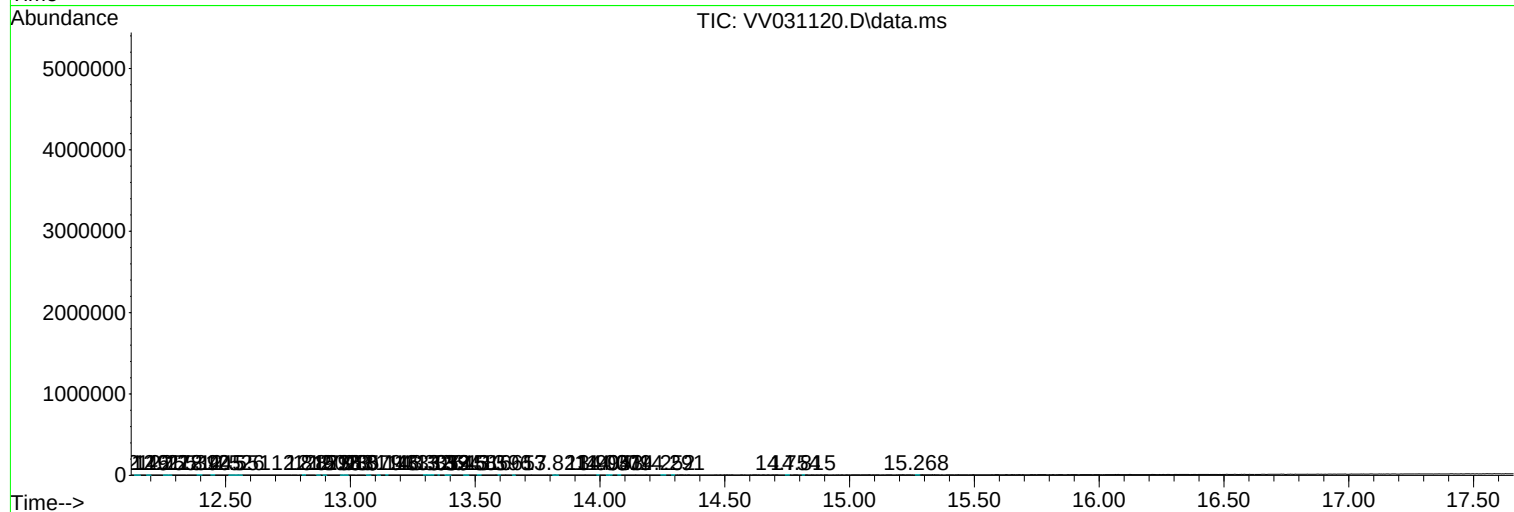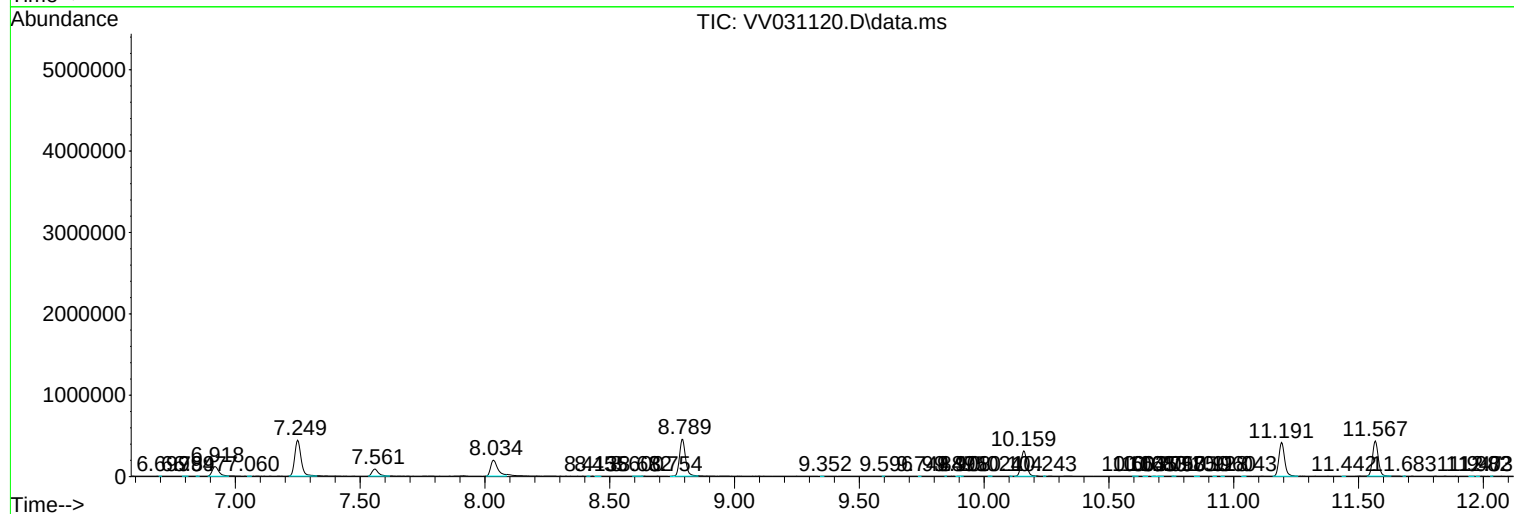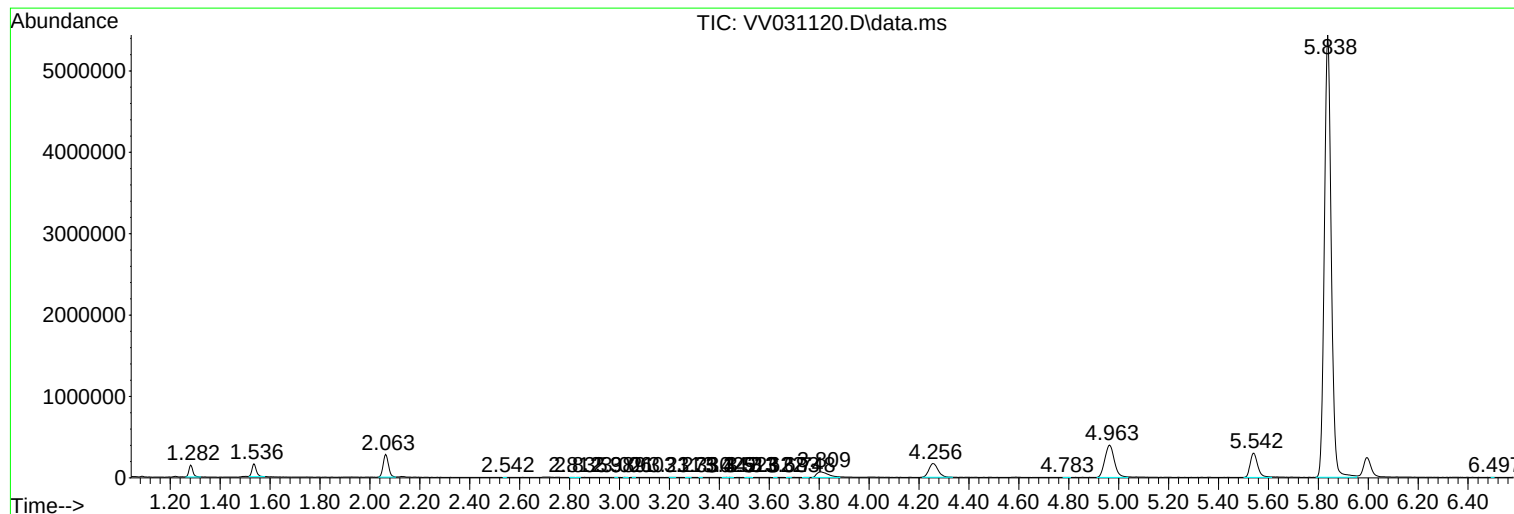

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031120.D
Acq On : 19 May 2023 20:38
Operator : SY/MD
Sample : 02866-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031120.D
Acq On : 19 May 2023 20:38
Operator : SY/MD
Sample : 02866-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------