

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031122.D
 Acq On : 19 May 2023 21:27
 Operator : SY/MD
 Sample : 02866-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	143940	160753	0.45%	0.352%
2	1.536	148	154	171	rVB	151358	180378	0.51%	0.395%
3	2.066	310	319	333	rVB2	304354	476570	1.34%	1.043%
4	2.375	412	415	417	rBV4	1713	1048	0.00%	0.002%
5	2.484	448	449	454	rBV5	1693	1134	0.00%	0.002%
6	2.928	585	587	593	rBV6	1793	1545	0.00%	0.003%
7	3.021	612	616	619	rBV5	1472	1171	0.00%	0.003%
8	3.079	632	634	636	rBV3	1178	475	0.00%	0.001%
9	3.198	667	671	672	rBV3	1219	753	0.00%	0.002%
10	3.343	712	716	720	rBV6	1937	2170	0.01%	0.005%
11	3.458	750	752	756	rBV4	1844	1196	0.00%	0.003%
12	3.822	849	865	901	rBV2	1172223	2889878	8.10%	6.325%
13	4.256	987	1000	1024	rVB2	172197	431163	1.21%	0.944%
14	4.773	1159	1161	1165	rBV5	1523	886	0.00%	0.002%
15	4.963	1204	1220	1248	rBV2	384415	1022587	2.87%	2.238%
16	5.387	1348	1352	1354	rBV5	2054	1691	0.00%	0.004%
17	5.542	1387	1400	1423	rBV	312156	658909	1.85%	1.442%
18	5.841	1477	1493	1531	rBV	19048773	35670153	100.00%	78.076%
19	6.815	1794	1796	1799	rVB4	2404	1193	0.00%	0.003%
20	6.828	1799	1800	1801	rBV	1244	416	0.00%	0.001%
21	6.918	1818	1828	1848	rBV2	111040	217519	0.61%	0.476%
22	7.194	1910	1914	1915	rBV3	2165	1352	0.00%	0.003%
23	7.249	1921	1931	1947	rBV	416319	725808	2.03%	1.589%
24	7.558	2019	2027	2045	rVB	80576	140710	0.39%	0.308%
25	7.850	2116	2118	2119	rBV2	1442	531	0.00%	0.001%
26	8.034	2166	2175	2204	rBV	196489	414810	1.16%	0.908%
27	8.436	2296	2300	2305	rBV8	2081	2036	0.01%	0.004%
28	8.744	2392	2396	2398	rBV5	1902	1397	0.00%	0.003%
29	8.789	2400	2410	2428	rBV	469228	787362	2.21%	1.723%
30	9.436	2607	2611	2612	rBV4	1944	1236	0.00%	0.003%
31	9.474	2619	2623	2624	rBV3	2448	1579	0.00%	0.003%
32	9.551	2645	2647	2651	rBV5	1500	1083	0.00%	0.002%
33	9.590	2657	2659	2661	rVB3	1139	377	0.00%	0.001%
34	9.664	2680	2682	2686	rBV5	1157	904	0.00%	0.002%
35	9.744	2705	2707	2708	rBV2	1485	460	0.00%	0.001%
36	10.159	2826	2836	2854	rVB	301947	473568	1.33%	1.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031122.D
 Acq On : 19 May 2023 21:27
 Operator : SY/MD
 Sample : 02866-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.436	2919	2922	2925	rBV5	2561	2061	0.01%	0.005%
38	10.661	2990	2992	2995	rBV4	1473	839	0.00%	0.002%
39	10.680	2995	2998	3001	rVB5	2167	1377	0.00%	0.003%
40	10.760	3019	3023	3024	rBV3	2304	1468	0.00%	0.003%
41	10.844	3045	3049	3051	rBV4	1473	1326	0.00%	0.003%
42	10.931	3073	3076	3077	rBV3	2237	966	0.00%	0.002%
43	11.027	3104	3106	3108	rBV3	1540	710	0.00%	0.002%
44	11.191	3146	3157	3179	rBV	435444	695592	1.95%	1.523%
45	11.567	3264	3274	3294	rVB	410196	655150	1.84%	1.434%
46	11.918	3381	3383	3386	rBV4	1442	914	0.00%	0.002%
47	11.976	3399	3401	3407	rVB6	2375	1313	0.00%	0.003%
48	12.101	3438	3440	3441	rBV2	1741	672	0.00%	0.001%
49	12.207	3470	3473	3476	rBV5	1413	1219	0.00%	0.003%
50	12.259	3487	3489	3491	rVB3	620	278	0.00%	0.001%
51	12.278	3491	3495	3497	rBV5	1056	939	0.00%	0.002%
52	12.288	3497	3498	3501	rVB3	1051	527	0.00%	0.001%
53	12.342	3512	3515	3517	rBV3	985	510	0.00%	0.001%
54	12.371	3521	3524	3525	rBV3	1148	688	0.00%	0.002%
55	12.416	3534	3538	3540	rVB5	1590	986	0.00%	0.002%
56	12.429	3540	3542	3545	rBV4	1089	686	0.00%	0.002%
57	12.474	3554	3556	3558	rBV3	682	286	0.00%	0.001%
58	12.487	3558	3560	3561	rBV2	846	356	0.00%	0.001%
59	12.525	3570	3572	3576	rVB5	1698	1120	0.00%	0.002%
60	12.545	3576	3578	3579	rBV2	1468	535	0.00%	0.001%
61	12.554	3579	3581	3583	rVB3	1121	439	0.00%	0.001%
62	12.577	3585	3588	3589	rBV3	854	541	0.00%	0.001%
63	12.641	3606	3608	3611	rBV3	1143	630	0.00%	0.001%
64	12.667	3611	3616	3618	rVV6	1916	1532	0.00%	0.003%
65	12.689	3621	3623	3625	rBV3	781	464	0.00%	0.001%
66	12.722	3630	3633	3634	rBV3	1186	603	0.00%	0.001%
67	12.747	3639	3641	3642	rBV2	971	384	0.00%	0.001%
68	12.886	3682	3684	3687	rBV4	1672	810	0.00%	0.002%
69	12.915	3687	3693	3695	rBV6	1798	1730	0.00%	0.004%
70	12.937	3698	3700	3702	rVB3	1191	477	0.00%	0.001%
71	13.017	3723	3725	3727	rVB3	753	297	0.00%	0.001%
72	13.188	3776	3778	3780	rBV3	836	423	0.00%	0.001%
73	13.242	3792	3795	3798	rBV5	1255	907	0.00%	0.002%
74	13.281	3802	3807	3810	rBV7	2402	2429	0.01%	0.005%
75	13.355	3826	3830	3833	rVV5	1840	1070	0.00%	0.002%
76	13.378	3835	3837	3839	rBV3	814	584	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031122.D
 Acq On : 19 May 2023 21:27
 Operator : SY/MD
 Sample : 02866-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	13.509	3876	3878	3879	rBV2	1506	626	0.00%	0.001%
78	13.551	3889	3891	3892	rBV2	600	272	0.00%	0.001%
79	13.564	3892	3895	3896	rBV3	1533	741	0.00%	0.002%
80	13.654	3921	3923	3925	rBV3	1278	593	0.00%	0.001%
81	13.705	3935	3939	3941	rBV4	1822	1437	0.00%	0.003%
82	13.831	3975	3978	3979	rBV2	1308	656	0.00%	0.001%
83	13.879	3989	3993	3996	rBV6	1401	1148	0.00%	0.003%
84	13.924	4004	4007	4009	rBV4	1190	632	0.00%	0.001%
85	14.027	4036	4039	4042	rBV4	1695	1267	0.00%	0.003%
86	14.085	4054	4057	4060	rBV4	1776	1319	0.00%	0.003%
87	14.133	4067	4072	4075	rBV7	1406	1376	0.00%	0.003%
88	14.172	4082	4084	4087	rVB3	2205	1130	0.00%	0.002%
89	14.197	4089	4092	4095	rBV5	1883	1626	0.00%	0.004%
90	14.226	4099	4101	4103	rBV3	1465	619	0.00%	0.001%
91	14.390	4148	4152	4156	rBV5	1784	1865	0.01%	0.004%
92	14.496	4180	4185	4187	rBV5	2400	2297	0.01%	0.005%
93	14.596	4213	4216	4218	rBV4	1952	1355	0.00%	0.003%
94	14.644	4226	4231	4232	rBV4	1787	1465	0.00%	0.003%
95	14.680	4240	4242	4244	rBV3	1851	1058	0.00%	0.002%
96	14.767	4267	4269	4272	rVB3	2085	984	0.00%	0.002%
97	15.069	4361	4363	4365	rBV3	1418	837	0.00%	0.002%
98	15.117	4374	4378	4380	rBV5	1377	1013	0.00%	0.002%
99	15.403	4465	4467	4470	rVB4	3093	1512	0.00%	0.003%
100	15.493	4490	4495	4498	rBV7	2505	2137	0.01%	0.005%




Sum of corrected areas: 45686604

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031122.D
Acq On : 19 May 2023 21:27
Operator : SY/MD
Sample : 02866-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

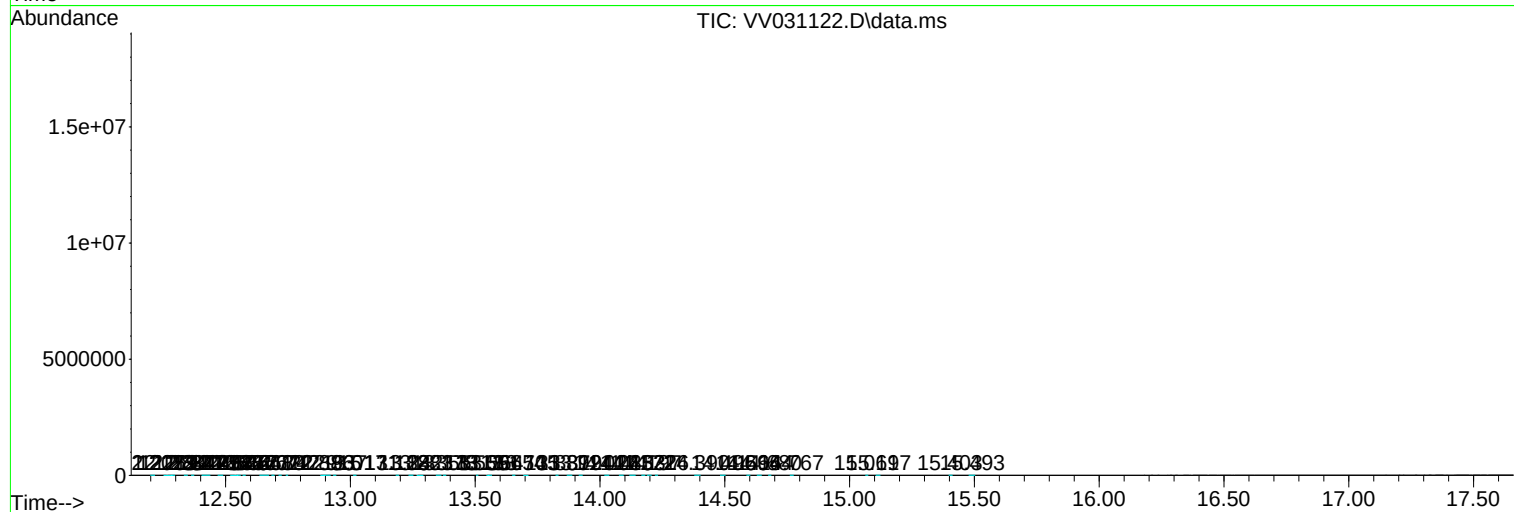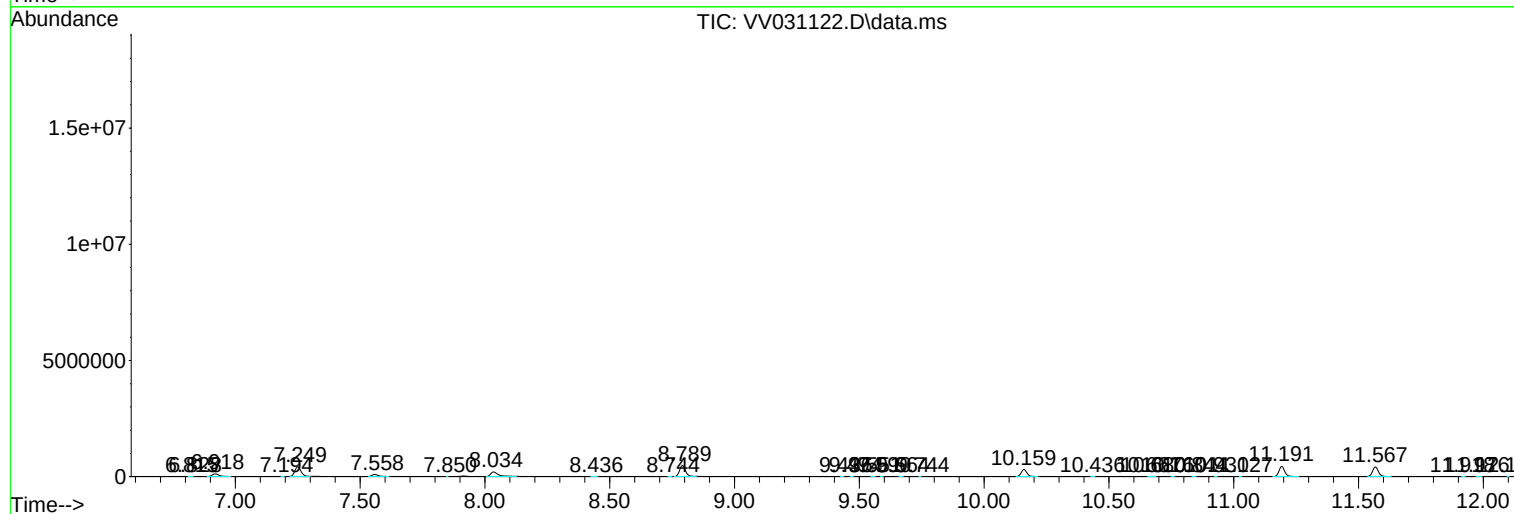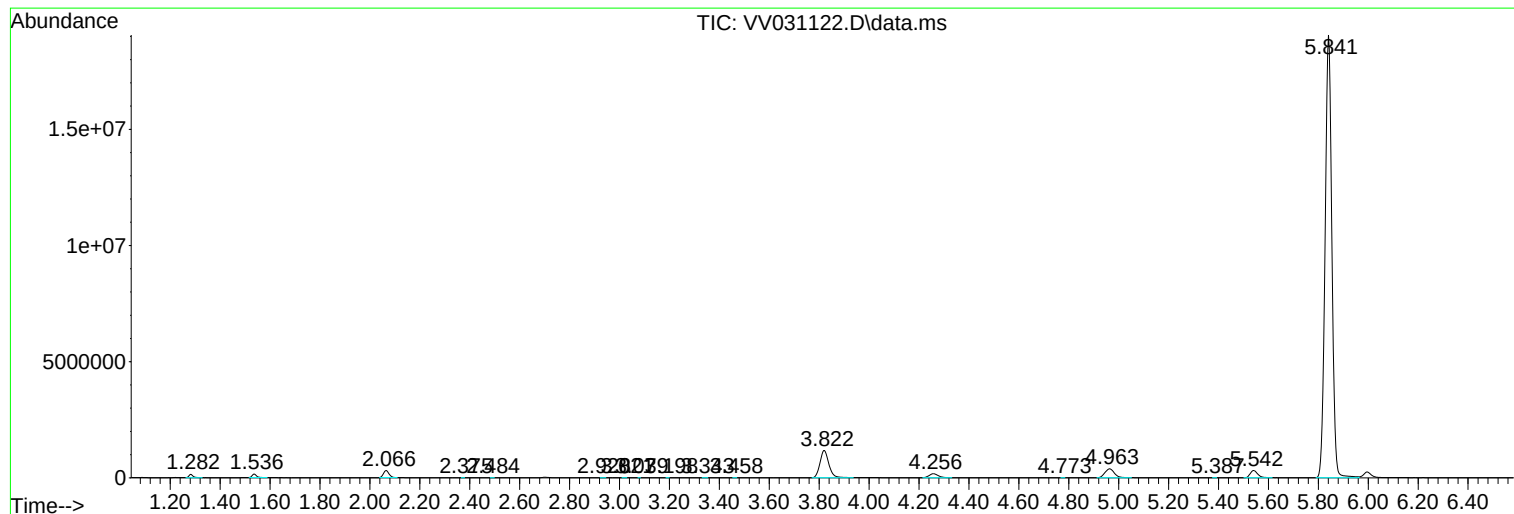

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031122.D
Acq On : 19 May 2023 21:27
Operator : SY/MD
Sample : 02866-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031122.D
Acq On : 19 May 2023 21:27
Operator : SY/MD
Sample : 02866-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------