

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031130.D
 Acq On : 20 May 2023 01:28
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rVB	135177	142004	14.33%	1.721%
2	1.532	148	153	167	rVB	126890	152451	15.39%	1.847%
3	2.063	309	318	332	rBV	258709	384672	38.82%	4.661%
4	2.362	408	411	414	rBV4	1959	1477	0.15%	0.018%
5	3.015	612	614	617	rBV4	1529	863	0.09%	0.010%
6	3.044	620	623	624	rBV3	1858	947	0.10%	0.011%
7	3.072	630	632	633	rBV2	1471	731	0.07%	0.009%
8	3.163	659	660	663	rVB3	1979	886	0.09%	0.011%
9	3.182	663	666	669	rBV5	2024	1578	0.16%	0.019%
10	3.455	748	751	757	rBV7	2661	2919	0.29%	0.035%
11	3.481	757	759	760	rBV2	1581	623	0.06%	0.008%
12	3.510	766	768	770	rBV2	2780	1537	0.16%	0.019%
13	3.577	787	789	792	rBV3	1888	1391	0.14%	0.017%
14	3.806	849	860	890	rBV3	69225	249673	25.20%	3.025%
15	4.256	988	1000	1026	rVB	165597	424627	42.85%	5.146%
16	4.732	1146	1148	1152	rBV5	1443	1081	0.11%	0.013%
17	4.963	1204	1220	1244	rBV2	378014	990871	100.00%	12.007%
18	5.365	1342	1345	1347	rBV3	2606	1457	0.15%	0.018%
19	5.539	1388	1399	1424	rBV	318846	662933	66.90%	8.033%
20	5.838	1482	1492	1510	rBV	320047	605691	61.13%	7.340%
21	5.995	1531	1541	1557	rVB	216512	426354	43.03%	5.166%
22	6.423	1672	1674	1676	rBV3	1297	569	0.06%	0.007%
23	6.545	1707	1712	1714	rBV6	2223	2038	0.21%	0.025%
24	6.918	1818	1828	1845	rBV	109946	202491	20.44%	2.454%
25	7.140	1895	1897	1904	rBV6	2693	2064	0.21%	0.025%
26	7.249	1921	1931	1952	rBV	413347	727434	73.41%	8.815%
27	7.561	2019	2028	2047	rBV	76227	137614	13.89%	1.668%
28	8.034	2166	2175	2205	rBV	207084	417100	42.09%	5.054%
29	8.532	2327	2330	2332	rBV3	1944	1375	0.14%	0.017%
30	8.789	2400	2410	2434	rBV	467086	797622	80.50%	9.665%
31	9.661	2674	2681	2687	rBV10	4671	8607	0.87%	0.104%
32	9.889	2750	2752	2753	rBV2	1705	673	0.07%	0.008%
33	10.159	2826	2836	2859	rVB	299355	476676	48.11%	5.776%
34	10.436	2917	2922	2924	rBV6	1590	1254	0.13%	0.015%
35	10.448	2924	2926	2928	rBV3	1693	733	0.07%	0.009%
36	10.484	2934	2937	2945	rBV9	2564	3044	0.31%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031130.D
 Acq On : 20 May 2023 01:28
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.731	3012	3014	3015	rBV2	1416	425	0.04%	0.005%
38	10.953	3079	3083	3084	rBV4	1004	621	0.06%	0.008%
39	11.085	3122	3124	3126	rBV3	1662	779	0.08%	0.009%
40	11.104	3126	3130	3134	rVV7	2235	2039	0.21%	0.025%
41	11.191	3146	3157	3176	rBV	421020	676873	68.31%	8.202%
42	11.387	3213	3218	3220	rBV5	2386	1992	0.20%	0.024%
43	11.452	3236	3238	3240	rVB2	1719	736	0.07%	0.009%
44	11.500	3240	3253	3262	rBV3	16501	33262	3.36%	0.403%
45	11.567	3264	3274	3295	rVB	411347	661487	66.76%	8.016%
46	11.722	3319	3322	3323	rBV4	1605	948	0.10%	0.011%
47	11.831	3354	3356	3360	rBV5	1670	1245	0.13%	0.015%
48	11.876	3364	3370	3374	rBV9	2392	2753	0.28%	0.033%
49	11.944	3389	3391	3392	rBV2	1130	417	0.04%	0.005%
50	11.979	3399	3402	3406	rBV7	1395	919	0.09%	0.011%
51	12.040	3419	3421	3422	rBV	1582	626	0.06%	0.008%
52	12.104	3439	3441	3444	rBV3	1446	872	0.09%	0.011%
53	12.156	3453	3457	3458	rBV4	984	656	0.07%	0.008%
54	12.230	3479	3480	3481	rBV2	895	202	0.02%	0.002%
55	12.291	3497	3499	3501	rBV3	1592	650	0.07%	0.008%
56	12.339	3511	3514	3517	rBV4	2040	2001	0.20%	0.024%
57	12.403	3532	3534	3535	rVB2	862	214	0.02%	0.003%
58	12.416	3535	3538	3539	rBV3	1601	969	0.10%	0.012%
59	12.455	3546	3550	3552	rBV4	1542	902	0.09%	0.011%
60	12.497	3561	3563	3567	rBV5	1428	1100	0.11%	0.013%
61	12.516	3567	3569	3573	rVB5	1590	700	0.07%	0.008%
62	12.545	3573	3578	3580	rBV6	1643	1584	0.16%	0.019%
63	12.599	3591	3595	3599	rVB7	2790	2468	0.25%	0.030%
64	12.622	3599	3602	3603	rBV3	1424	750	0.08%	0.009%
65	12.693	3623	3624	3628	rBV4	1116	672	0.07%	0.008%
66	12.712	3628	3630	3631	rBV2	1074	329	0.03%	0.004%
67	12.744	3638	3640	3643	rBV4	1360	838	0.08%	0.010%
68	12.779	3649	3651	3652	rBV2	910	272	0.03%	0.003%
69	12.812	3660	3661	3664	rVB3	1551	664	0.07%	0.008%
70	12.834	3666	3668	3675	rVB8	1711	1738	0.18%	0.021%
71	12.863	3675	3677	3679	rVB3	964	375	0.04%	0.005%
72	12.879	3679	3682	3685	rBV5	1328	1165	0.12%	0.014%
73	12.924	3694	3696	3699	rBV5	984	335	0.03%	0.004%
74	12.940	3699	3701	3706	rBV5	1172	798	0.08%	0.010%
75	13.017	3724	3725	3728	rBV3	696	399	0.04%	0.005%
76	13.069	3739	3741	3745	rBV4	1794	1487	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031130.D
 Acq On : 20 May 2023 01:28
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	13.088	3745	3747	3751	rVV5	1201	757	0.08%	0.009%
78	13.124	3756	3758	3763	rVB6	1450	1058	0.11%	0.013%
79	13.146	3763	3765	3768	rBV4	1386	998	0.10%	0.012%
80	13.178	3774	3775	3778	rBV3	1280	865	0.09%	0.010%
81	13.300	3810	3813	3814	rBV3	1180	533	0.05%	0.006%
82	13.490	3870	3872	3876	rBV5	1204	593	0.06%	0.007%
83	13.622	3911	3913	3915	rBV3	1332	556	0.06%	0.007%
84	14.120	4066	4068	4072	rVB5	3655	2507	0.25%	0.030%
85	14.140	4072	4074	4075	rBV2	1528	770	0.08%	0.009%
86	14.358	4140	4142	4143	rBV2	2454	1171	0.12%	0.014%
87	15.146	4385	4387	4389	rVB3	3019	1188	0.12%	0.014%


Sum of corrected areas: 8252318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031130.D
Acq On : 20 May 2023 01:28
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

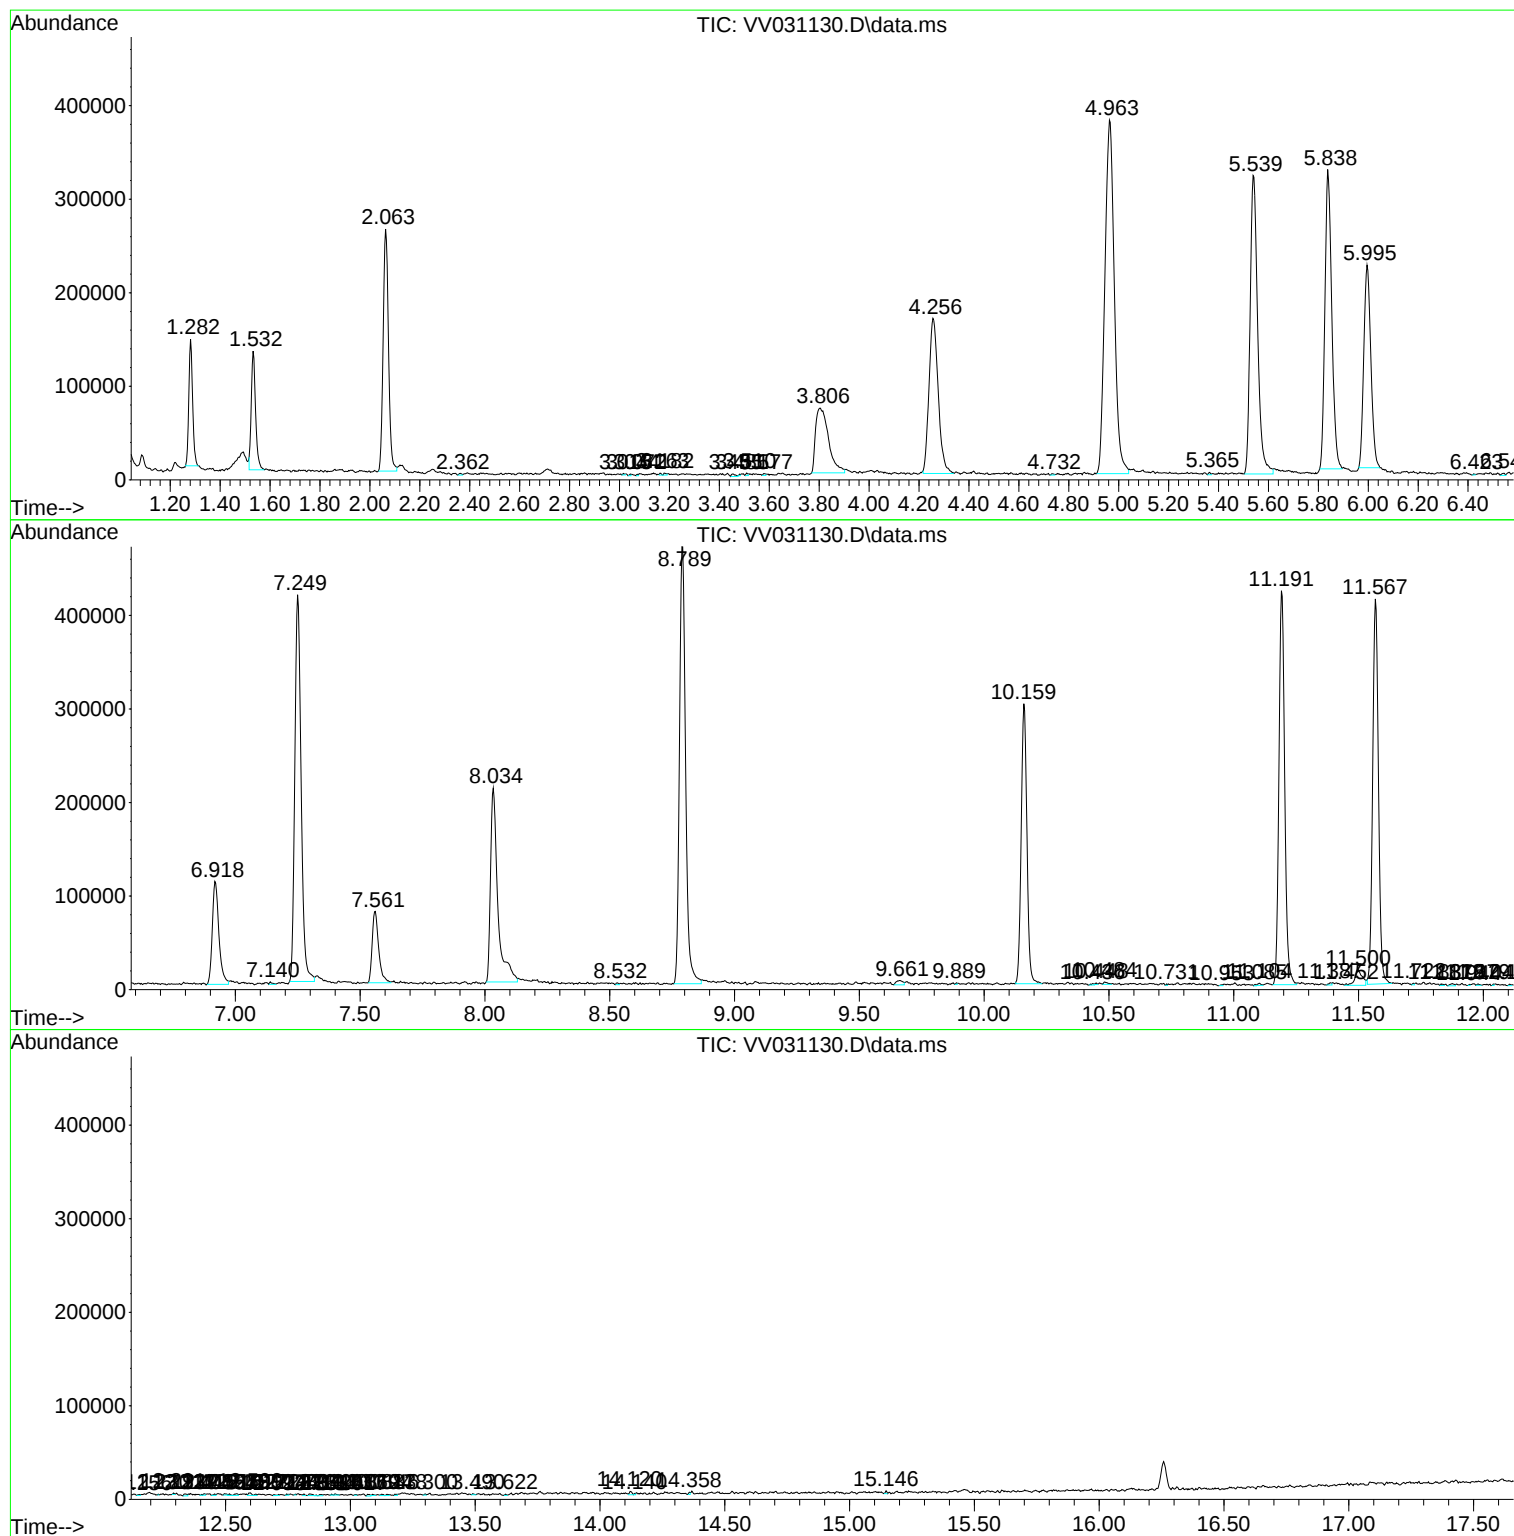

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031130.D
Acq On : 20 May 2023 01:28
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031130.D
Acq On : 20 May 2023 01:28
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------