

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031143.D
 Acq On : 20 May 2023 06:48
 Operator : SY/MD
 Sample : 02865-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	86	rVB	130318	136871	14.40%	1.907%
2	1.532	147	153	169	rVB	105564	135835	14.29%	1.892%
3	2.063	310	318	331	rVB	248633	351303	36.96%	4.893%
4	2.555	469	471	472	rBV2	1343	433	0.05%	0.006%
5	3.224	674	679	683	rBV8	2549	2035	0.21%	0.028%
6	3.793	847	856	883	rBV2	66540	248370	26.13%	3.460%
7	4.166	970	972	973	rBV2	2276	919	0.10%	0.013%
8	4.256	987	1000	1022	rBV	160676	403696	42.47%	5.623%
9	4.963	1205	1220	1240	rBV3	358849	950508	100.00%	13.240%
10	5.542	1387	1400	1422	rBV	279866	594911	62.59%	8.287%
11	5.844	1484	1494	1505	rBV2	61131	122365	12.87%	1.704%
12	5.995	1530	1541	1560	rBV	213586	429534	45.19%	5.983%
13	6.262	1622	1624	1625	rBV2	1619	690	0.07%	0.010%
14	6.542	1707	1711	1712	rBV5	1868	1215	0.13%	0.017%
15	6.844	1803	1805	1809	rBV4	1938	1377	0.14%	0.019%
16	6.921	1819	1829	1849	rBV2	100476	189502	19.94%	2.640%
17	7.249	1921	1931	1953	rBV	394650	698383	73.47%	9.728%
18	7.558	2019	2027	2042	rBV	74772	130172	13.69%	1.813%
19	8.031	2165	2174	2204	rBV	196134	392164	41.26%	5.463%
20	8.645	2363	2365	2367	rBV3	1452	742	0.08%	0.010%
21	8.793	2401	2411	2433	rBV	431901	707991	74.49%	9.862%
22	9.252	2551	2554	2559	rBV5	2071	2253	0.24%	0.031%
23	9.436	2609	2611	2612	rBV2	1463	696	0.07%	0.010%
24	10.092	2813	2815	2817	rBV3	1481	815	0.09%	0.011%
25	10.159	2825	2836	2858	rVB	274588	442765	46.58%	6.168%
26	10.268	2868	2870	2872	rBV3	1327	825	0.09%	0.011%
27	10.452	2923	2927	2929	rBV4	1798	1355	0.14%	0.019%
28	10.555	2956	2959	2960	rBV3	1453	729	0.08%	0.010%
29	10.596	2968	2972	2979	rVB10	1641	1867	0.20%	0.026%
30	10.625	2979	2981	2984	rBV4	1519	1191	0.13%	0.017%
31	10.690	2996	3001	3005	rBV8	1857	1740	0.18%	0.024%
32	10.776	3024	3028	3031	rBV6	1699	1256	0.13%	0.017%
33	10.825	3041	3043	3045	rBV2	1129	633	0.07%	0.009%
34	10.899	3061	3066	3071	rBV7	2099	2252	0.24%	0.031%
35	10.921	3071	3073	3076	rBV3	1776	1223	0.13%	0.017%
36	11.127	3135	3137	3138	rBV2	1198	554	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031143.D
 Acq On : 20 May 2023 06:48
 Operator : SY/MD
 Sample : 02865-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	11.191	3142	3157	3175	rBV	366932	593441	62.43%	8.266%
38	11.397	3219	3221	3225	rBV5	1260	885	0.09%	0.012%
39	11.468	3241	3243	3244	rBV2	1070	345	0.04%	0.005%
40	11.567	3264	3274	3294	rVB	384579	607153	63.88%	8.457%
41	11.760	3332	3334	3335	rBV2	811	331	0.03%	0.005%
42	11.776	3335	3339	3342	rBV6	2167	2035	0.21%	0.028%
43	11.911	3379	3381	3382	rBV2	811	275	0.03%	0.004%
44	11.989	3400	3405	3408	rBV7	2585	3104	0.33%	0.043%
45	12.018	3411	3414	3415	rBV3	976	675	0.07%	0.009%
46	12.120	3444	3446	3447	rBV2	745	270	0.03%	0.004%
47	12.249	3483	3486	3487	rBV3	1450	788	0.08%	0.011%
48	12.259	3487	3489	3492	rBV4	1274	813	0.09%	0.011%
49	12.368	3521	3523	3524	rBV2	1359	656	0.07%	0.009%
50	12.442	3543	3546	3550	rBV5	1076	879	0.09%	0.012%
51	12.484	3556	3559	3561	rBV4	1733	1167	0.12%	0.016%
52	12.571	3584	3586	3589	rBV4	1288	692	0.07%	0.010%
53	12.648	3608	3610	3612	rBV3	1185	526	0.06%	0.007%
54	12.802	3657	3658	3659	rBV	1311	407	0.04%	0.006%
55	12.934	3695	3699	3700	rBV4	1581	1044	0.11%	0.015%
56	12.963	3705	3708	3712	rBV5	2090	1517	0.16%	0.021%
57	14.085	4055	4057	4058	rBV2	2215	869	0.09%	0.012%
58	14.757	4262	4266	4267	rBV4	2483	1955	0.21%	0.027%




Sum of corrected areas: 7178997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031143.D
Acq On : 20 May 2023 06:48
Operator : SY/MD
Sample : 02865-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

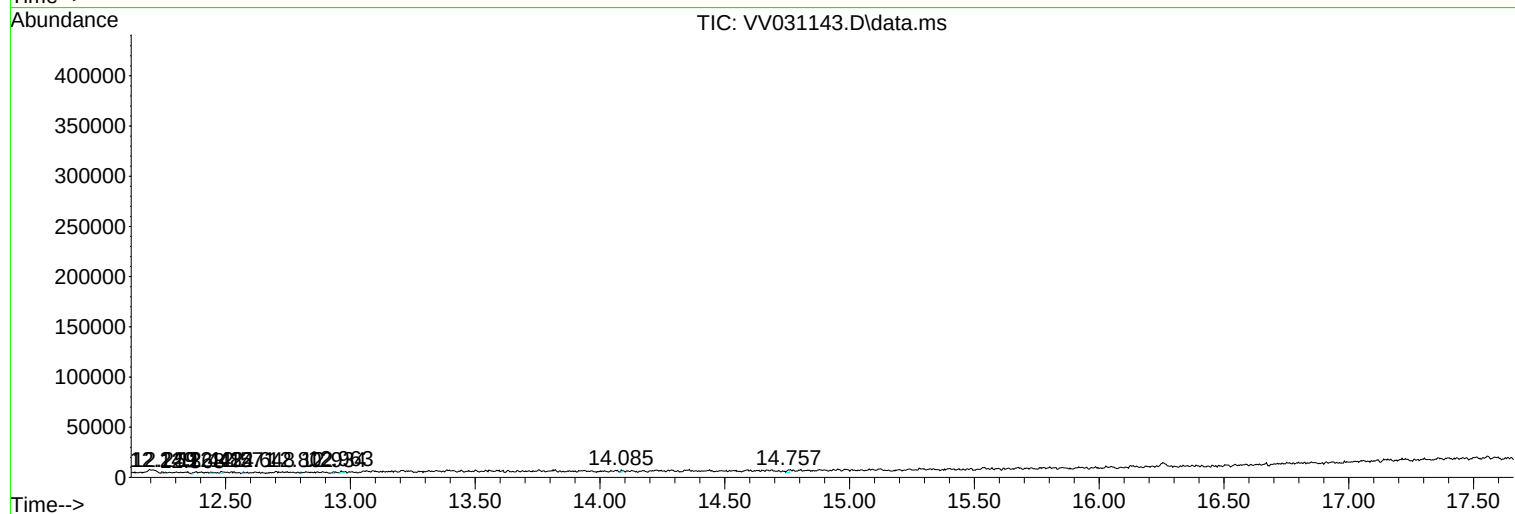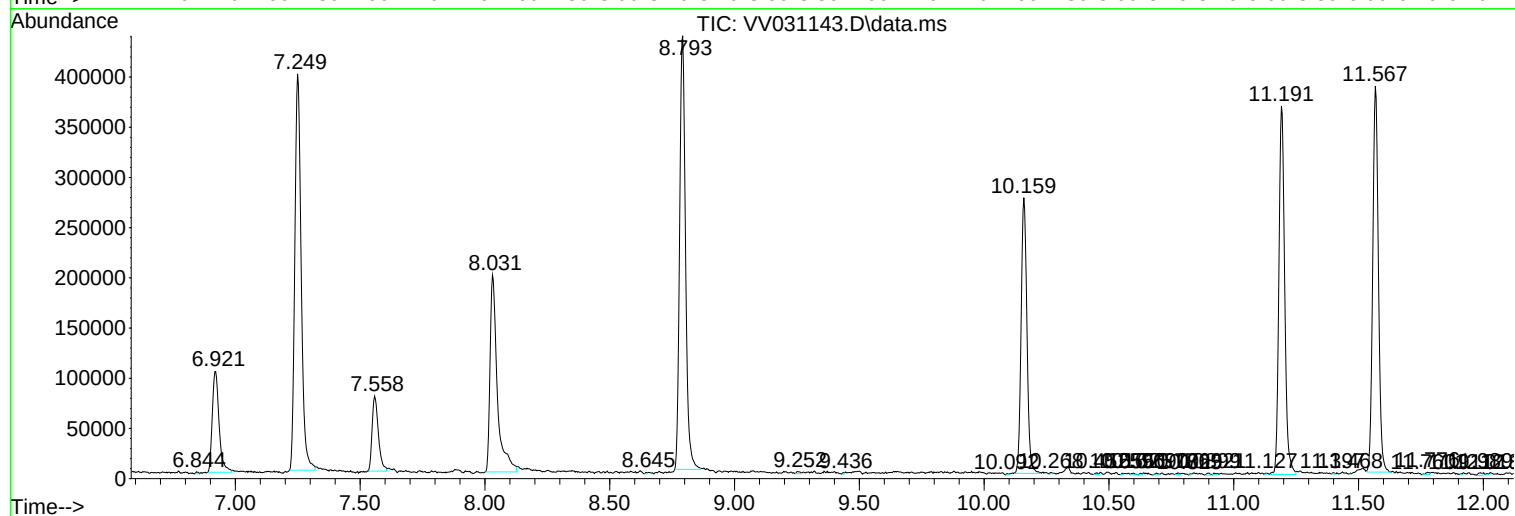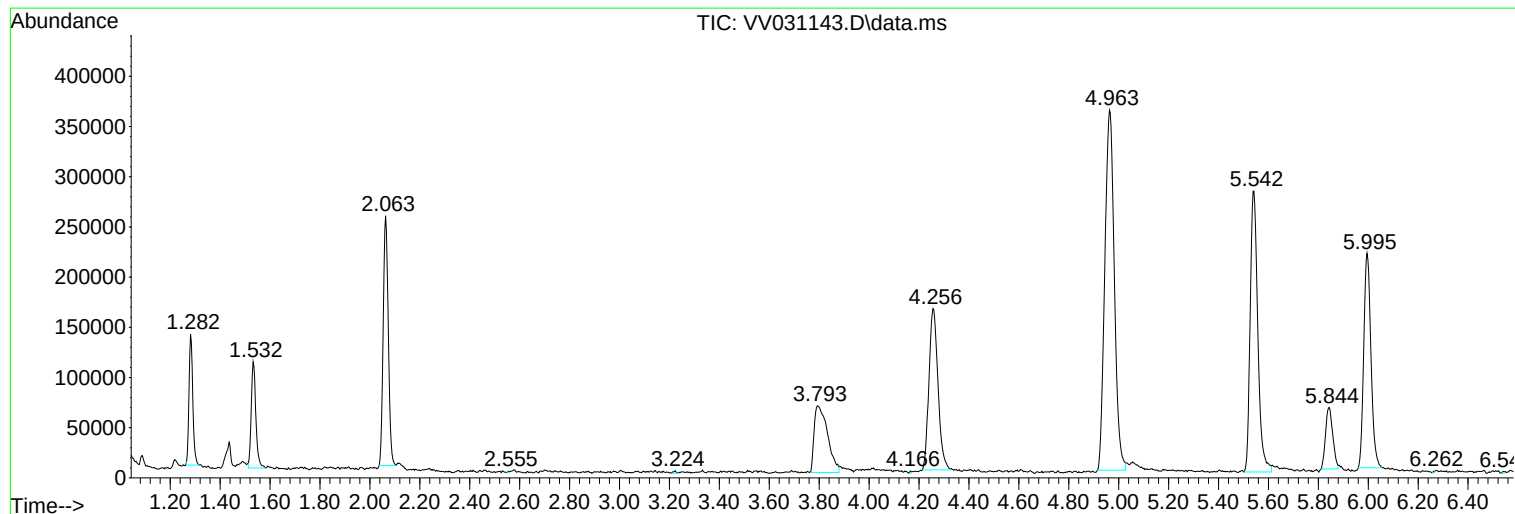

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031143.D
Acq On : 20 May 2023 06:48
Operator : SY/MD
Sample : 02865-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031143.D
Acq On : 20 May 2023 06:48
Operator : SY/MD
Sample : 02865-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------