

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031145.D
 Acq On : 20 May 2023 07:37
 Operator : SY/MD
 Sample : 02865-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	134113	150752	15.19%	2.020%
2	1.532	147	153	165	rVB	113822	135591	13.66%	1.817%
3	2.063	309	318	329	rBV	251413	358901	36.16%	4.809%
4	2.230	361	370	387	rBV2	40067	82921	8.35%	1.111%
5	2.574	471	477	481	rVV6	3927	4907	0.49%	0.066%
6	2.735	524	527	530	rVB4	1828	1076	0.11%	0.014%
7	2.751	530	532	535	rBV4	1605	988	0.10%	0.013%
8	2.802	545	548	552	rBV5	1324	1173	0.12%	0.016%
9	2.944	590	592	595	rBV3	2015	1243	0.13%	0.017%
10	3.005	609	611	615	rVB4	1697	1206	0.12%	0.016%
11	3.040	615	622	624	rBV7	2118	2007	0.20%	0.027%
12	3.079	632	634	636	rBV3	1436	917	0.09%	0.012%
13	3.185	660	667	670	rBV9	1666	1817	0.18%	0.024%
14	3.352	717	719	726	rVV8	1531	1447	0.15%	0.019%
15	3.468	752	755	762	rVB9	3134	3016	0.30%	0.040%
16	3.503	764	766	769	rVB4	1751	973	0.10%	0.013%
17	3.523	769	772	775	rBV5	1507	1008	0.10%	0.014%
18	3.629	802	805	806	rBV3	1732	1071	0.11%	0.014%
19	3.690	821	824	828	rBV6	2477	1798	0.18%	0.024%
20	3.722	831	834	836	rBV4	1665	1172	0.12%	0.016%
21	3.793	846	856	883	rVV	65606	182080	18.34%	2.440%
22	4.098	949	951	956	rVB6	2726	1752	0.18%	0.023%
23	4.137	959	963	966	rBV6	1703	1586	0.16%	0.021%
24	4.256	987	1000	1024	rVB2	164144	407037	41.01%	5.454%
25	4.510	1075	1079	1081	rBV5	2248	1341	0.14%	0.018%
26	4.831	1178	1179	1184	rVB4	1848	1015	0.10%	0.014%
27	4.870	1188	1191	1195	rVV6	1719	1281	0.13%	0.017%
28	4.963	1203	1220	1243	rBV2	372451	992628	100.00%	13.300%
29	5.191	1288	1291	1296	rBV6	1385	1289	0.13%	0.017%
30	5.461	1373	1375	1380	rVB6	1723	1046	0.11%	0.014%
31	5.542	1388	1400	1425	rBV	286294	597957	60.24%	8.012%
32	5.934	1516	1522	1524	rBV7	1840	1974	0.20%	0.026%
33	5.995	1530	1541	1559	rBV	221767	447504	45.08%	5.996%
34	6.288	1627	1632	1633	rBV4	2359	1352	0.14%	0.018%
35	6.445	1678	1681	1684	rBV4	2458	1737	0.17%	0.023%
36	6.513	1699	1702	1708	rVV7	1776	1981	0.20%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031145.D
 Acq On : 20 May 2023 07:37
 Operator : SY/MD
 Sample : 02865-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.580	1716	1723	1724	rBV7	1997	1923	0.19%	0.026%
38	6.799	1789	1791	1795	rBV5	2067	1736	0.17%	0.023%
39	6.921	1819	1829	1845	rVV	104883	190603	19.20%	2.554%
40	7.137	1891	1896	1898	rBV5	2426	2232	0.22%	0.030%
41	7.249	1917	1931	1949	rBV	409311	732003	73.74%	9.808%
42	7.558	2019	2027	2047	rBV	79275	134933	13.59%	1.808%
43	8.030	2164	2174	2205	rBV	203542	417092	42.02%	5.588%
44	8.493	2313	2318	2320	rBV6	1347	1338	0.13%	0.018%
45	8.513	2320	2324	2326	rVV5	1909	1423	0.14%	0.019%
46	8.526	2326	2328	2331	rVB4	1835	1044	0.11%	0.014%
47	8.686	2376	2378	2383	rBV6	1559	1186	0.12%	0.016%
48	8.792	2399	2411	2431	rBV	446792	746913	75.25%	10.008%
49	8.985	2469	2471	2474	rBV4	1636	1126	0.11%	0.015%
50	9.075	2496	2499	2500	rBV3	3514	1755	0.18%	0.024%
51	9.120	2511	2513	2518	rVB5	2929	1491	0.15%	0.020%
52	9.239	2547	2550	2554	rBV5	1425	1081	0.11%	0.014%
53	9.307	2568	2571	2573	rBV4	1844	1112	0.11%	0.015%
54	9.333	2576	2579	2582	rVV5	1814	1315	0.13%	0.018%
55	9.452	2612	2616	2619	rVB6	2168	1762	0.18%	0.024%
56	9.545	2643	2645	2649	rBV4	1688	1081	0.11%	0.014%
57	9.757	2708	2711	2715	rBV5	1604	999	0.10%	0.013%
58	9.873	2744	2747	2748	rBV2	2306	1320	0.13%	0.018%
59	9.921	2758	2762	2765	rBV6	1589	1400	0.14%	0.019%
60	9.947	2767	2770	2771	rBV3	1456	949	0.10%	0.013%
61	10.021	2790	2793	2797	rVB6	1910	1562	0.16%	0.021%
62	10.159	2826	2836	2852	rBV	301745	483425	48.70%	6.477%
63	10.432	2917	2921	2922	rBV4	1704	1033	0.10%	0.014%
64	10.509	2943	2945	2951	rVB7	2490	1590	0.16%	0.021%
65	10.638	2983	2985	2988	rBV4	1735	1197	0.12%	0.016%
66	10.689	2997	3001	3002	rBV3	1692	1222	0.12%	0.016%
67	10.734	3013	3015	3019	rVB4	1917	1025	0.10%	0.014%
68	10.770	3019	3026	3027	rBV7	1768	2256	0.23%	0.030%
69	10.831	3043	3045	3048	rBV4	1830	1397	0.14%	0.019%
70	10.921	3071	3073	3075	rBV3	2081	1245	0.13%	0.017%
71	11.037	3105	3109	3114	rVB7	1555	1611	0.16%	0.022%
72	11.191	3145	3157	3176	rVV	406344	637938	64.27%	8.547%
73	11.426	3228	3230	3232	rVV3	2539	1079	0.11%	0.014%
74	11.567	3264	3274	3289	rBV	414402	645337	65.01%	8.647%
75	11.783	3336	3341	3342	rBV5	1805	1367	0.14%	0.018%
76	11.921	3381	3384	3387	rVB5	2023	1033	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
 Data File : VV031145.D
 Acq On : 20 May 2023 07:37
 Operator : SY/MD
 Sample : 02865-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.168	3458	3461	3466	rBV7	3087	2593	0.26%	0.035%
78	12.194	3466	3469	3470	rBV3	1883	989	0.10%	0.013%
79	12.320	3505	3508	3510	rBV4	2352	1443	0.15%	0.019%
80	12.403	3529	3534	3535	rBV4	1696	1398	0.14%	0.019%
81	12.574	3585	3587	3594	rVB7	1700	1386	0.14%	0.019%
82	12.615	3598	3600	3604	rBV4	1620	1209	0.12%	0.016%
83	12.815	3660	3662	3666	rBV4	1600	1081	0.11%	0.014%
84	12.969	3707	3710	3713	rBV5	1651	1417	0.14%	0.019%
85	13.001	3719	3720	3724	rBV3	1339	936	0.09%	0.013%
86	13.043	3729	3733	3736	rBV5	1744	1793	0.18%	0.024%
87	13.091	3745	3748	3750	rBV4	1832	993	0.10%	0.013%
88	13.168	3767	3772	3774	rBV5	1669	1070	0.11%	0.014%
89	13.213	3783	3786	3793	rVB9	2222	2340	0.24%	0.031%
90	13.287	3805	3809	3810	rBV4	1888	1152	0.12%	0.015%
91	13.448	3855	3859	3862	rBV5	2040	1838	0.19%	0.025%
92	13.561	3891	3894	3900	rVB7	1867	1382	0.14%	0.019%
93	13.686	3930	3933	3936	rVV5	2277	1567	0.16%	0.021%
94	13.914	4000	4004	4006	rBV4	1926	1309	0.13%	0.018%
95	14.104	4058	4063	4066	rBV7	2285	2112	0.21%	0.028%
96	14.120	4066	4068	4070	rVB3	2127	995	0.10%	0.013%
97	14.374	4144	4147	4149	rBV4	1663	966	0.10%	0.013%
98	14.477	4177	4179	4183	rVB5	1778	1124	0.11%	0.015%
99	14.538	4195	4198	4200	rBV4	1773	996	0.10%	0.013%
100	15.573	4518	4520	4523	rBV4	2231	1696	0.17%	0.023%




Sum of corrected areas: 7463463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031145.D
Acq On : 20 May 2023 07:37
Operator : SY/MD
Sample : 02865-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

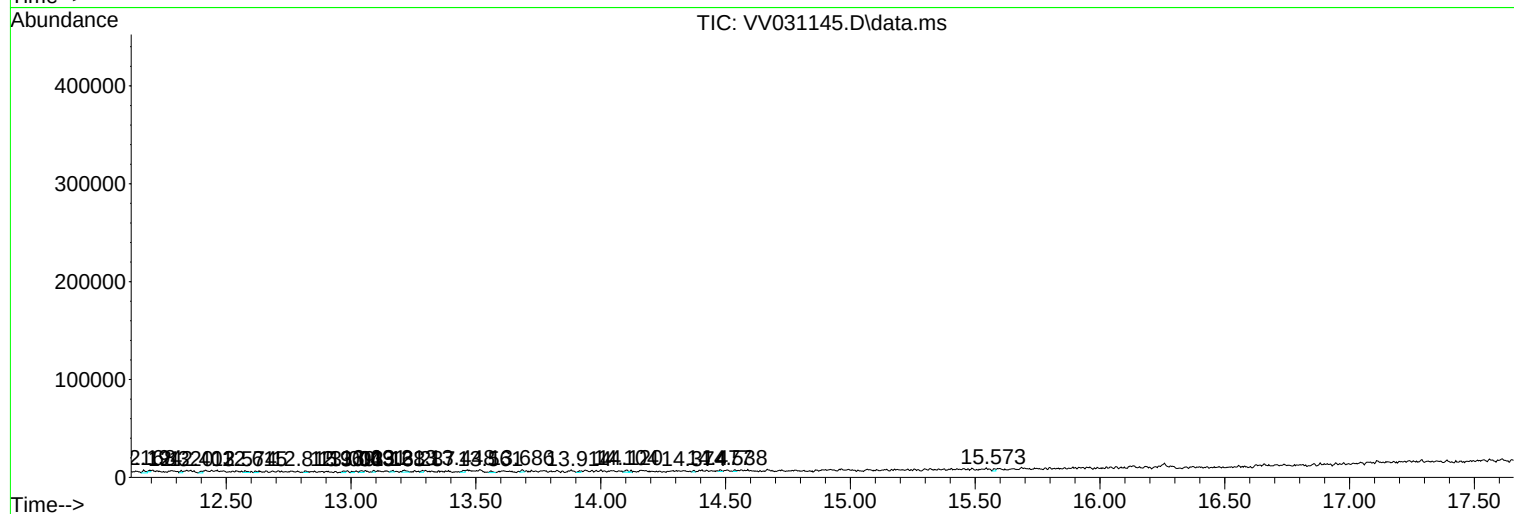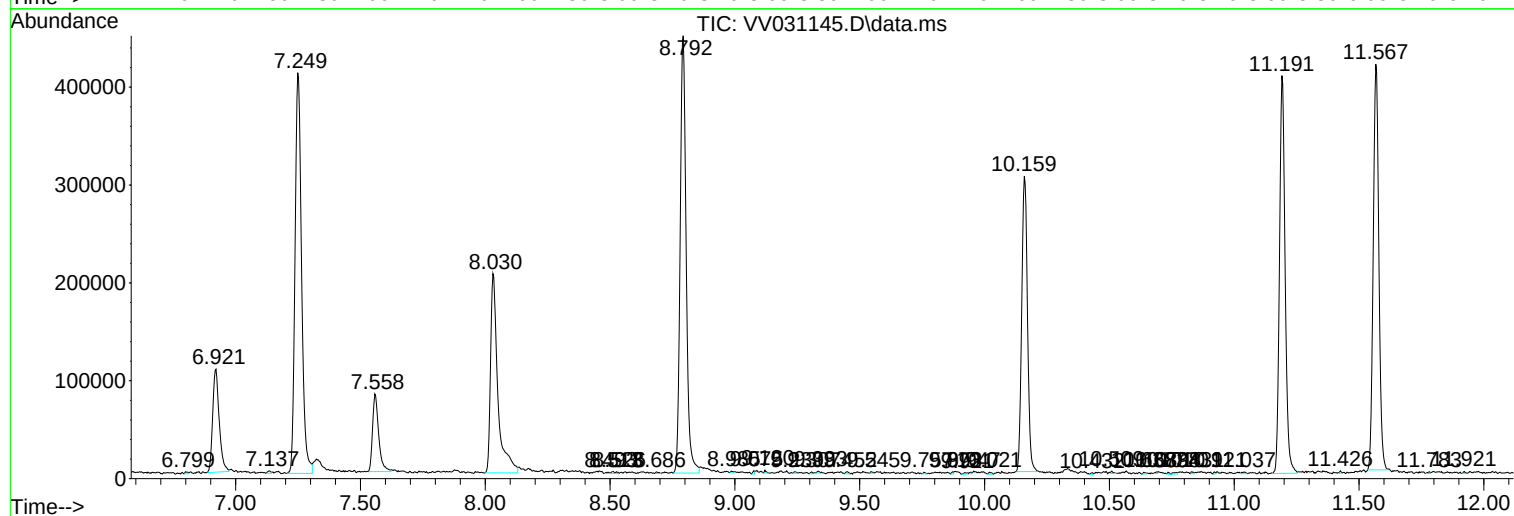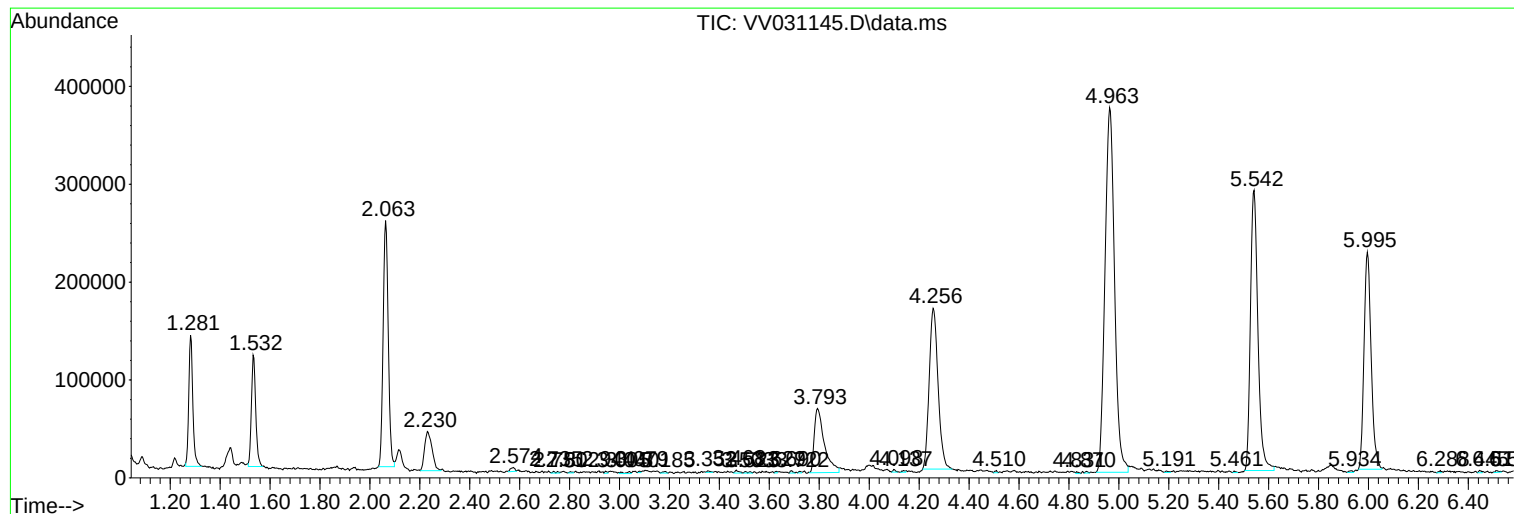

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031145.D
Acq On : 20 May 2023 07:37
Operator : SY/MD
Sample : 02865-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031145.D
Acq On : 20 May 2023 07:37
Operator : SY/MD
Sample : 02865-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------