
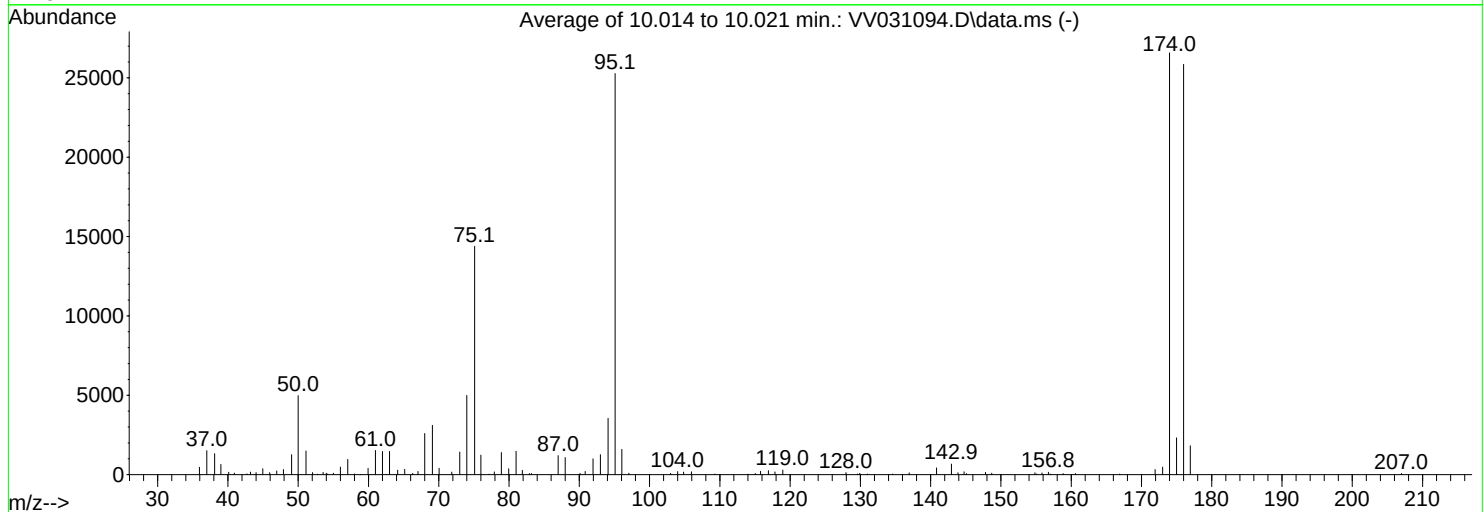


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051923\
Data File : VV031094.D
Acq On : 19 May 2023 08:58
Operator : SY/MD
Sample : BFB376
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB376

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis
Last Update : Thu May 25 01:11:46 2023

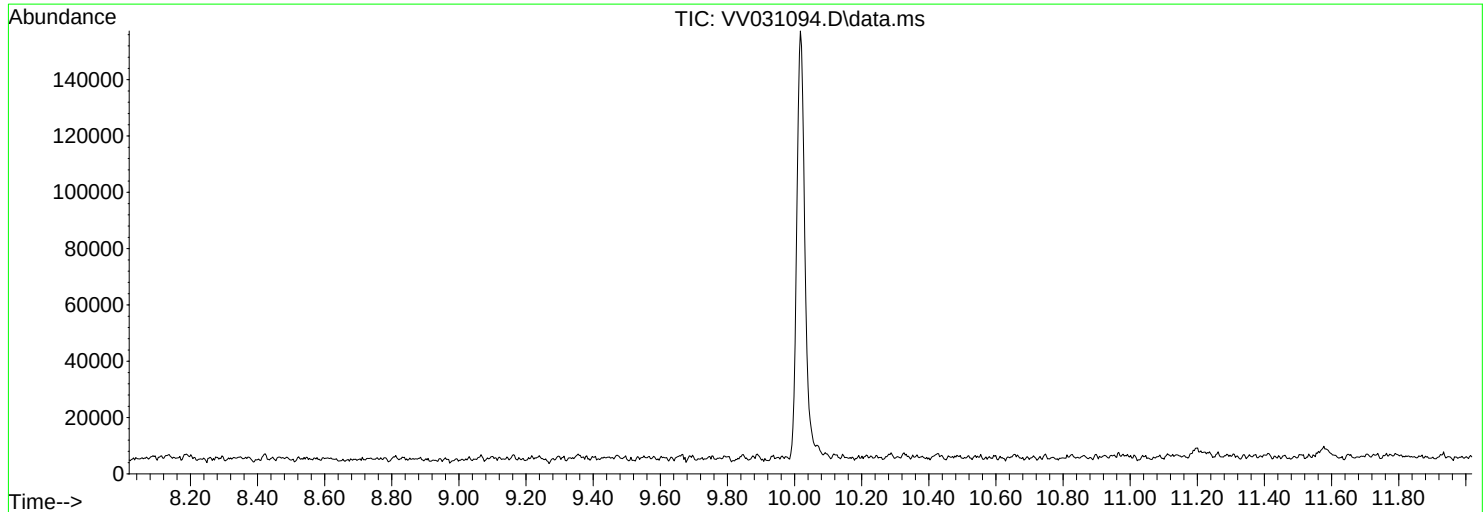

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4983	PASS
75	95	30	80	56.9	14383	PASS
95	95	100	100	100.0	25275	PASS
96	95	5	9	6.3	1593	PASS
173	174	0.00	2	1.8	478	PASS
174	95	50	120	105.1	26573	PASS
175	174	5	9	8.7	2316	PASS
176	174	95	105	97.3	25845	PASS
177	176	5	10	7.0	1815	PASS

m/z	Abundance
35.10	242.0
36.20	172.0
37.20	148.0
37.80	212.0
38.50	147.0
39.30	191.0
39.90	271.0
41.20	142.0
41.70	131.0
42.50	169.0
44.00	334.0
47.10	118.0
48.50	166.0
50.00	137.0
50.70	188.0
52.40	125.0
52.90	108.0
54.90	127.0
56.00	123.0
56.80	102.0
58.10	106.0
58.90	105.0
59.50	102.0
60.40	141.0
61.40	156.0
63.50	155.0
64.60	114.0
70.90	126.0
71.80	104.0
75.10	114.0
77.20	151.0
81.10	127.0
85.00	175.0
85.70	130.0
91.20	106.0
93.10	115.0
105.30	111.0
110.70	105.0
131.30	104.0
161.00	102.0
211.30	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
36.00	449.0
37.00	1632.0
38.10	1322.0
39.00	614.0
39.90	209.0
41.30	132.0
42.50	191.0
43.20	187.0
44.10	425.0
45.00	327.0
46.00	116.0
47.00	371.0
47.90	283.0
49.10	1315.0
50.10	5312.0
51.10	1514.0
52.10	141.0
52.80	102.0
53.50	123.0
54.00	146.0
55.10	210.0
56.00	555.0
57.00	909.0
58.00	187.0
58.90	113.0
59.90	333.0
61.00	1521.0
62.00	1482.0
63.00	1453.0
64.20	285.0
65.20	270.0
66.30	116.0
67.00	183.0
68.00	2648.0
69.10	3093.0
70.00	369.0
72.00	295.0
73.00	1312.0
74.00	4809.0
75.10	14015.0
76.00	1319.0
77.20	170.0
78.00	115.0
78.90	1404.0
79.90	360.0
81.00	1685.0
81.90	254.0
83.00	104.0
85.80	141.0
87.00	1143.0
88.00	1038.0
90.80	176.0
92.00	972.0
93.00	1349.0
94.10	3510.0
95.10	25040.0
96.10	1662.0
97.10	143.0
104.00	180.0
104.80	164.0
106.00	180.0
114.00	100.0
115.80	213.0
116.90	283.0
117.90	133.0
118.90	286.0
128.00	128.0
129.60	119.0
131.00	116.0
134.60	108.0
137.00	121.0
140.80	359.0
142.90	704.0
143.90	114.0
145.10	184.0
147.80	135.0
154.90	124.0
155.80	107.0
156.70	262.0
158.90	107.0
171.90	298.0
173.00	532.0
174.00	25800.0
175.00	2125.0
176.00	24672.0
176.90	1703.0
207.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
36.00	468.0
37.00	1697.0
38.10	1338.0
39.00	666.0
40.10	207.0
40.90	138.0
41.90	143.0
42.50	153.0
43.20	159.0
44.00	467.0
44.90	368.0
46.00	129.0
46.90	345.0
47.90	323.0
49.10	1252.0
50.10	5277.0
51.10	1545.0
52.00	132.0
52.70	142.0
53.60	151.0
54.00	135.0
55.10	215.0
56.00	622.0
57.10	992.0
58.00	141.0
58.90	122.0
60.00	397.0
61.00	1557.0
62.00	1506.0
63.00	1453.0
64.10	297.0
65.10	336.0
66.30	130.0
67.00	213.0
68.00	2630.0
69.10	3207.0
70.00	441.0
72.00	261.0
73.00	1470.0
74.00	5134.0
75.10	15101.0
76.00	1271.0
77.20	182.0
77.90	159.0
78.90	1413.0
80.00	386.0
81.00	1716.0
81.90	279.0
83.20	104.0
85.80	116.0
87.00	1230.0
88.00	1098.0
90.10	126.0
90.90	209.0
92.00	995.0
93.00	1436.0
94.10	3679.0
95.10	25840.0
96.00	1646.0
97.00	128.0
103.00	121.0
104.00	188.0
104.80	163.0
106.00	180.0
115.00	107.0
115.80	214.0
116.90	243.0
117.90	175.0
119.00	306.0
128.00	136.0
129.90	110.0
136.90	110.0
140.90	436.0
142.90	700.0
143.90	120.0
144.80	245.0
147.80	157.0
148.70	141.0
154.90	125.0
155.90	118.0
156.80	199.0
158.80	106.0
160.60	106.0
172.00	329.0
173.00	491.0
174.00	27376.0
175.00	2405.0
176.00	26680.0
177.00	1917.0
207.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
35.90	468.0
37.00	1656.0
38.10	1296.0
39.00	662.0
40.10	239.0
40.90	174.0
41.90	173.0
42.70	151.0
43.20	142.0
44.00	517.0
44.90	412.0
45.90	150.0
46.90	323.0
47.90	367.0
49.00	1202.0
50.00	4771.0
51.10	1429.0
52.00	115.0
52.60	159.0
53.60	161.0
54.20	112.0
55.10	224.0
56.00	616.0
57.10	957.0
58.10	100.0
58.90	143.0
60.00	439.0
61.00	1478.0
62.00	1383.0
63.00	1468.0
64.10	270.0
65.10	389.0
67.10	202.0
68.00	2501.0
69.10	3017.0
70.10	395.0
71.90	232.0
73.00	1470.0
74.00	5036.0
75.10	14375.0
76.00	1114.0
77.00	184.0
77.80	231.0
78.90	1352.0
80.00	384.0
81.00	1411.0
81.90	298.0
82.80	120.0
83.20	106.0
85.80	110.0
87.00	1224.0
88.00	1088.0
90.10	112.0
90.90	229.0
91.90	1027.0
93.00	1339.0
94.10	3443.0
95.10	24944.0
96.10	1470.0
103.00	122.0
104.00	201.0
104.90	144.0
105.90	199.0
109.30	120.0
115.10	115.0
115.80	210.0
116.90	234.0
117.80	193.0
119.00	289.0
127.80	143.0
129.90	139.0
137.00	103.0
140.90	467.0
143.00	589.0
143.90	126.0
144.70	291.0
147.80	128.0
148.70	140.0
154.80	108.0
155.10	110.0
155.90	101.0
157.00	118.0
160.60	117.0
166.90	109.0
172.00	336.0
173.00	412.0
174.00	26544.0
175.00	2417.0
176.00	26184.0
177.00	1824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376