


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
Data File : VV016136.D
Acq On : 20 May 2020 17:02
Operator : SY/MD
Sample : L2725-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9B17

Manual Integrations
APPROVED

apatel
5/22/2020 11:27:23 AM

Quant Time: May 21 03:54:16 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 21 01:36:12 2020
Response via : Initial Calibration

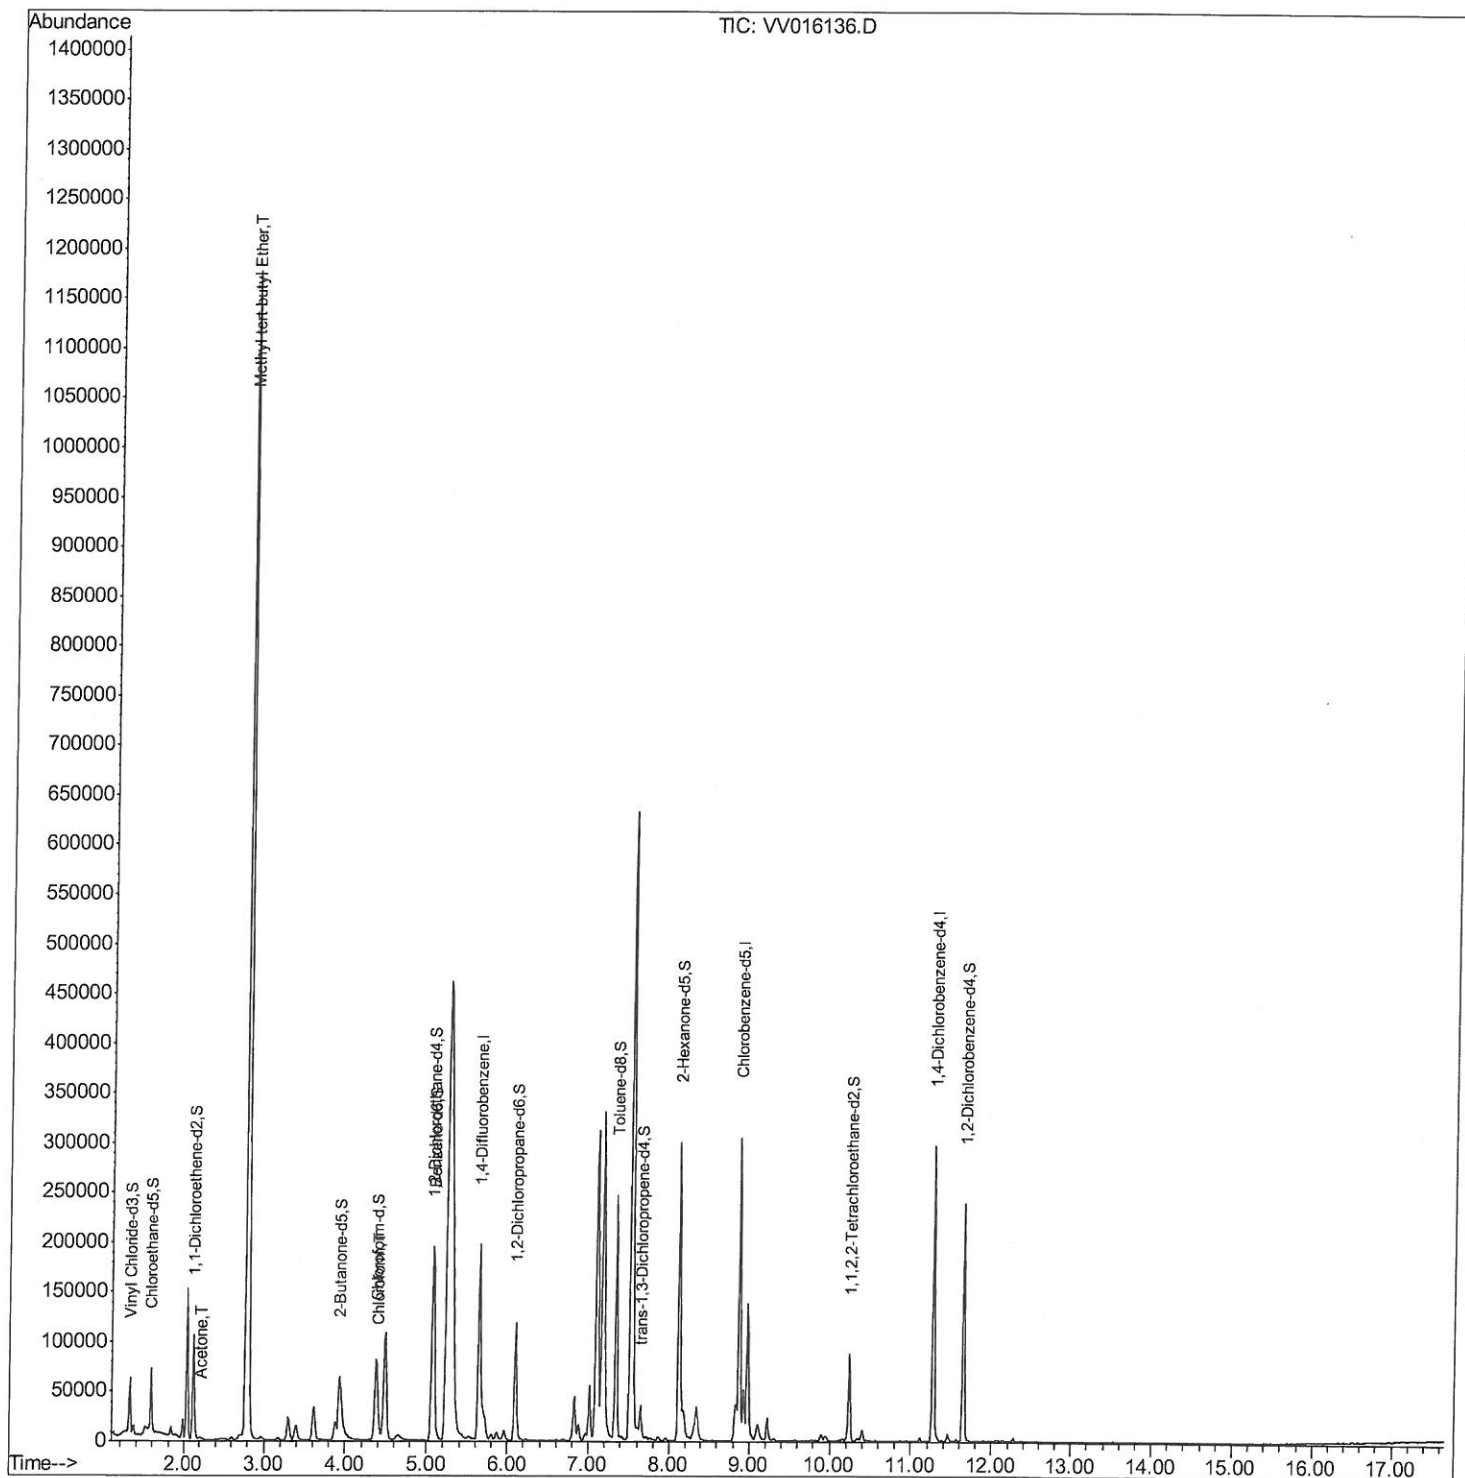

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
 Data File : VV016136.D
 Acq On : 20 May 2020 17:02
 Operator : SY/MD
 Sample : L2725-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 F9B17

Manual Integrations
APPROVED

apatel
 5/22/2020 11:27:23 AM

Quant Time: May 21 01:42:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:36:12 2020
 Response via : Initial Calibration

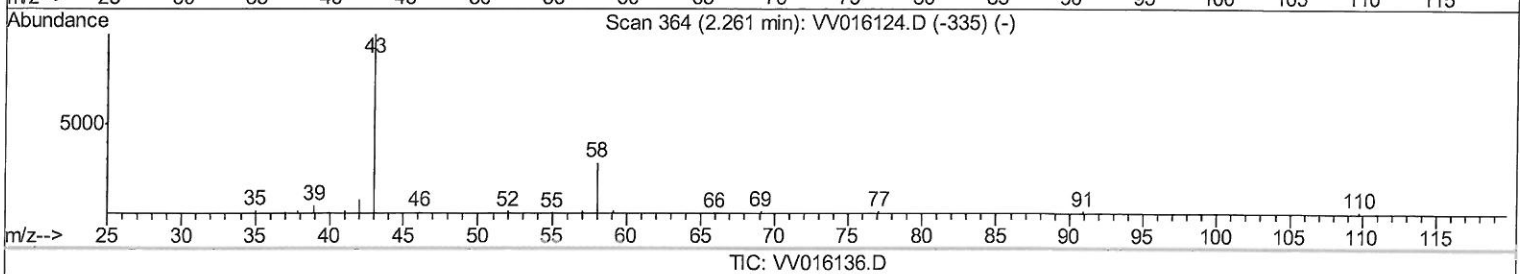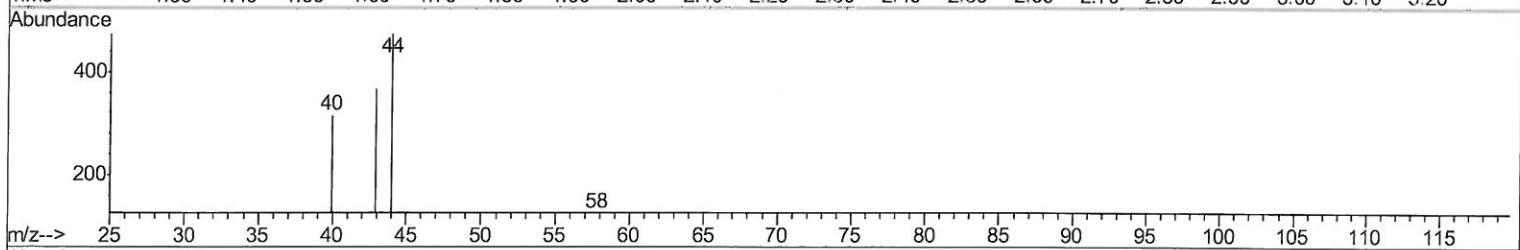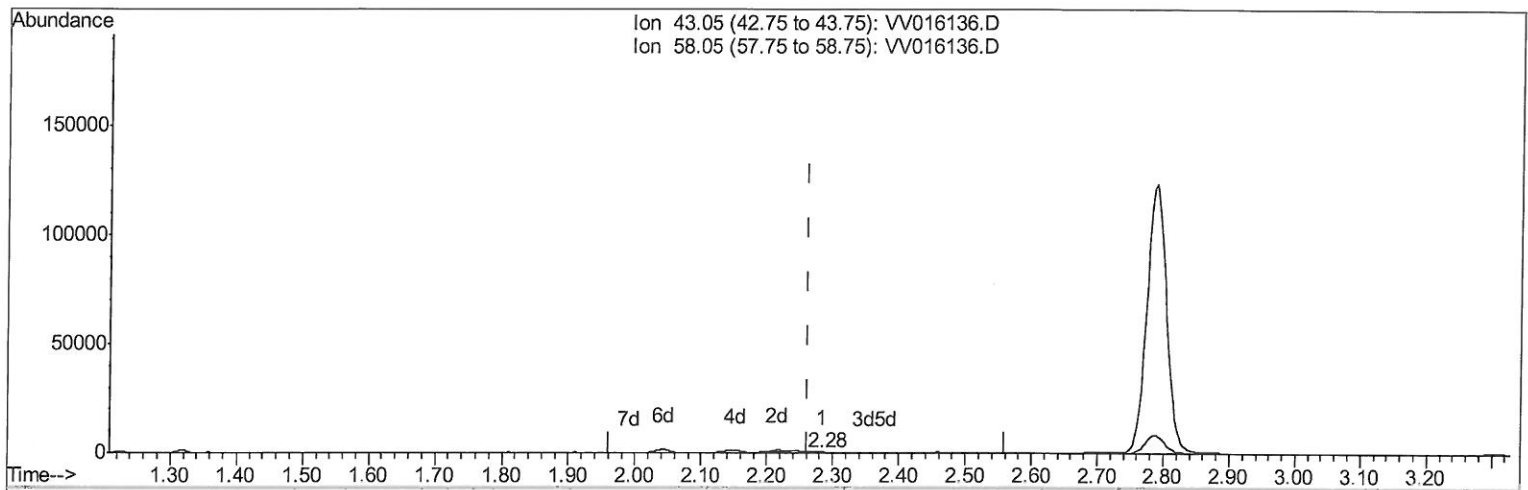

TIC: VV016136.D

(13) Acetone (T)

2.283min (+0.023) 0.22ug/L

response 358

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	19.83
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
 Data File : VV016136.D
 Acq On : 20 May 2020 17:02
 Operator : SY/MD
 Sample : L2725-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B17

Manual Integrations
 APPROVED

apatel
 5/22/2020 11:27:23 AM

Quant Time: May 21 01:42:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:36:12 2020
 Response via : Initial Calibration

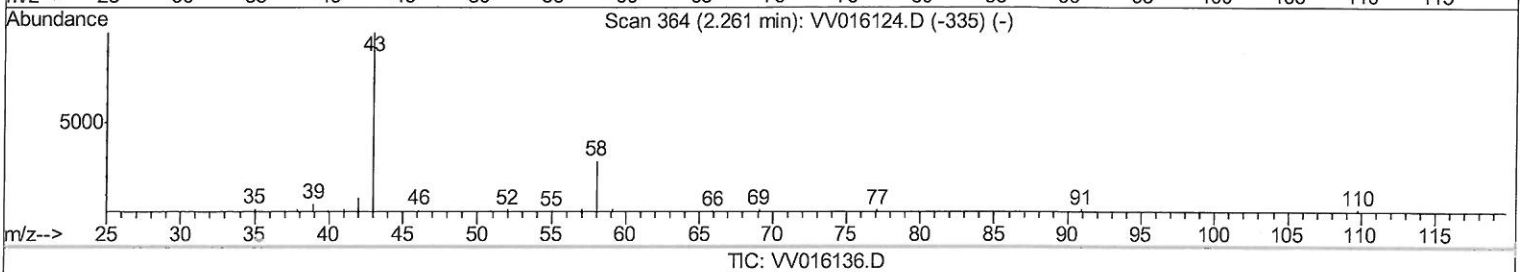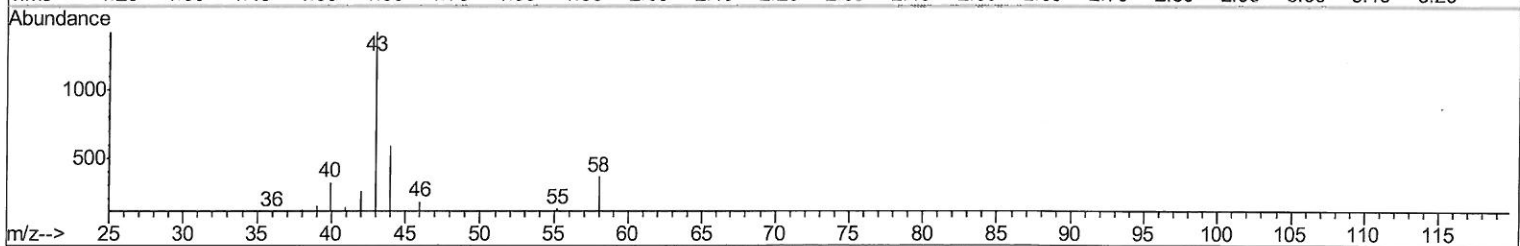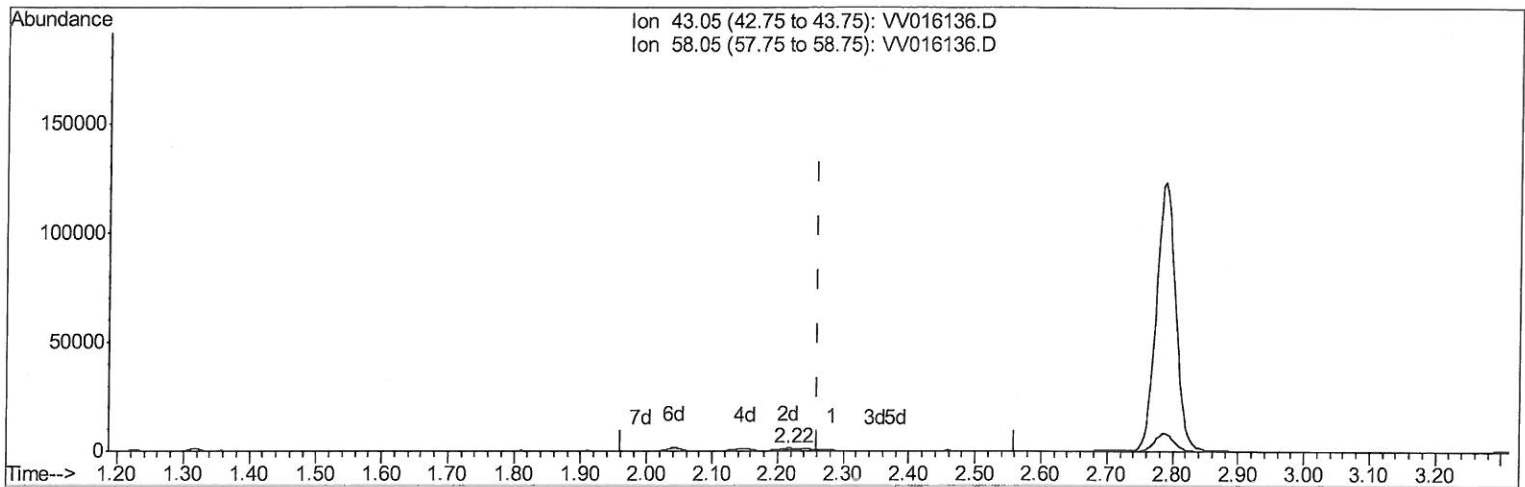

(13) Acetone (T)

2.216min (-0.045) 2.84ug/L m

response 4578

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	1.55
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
5/28/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
 Data File : VV016136.D
 Acq On : 20 May 2020 17:02
 Operator : SY/MD
 Sample : L2725-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B17

Manual Integrations
 APPROVED

apatel
 5/22/2020 11:27:23 AM

Quant Time: May 21 03:54:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:36:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	158045	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	150735	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	69488	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31333	3.65	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	73.00%		
7) Chloroethane-d5	1.58	69	36772	4.53	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	90.60%		
11) 1,1-Dichloroethene-d2	2.13	63	57792	3.13	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	62.60%		
20) 2-Butanone-d5	3.93	46	130335	53.29	ug/L	-0.06
Spiked Amount 50.000	Range 40 - 130		Recovery =	106.58%		
24) Chloroform-d	4.38	84	79042	4.22	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.40%		
26) 1,2-Dichloroethane-d4	5.06	65	48987	4.56	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	91.20%		
32) Benzene-d6	5.08	84	164100	4.57	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.40%		
36) 1,2-Dichloropropane-d6	6.10	67	54281	4.96	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	99.20%		
41) Toluene-d8	7.34	98	150980	4.45	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.00%		
45) trans-1,3-Dichloropropene-	7.65	79	17948	4.18	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.60%		
48) 2-Hexanone-d5	8.11	63	102798	54.46	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	108.92%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	39512	5.13	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	102.60%		
65) 1,2-Dichlorobenzene-d4	11.65	152	56210	4.98	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	99.60%		

Target Compounds

					Ovalue
13) Acetone	2.22	43	4578m	2.838	ug/L
17) Methyl tert-butyl Ether	2.79	73	1135597	50.247	ug/L
25) Chloroform	4.41	83	11439	0.561	ug/L

MO
 5/28/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed