

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
 Data File : VV016139.D
 Acq On : 20 May 2020 18:11
 Operator : SY/MD
 Sample : L2725-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B20

Quant Time: May 21 05:12:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:36:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	140186	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	139604	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	65236	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	33669	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.58	69	37652	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.13	63	59736	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	3.93	46	133142	61.37	ug/L	-0.06
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.74%
24) Chloroform-d	4.38	84	92149	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.80%
26) 1,2-Dichloroethane-d4	5.06	65	51055	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.20%
32) Benzene-d6	5.08	84	169513	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.10	67	54810	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.34	98	148801	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
45) trans-1,3-Dichloropropene-	7.65	79	16748	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
48) 2-Hexanone-d5	8.12	63	105464	60.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.66%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	41609	5.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	59164	5.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	3772	2.636 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052020\
Data File : VV016139.D
Acq On : 20 May 2020 18:11
Operator : SY/MD
Sample : L2725-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9B20

Quant Time: May 21 05:12:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 21 01:36:12 2020
Response via : Initial Calibration

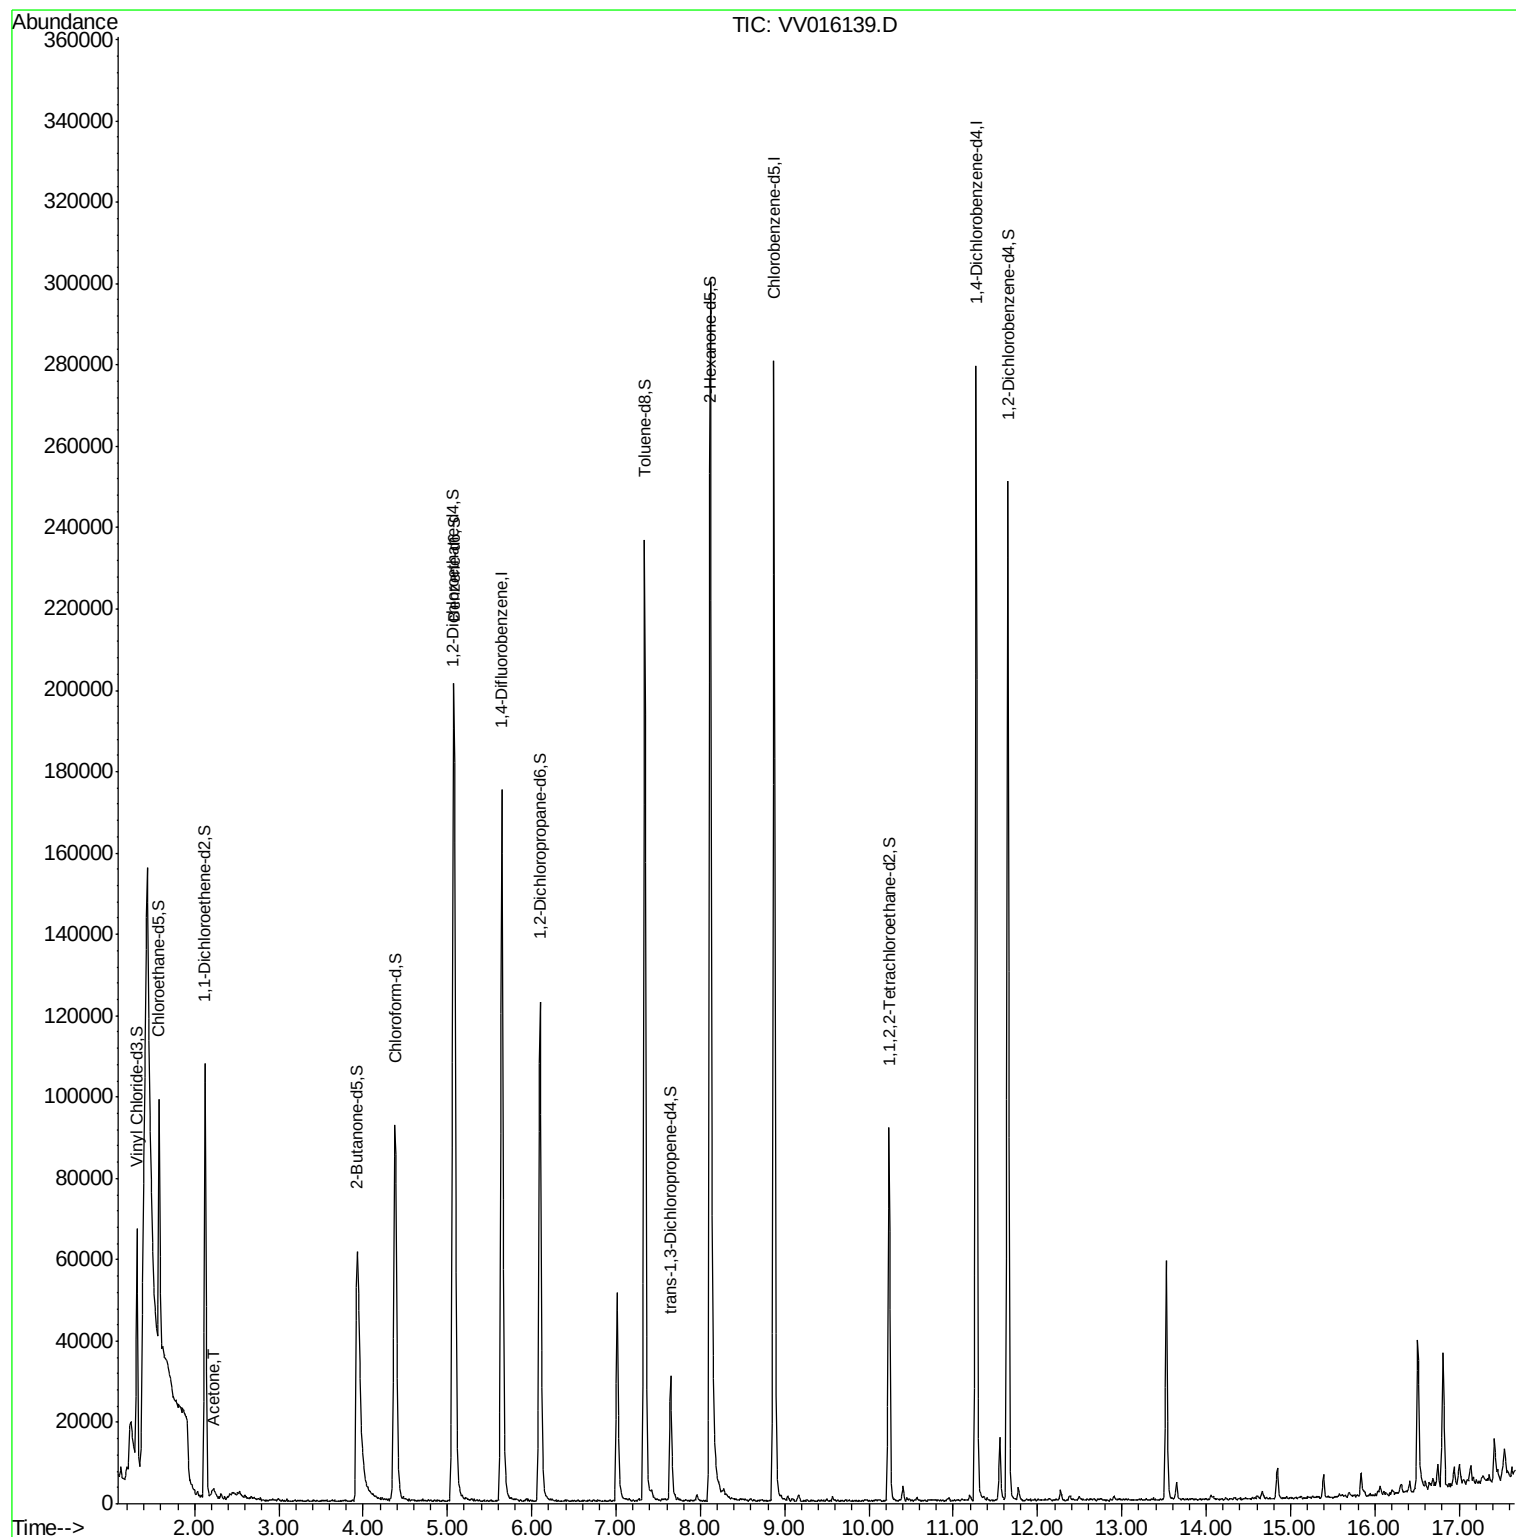

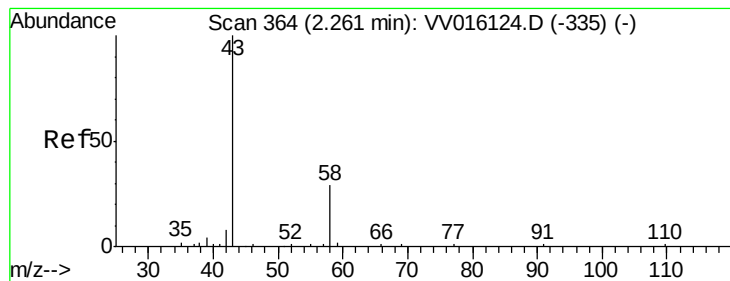

#13

Acetone

Concen: 2.636 ug/L

RT: 2.23 min Scan# 353

Delta R.T. -0.04 min

Lab File: VV016139.D

Acq: 20 May 2020 18:11

Instrument :
MSVOA_V
ClientSampleId :
F9B20

Tot Ion: 43 Resp: 3772

Ion Ratio Lower Upper

43 100

58 17.1 0.0 30.8

