

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052020\
 Data File : VV016142.D
 Acq On : 20 May 2020 19:20
 Operator : SY/MD
 Sample : L2725-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B28

Quant Time: May 21 05:32:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:36:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	157350	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	152489	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	74932	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34330	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.58	69	37089	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.60%
11) 1,1-Dichloroethene-d2	2.13	63	59008	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.91	46	137432	56.44	ug/L	-0.08
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.88%
24) Chloroform-d	4.38	84	87387	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.06	65	50101	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.08	84	174663	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.10	67	56121	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.34	98	154260	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
45) trans-1,3-Dichloropropene-	7.65	79	15155	3.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.80%
48) 2-Hexanone-d5	8.11	63	114559	59.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.98%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	42044	5.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	60843	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
25) Chloroform	4.41	83	5809	0.286 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052020\
Data File : VV016142.D
Acq On : 20 May 2020 19:20
Operator : SY/MD
Sample : L2725-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9B28

Quant Time: May 21 05:32:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 21 01:36:12 2020
Response via : Initial Calibration



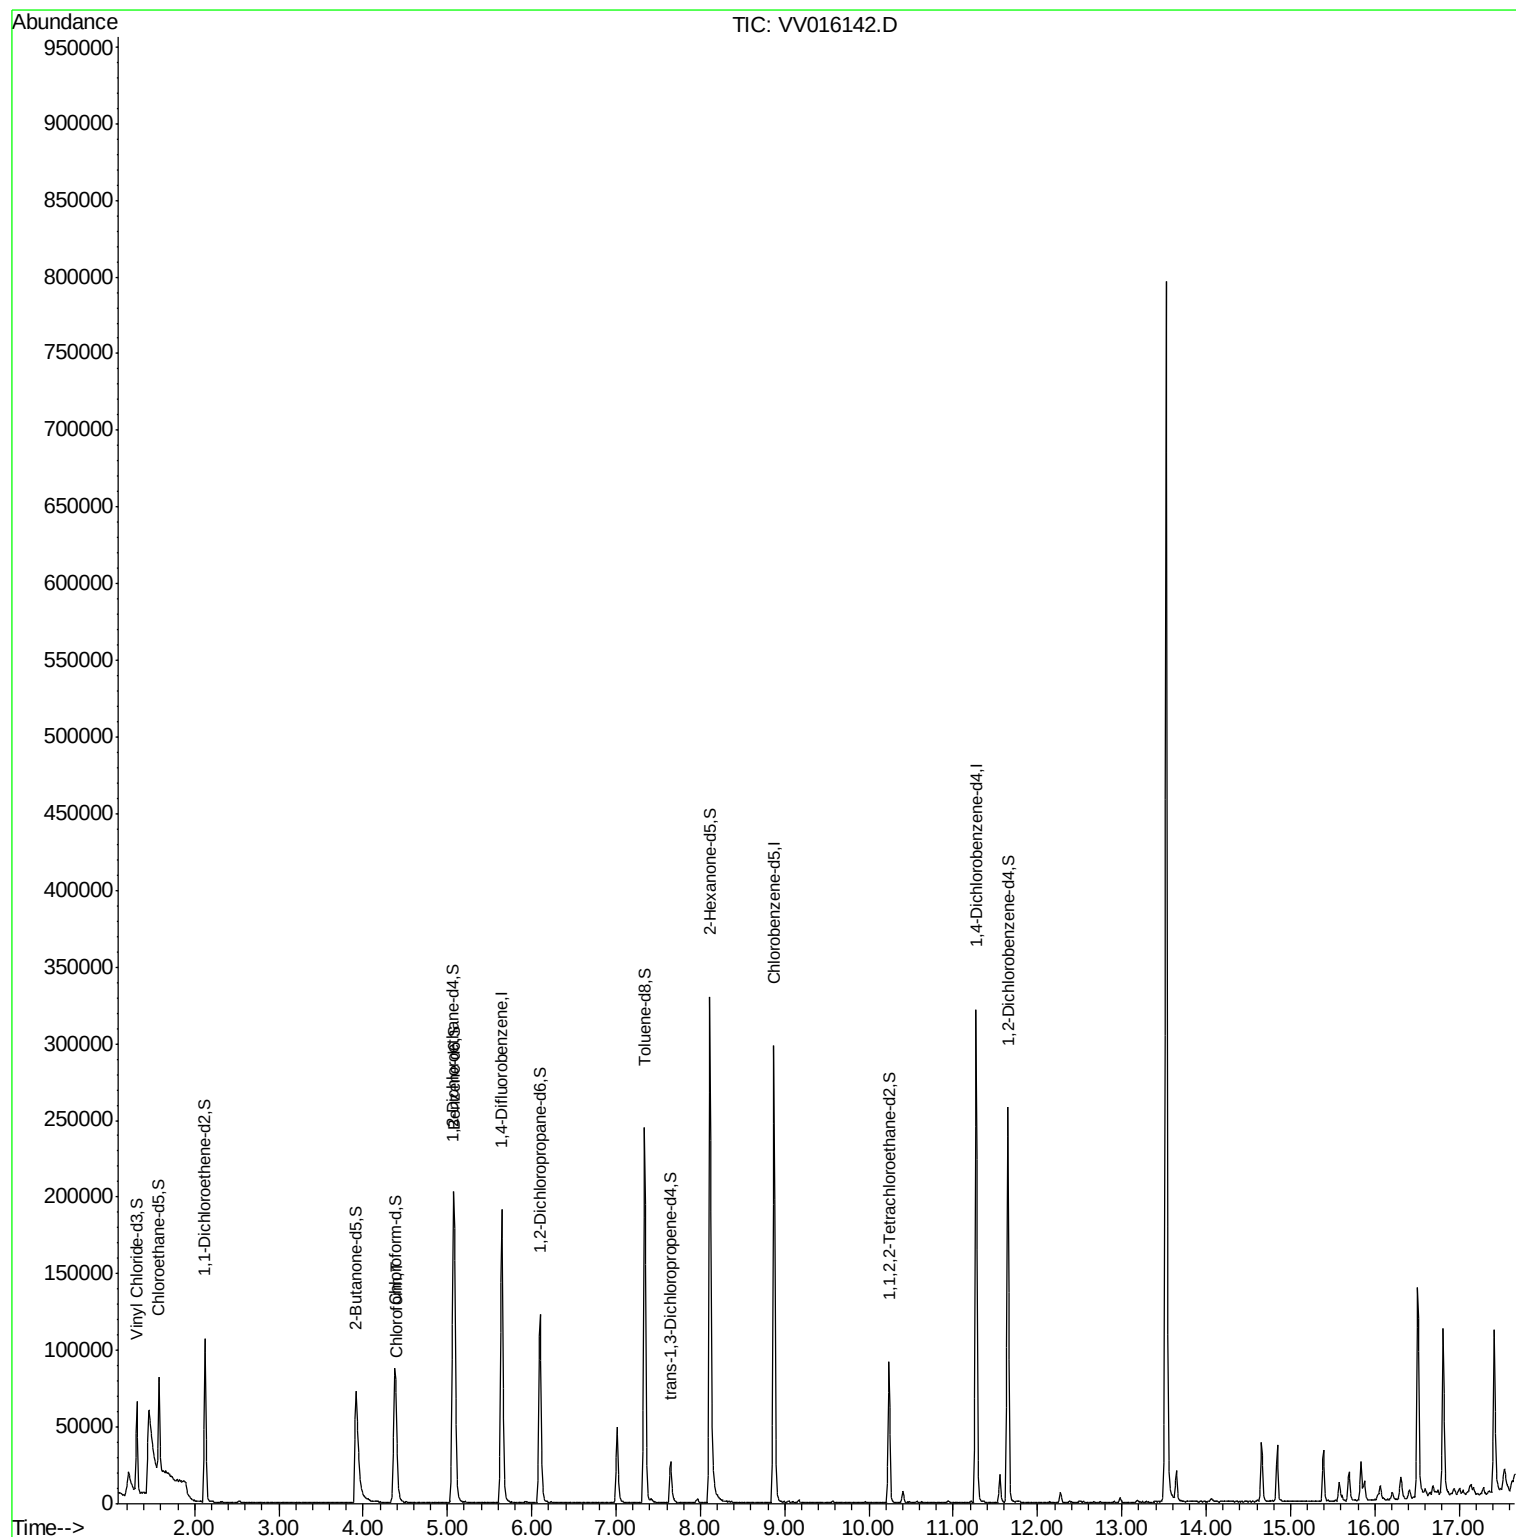


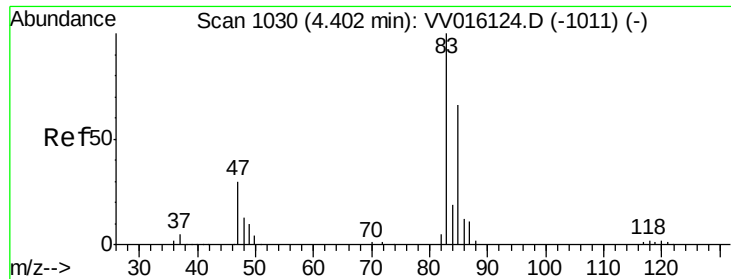

#25
 Chloroform
 Concen: 0.286 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.00 min
 Lab File: VV016142.D
 Acq: 20 May 2020 19:20

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B28

Tot Ion: 83 Resp: 5809
 Ion Ratio Lower Upper
 83 100
 85 60.5 45.7 84.9

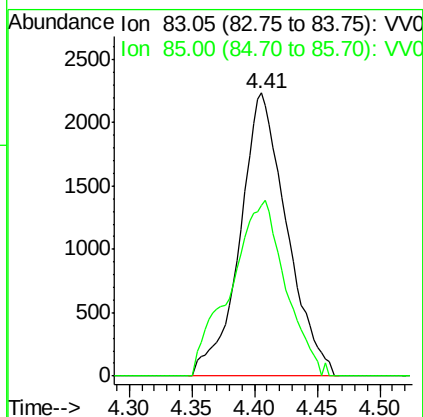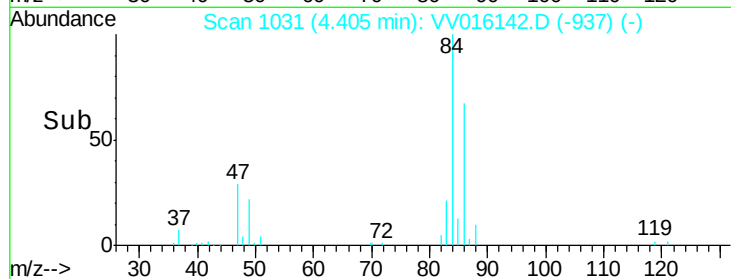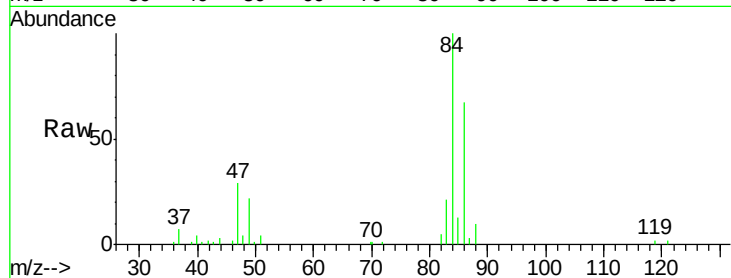

Instrument :

MSVOA_V

ClientSampleId :

F9B28