


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052020\
 Data File : VV016123.D
 Acq On : 20 May 2020 09:25
 Operator : SY/MD
 Sample : BFB60
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB60

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 21 01:36:12 2020

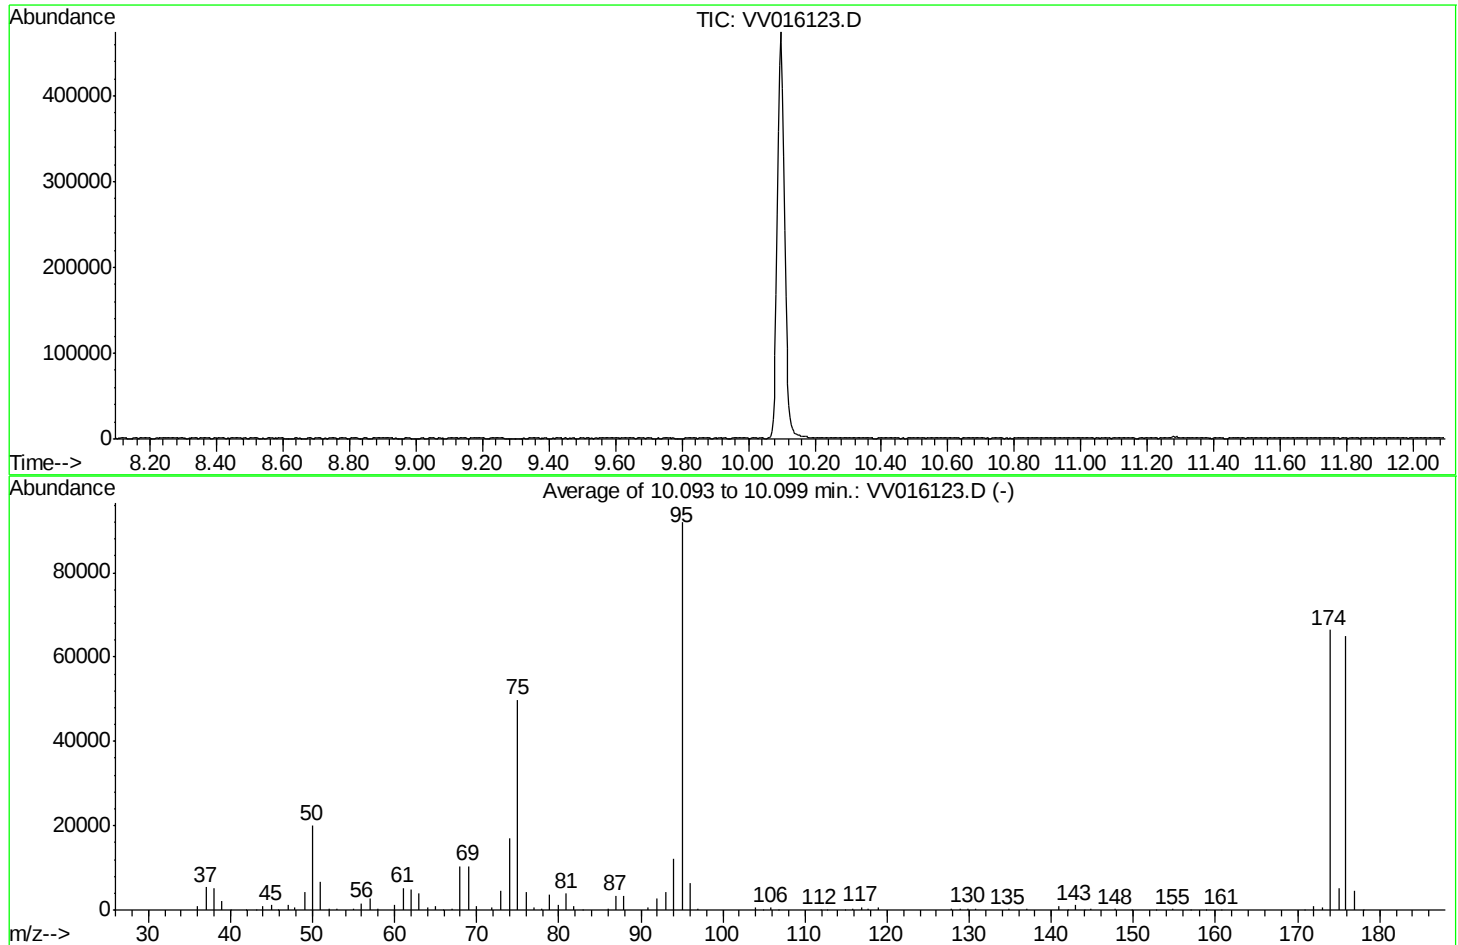

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	20018	PASS
75	95	30	80	54.3	49917	PASS
95	95	100	100	100.0	91941	PASS
96	95	5	9	6.8	6240	PASS
173	174	0.00	2	1.0	651	PASS
174	95	50	120	72.2	66413	PASS
175	174	5	9	7.8	5194	PASS
176	174	95	101	97.8	64946	PASS
177	176	5	9	6.9	4463	PASS

m/z	Abundance
36.00	819.0
37.00	5079.0
38.00	4847.0
39.00	2138.0
40.00	335.0
43.10	109.0
44.00	1219.0
45.00	994.0
45.90	156.0
47.00	1028.0
47.90	693.0
49.00	4125.0
50.00	19680.0
51.00	6537.0
52.00	306.0
53.00	210.0
55.00	261.0
55.90	1555.0
57.00	2712.0
57.90	168.0
60.00	1038.0
61.00	5044.0
62.00	4916.0
63.00	3764.0
64.00	532.0
65.00	842.0
66.00	103.0
67.00	414.0
68.00	9884.0
69.00	10010.0
70.00	698.0
71.90	643.0
73.00	4503.0
74.00	16800.0
75.00	47904.0
76.00	4286.0
77.00	642.0
77.90	426.0
78.90	3460.0
79.90	1031.0
80.90	3712.0
81.90	889.0
86.00	163.0
87.00	3434.0
87.90	3240.0
90.80	464.0
92.00	2668.0
93.00	4090.0
94.00	11636.0
95.00	88160.0
96.00	6046.0
97.00	120.0
104.00	492.0
105.00	119.0
105.90	519.0
111.90	111.0
112.80	143.0
114.80	146.0
115.80	394.0
116.90	696.0
117.70	401.0
118.90	634.0
127.80	302.0
128.90	237.0
129.90	352.0
130.80	210.0
134.80	221.0
136.90	195.0
140.80	1027.0
142.00	118.0
142.90	1200.0
143.90	108.0
144.80	226.0
147.80	271.0
149.80	107.0
152.80	135.0
154.90	249.0
156.90	138.0
160.80	111.0
170.80	135.0
172.00	1051.0
173.90	61688.0
175.00	4723.0
175.90	60712.0
177.00	4144.0
178.00	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.00	949.0
37.00	5520.0
38.00	5236.0
39.00	2258.0
40.00	364.0
41.90	101.0
43.10	115.0
44.00	1337.0
45.00	1163.0
45.90	139.0
47.00	1203.0
47.90	710.0
49.00	4395.0
50.00	20808.0
51.00	6835.0
52.00	352.0
53.00	233.0
55.00	276.0
56.00	1654.0
57.00	2917.0
58.00	192.0
60.00	1256.0
61.00	5327.0
62.00	5025.0
63.00	3971.0
64.00	588.0
64.90	870.0
66.00	121.0
67.00	462.0
68.00	10585.0
69.00	10783.0
70.00	810.0
71.90	641.0
73.00	4844.0
74.00	17648.0
75.00	51736.0
76.00	4425.0
77.00	640.0
77.90	409.0
78.90	3885.0
79.90	1179.0
80.90	4037.0
81.80	874.0
82.90	109.0
86.00	233.0
87.00	3629.0
87.90	3460.0
90.80	490.0
92.00	2950.0
93.00	4519.0
94.00	12648.0
95.00	95072.0
96.00	6500.0
97.00	171.0
103.90	509.0
105.00	121.0
105.90	590.0
111.90	106.0
112.70	121.0
114.80	125.0
115.80	424.0
116.90	740.0
117.70	366.0
118.90	683.0
127.90	347.0
128.90	250.0
129.90	368.0
130.70	161.0
134.80	235.0
137.00	221.0
140.90	1108.0
142.00	156.0
142.90	1270.0
144.00	141.0
144.80	236.0
147.80	270.0
149.80	106.0
152.80	138.0
154.80	301.0
156.90	130.0
158.80	100.0
160.70	107.0
170.90	135.0
171.90	1077.0
173.00	963.0
173.90	68872.0
175.00	5433.0
175.90	67240.0
176.90	4652.0
178.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.00	954.0
37.00	5442.0
38.00	5028.0
39.00	2101.0
40.00	406.0
43.10	103.0
44.00	1281.0
45.00	1147.0
45.80	133.0
47.00	1201.0
47.90	671.0
49.00	4321.0
50.00	19568.0
51.00	6508.0
52.00	353.0
53.00	215.0
55.00	267.0
56.00	1563.0
57.00	2857.0
58.00	192.0
60.00	1279.0
61.00	5308.0
62.00	4807.0
63.00	3824.0
64.00	595.0
64.90	786.0
65.90	124.0
67.00	452.0
68.00	10301.0
69.00	10490.0
70.00	828.0
71.90	575.0
73.00	4522.0
74.00	16776.0
75.00	50112.0
76.00	4145.0
77.00	560.0
77.90	364.0
78.90	3778.0
79.90	1207.0
80.90	3927.0
81.80	817.0
82.90	117.0
86.00	263.0
86.90	3389.0
88.00	3380.0
90.90	452.0
92.00	2852.0
93.00	4468.0
94.00	12012.0
95.00	92592.0
96.00	6175.0
97.00	226.0
103.90	468.0
104.90	139.0
105.80	540.0
106.80	132.0
112.70	116.0
114.80	105.0
115.80	447.0
116.90	686.0
117.80	333.0
118.90	674.0
127.80	353.0
128.90	233.0
129.90	330.0
130.70	123.0
134.80	230.0
137.00	222.0
140.90	1021.0
142.10	201.0
142.90	1148.0
144.00	143.0
144.90	255.0
147.80	243.0
152.70	103.0
154.80	300.0
156.90	139.0
158.80	102.0
160.80	102.0
171.00	113.0
171.90	1012.0
173.00	991.0
173.90	68680.0
175.00	5426.0
175.90	66888.0
176.90	4595.0
178.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

Scan 2788 (10.054 min): VV016123.D
BFB60

m/z	Abundance
39.90	298.0
43.90	412.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60