

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
 Data File : VV021341.D
 Acq On : 20 May 2021 11:03
 Operator : SY/MD
 Sample : VSTD0.563
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 21 05:01:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 21 05:00:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	29480	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	27930	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	14980	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	8279	0.33	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	8122	0.43	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	11410	0.46	ug/L	0.00
8) Toluene-d8	7.317	98	31373	0.59	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	6198	0.40	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.303	62	13020	0.30	ug/L	100
6) Trichloroethene	5.925	95	11336	0.44	ug/L	100
9) 1,2-Dibromoethane	8.368	107	7617	0.51	ug/L	100
12) 1,2,3-Trichloropropane	10.267	75	6272	0.41	ug/L	100
13) 1,2-Dibromo-3-chloropr...	12.409	75	968	0.43	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
Data File : VV021341.D
Acq On : 20 May 2021 11:03
Operator : SY/MD
Sample : VSTD0.563
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 21 05:01:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 21 05:00:22 2021
Response via : Initial Calibration




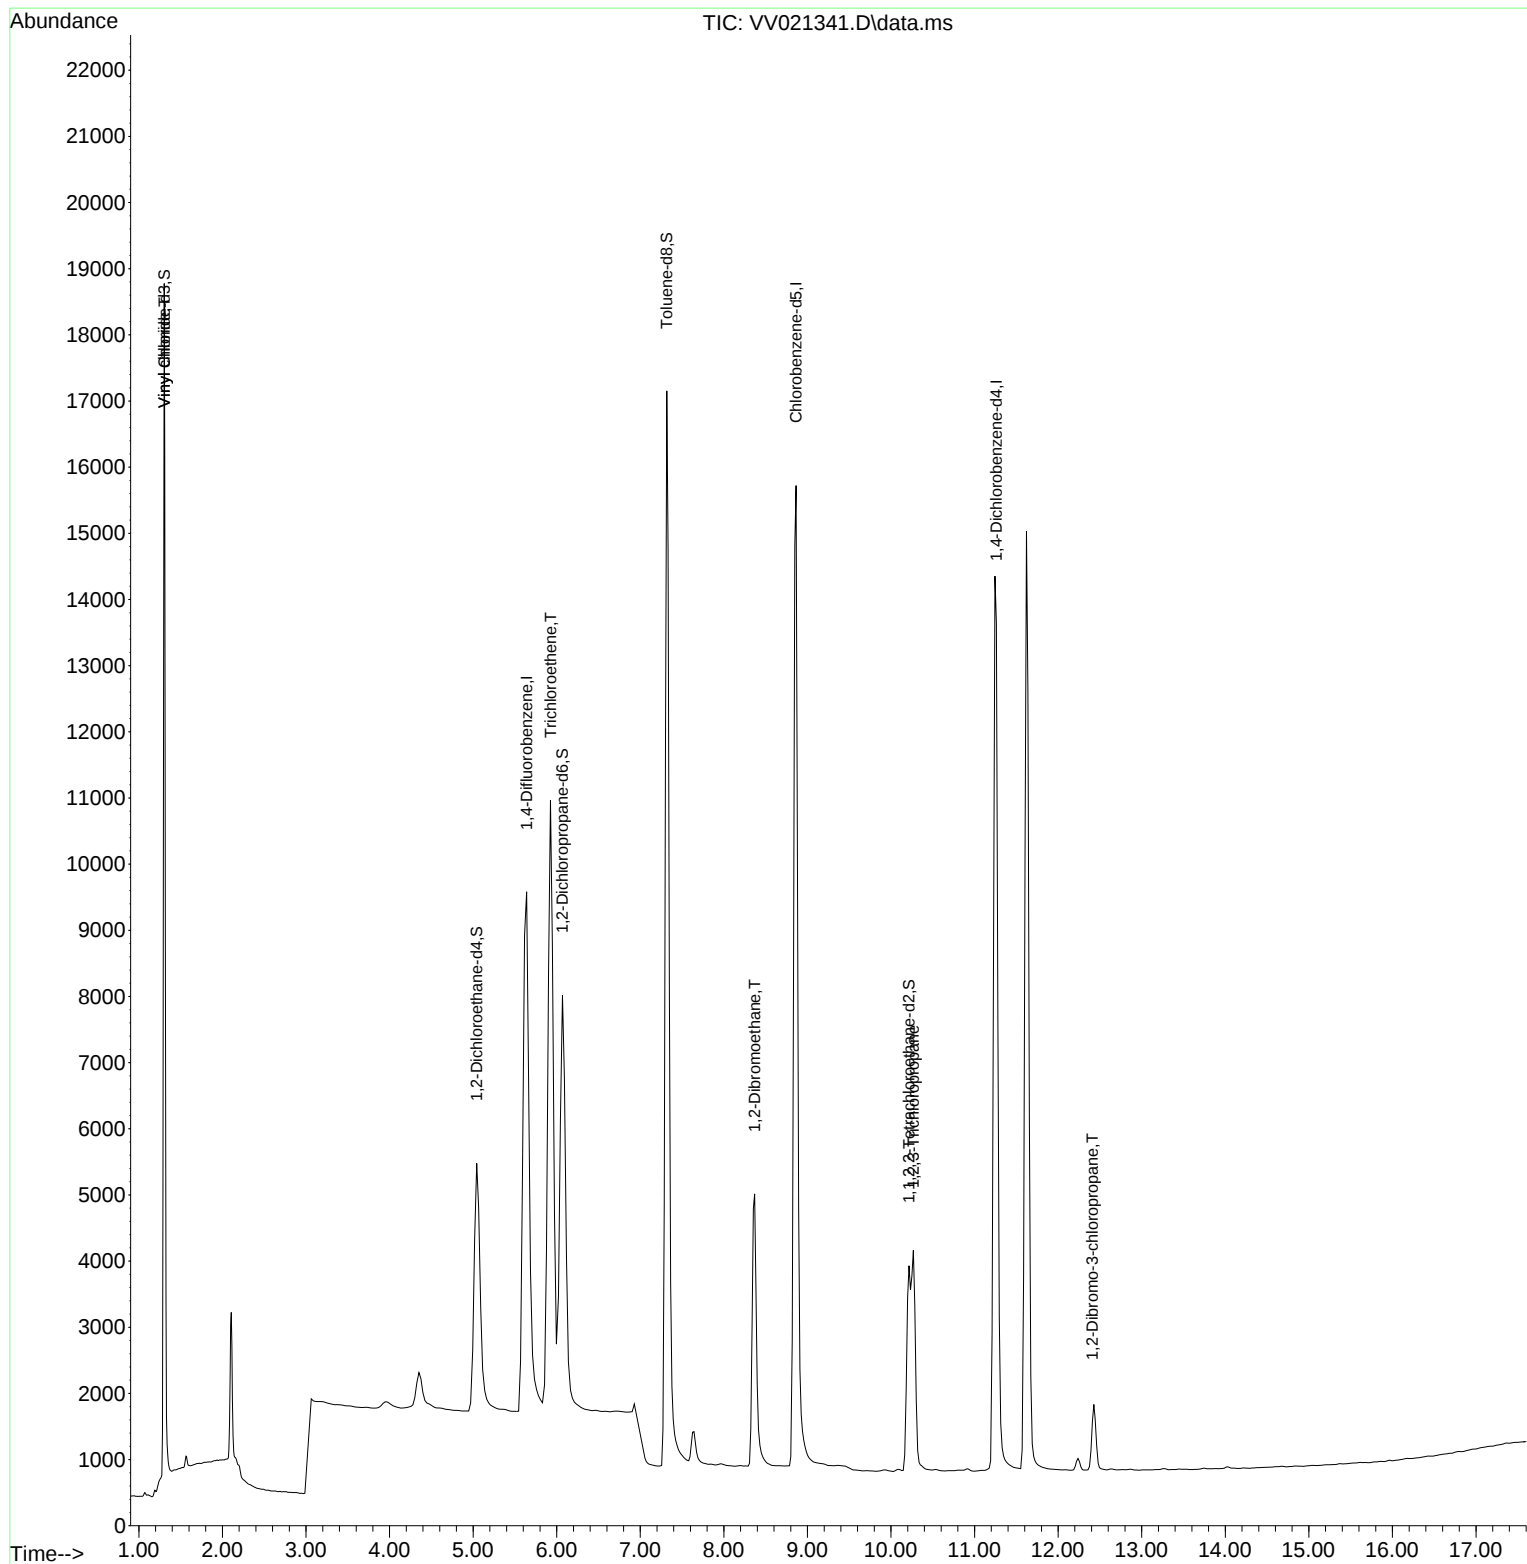


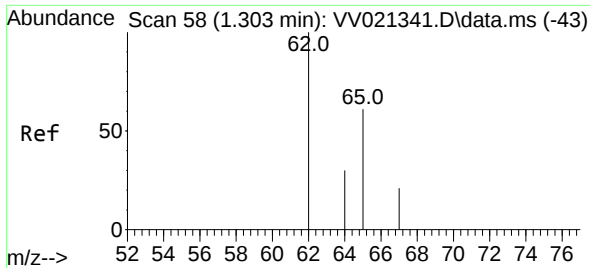

#3
 Vinyl chloride
 Concen: 0.30 ug/L
 RT: 1.303 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: VV021341.D
 Acq: 20 May 2021 11:03




Instrument :
 MSVOA_V
 ClientSampled :


Tgt Ion: 62 Resp: 13020
 Ion Ratio Lower Upper
 62 100
 64 32.2 22.5 41.9

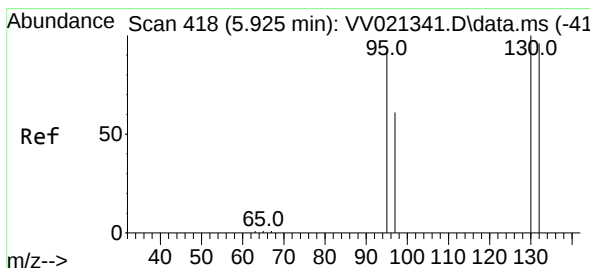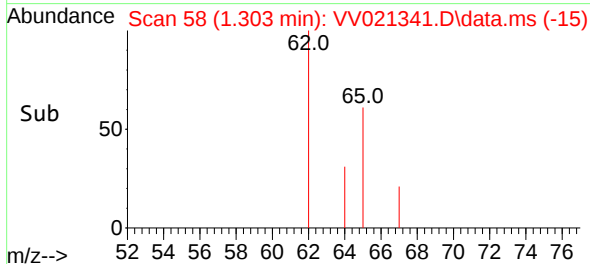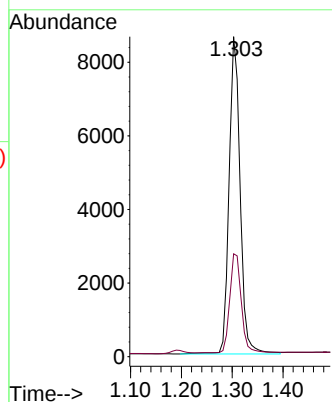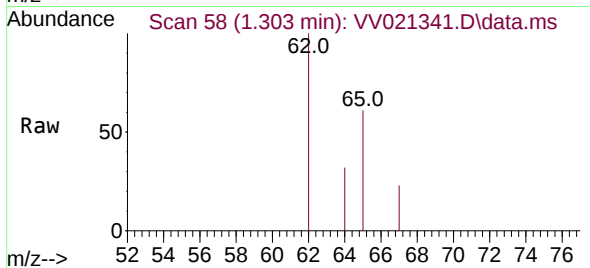

#6
 Trichloroethene
 Concen: 0.44 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV021341.D
 Acq: 20 May 2021 11:03

Tgt Ion: 95 Resp: 11336
 Ion Ratio Lower Upper
 95 100
 97 67.8 47.5 88.1
 132 102.3 71.6 133.0
 130 106.4 74.5 138.3


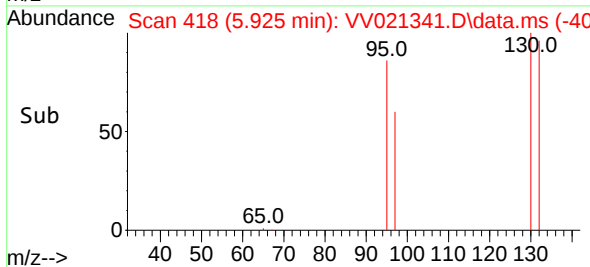
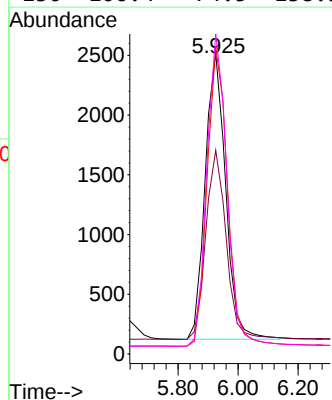
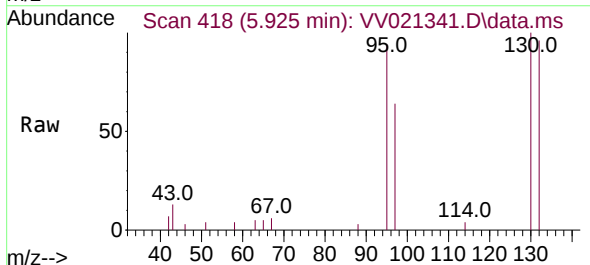


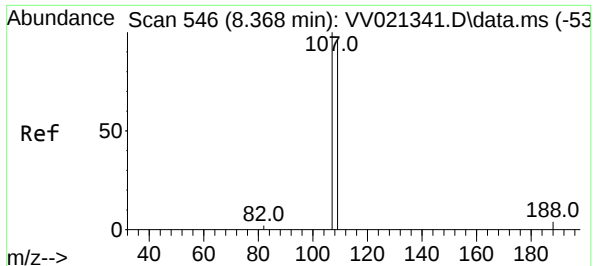

#9
1,2-Dibromoethane
Concen: 0.51 ug/L
RT: 8.368 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV021341.D
Acq: 20 May 2021 11:03




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:	107	Resp:	7617
Ion	Ratio	Lower	Upper
107	100		
109	96.1	67.3	124.9
188	6.9	5.5	8.3

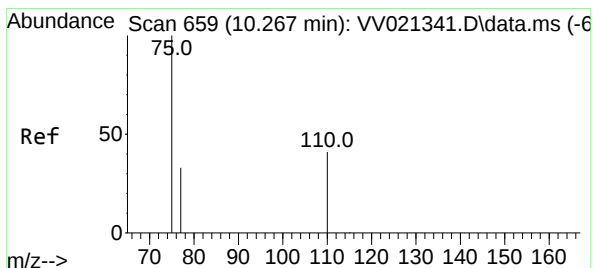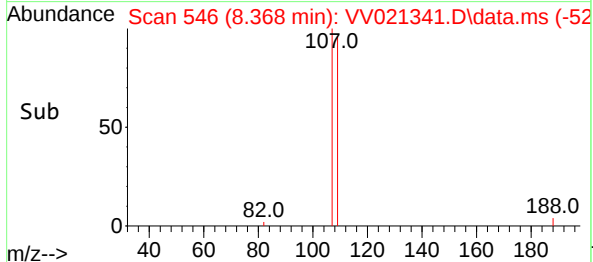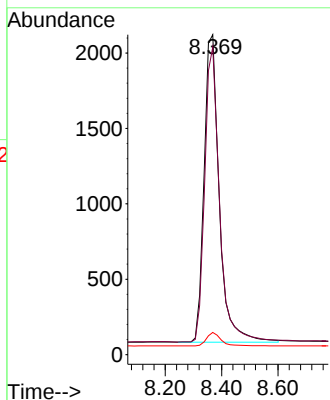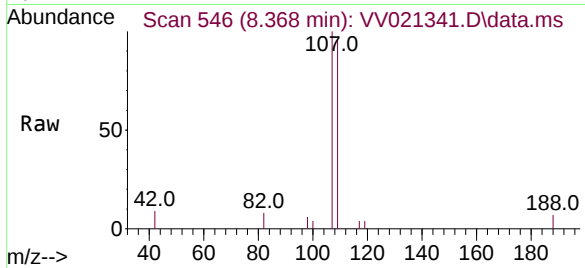

#12
1,2,3-Trichloropropane
Concen: 0.41 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV021341.D
Acq: 20 May 2021 11:03


Tgt Ion:	75	Resp:	6272
Ion	Ratio	Lower	Upper
75	100		
110	41.9	33.5	50.3
77	33.4	26.7	40.1

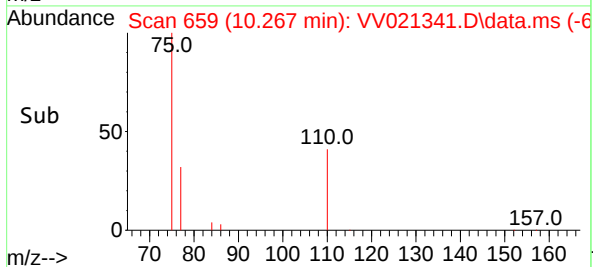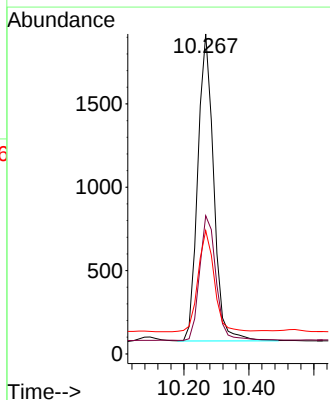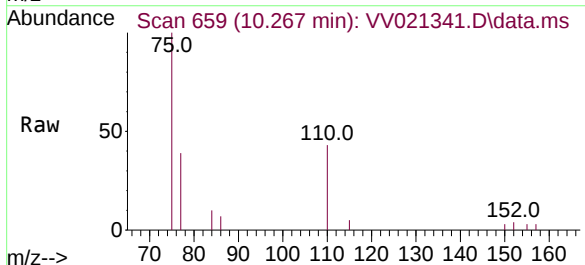

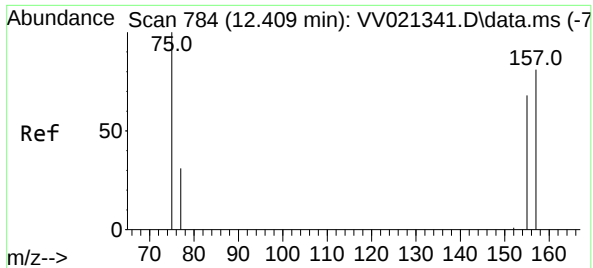

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.43 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. 0.000 min
 Lab File: VV021341.D
 Acq: 20 May 2021 11:03

Instrument :
 MSVOA_V
 ClientSampleId :

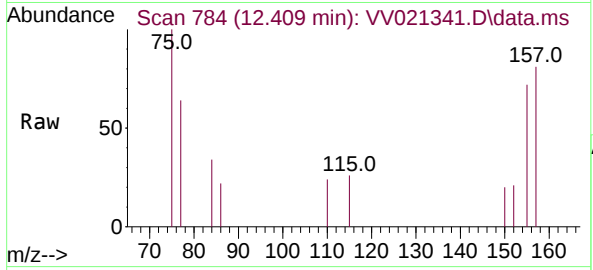

Tgt Ion:	75	Resp:	968
Ion	Ratio	Lower	Upper
75	100		
157	81.1	64.9	97.3
155	71.7	57.4	86.0

