

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
 Data File : VV021343.D
 Acq On : 20 May 2021 12:04
 Operator : SY/MD
 Sample : VSTD00265
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 21 05:01:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 21 05:00:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	28785	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	27534	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	14546	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	27720	1.12	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	28857	1.56	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	40265	1.66	ug/L	0.00
8) Toluene-d8	7.317	98	111946	2.13	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	22216	1.46	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.310	62	46131	1.10	ug/L	96
6) Trichloroethene	5.925	95	40913	1.61	ug/L	97
9) 1,2-Dibromoethane	8.353	107	27013	1.82	ug/L #	97
12) 1,2,3-Trichloropropane	10.267	75	22112	1.49	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.409	75	3520	1.61	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
Data File : VV021343.D
Acq On : 20 May 2021 12:04
Operator : SY/MD
Sample : VSTD00265
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 21 05:01:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 21 05:00:22 2021
Response via : Initial Calibration




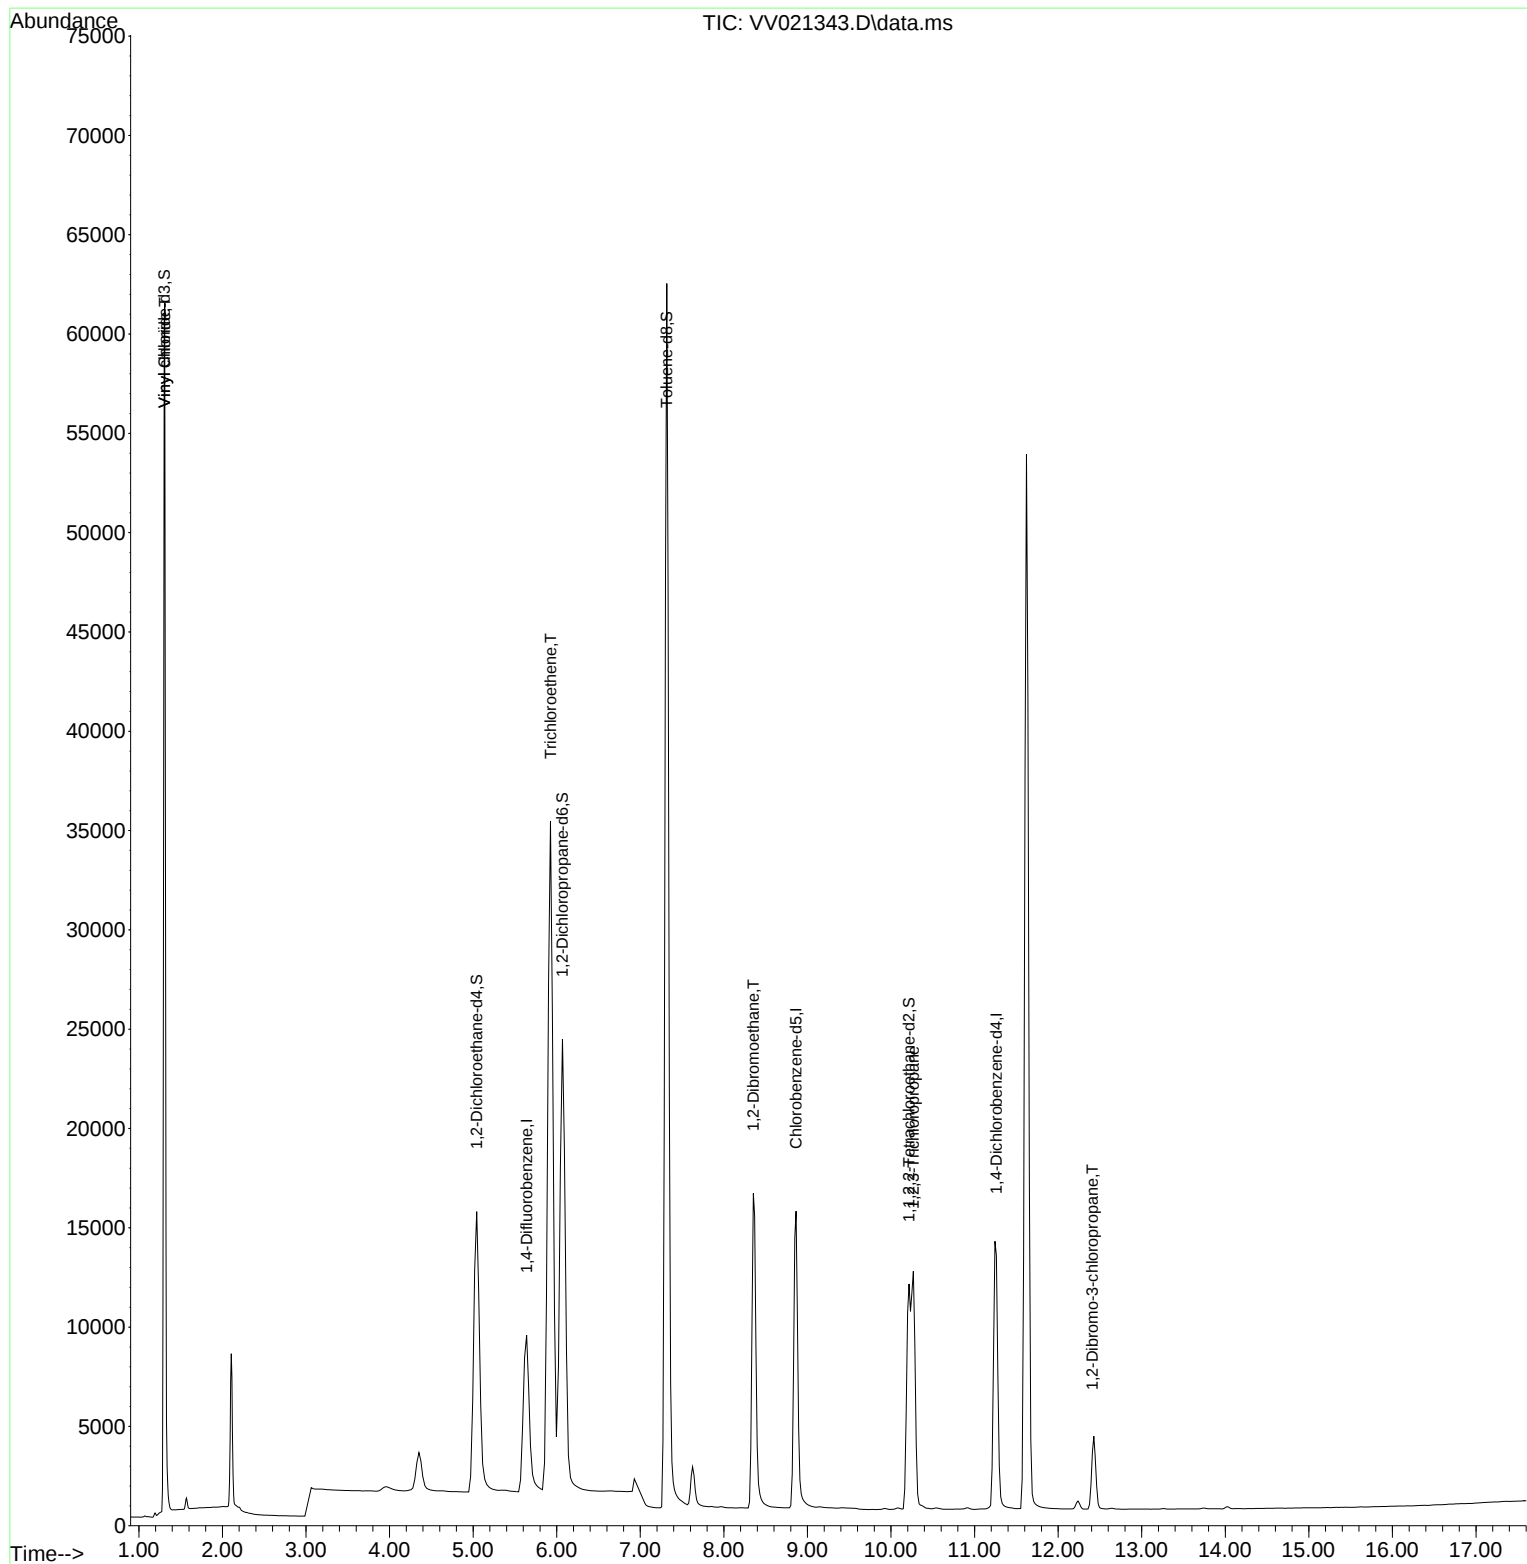


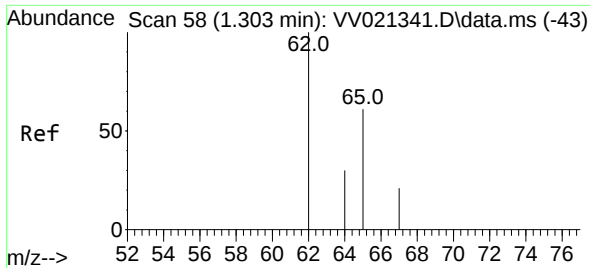

#3
 Vinyl chloride
 Concen: 1.10 ug/L
 RT: 1.310 min Scan# 59
 Delta R.T. 0.007 min
 Lab File: VV021343.D
 Acq: 20 May 2021 12:04




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion: 62 Resp: 46131
 Ion Ratio Lower Upper
 62 100
 64 34.2 22.5 41.9

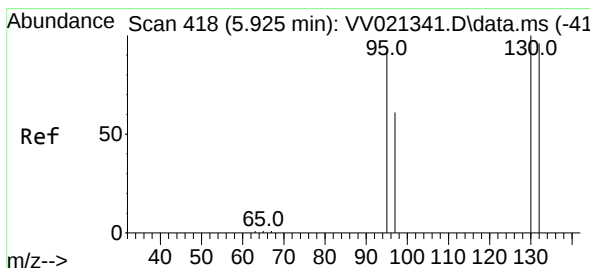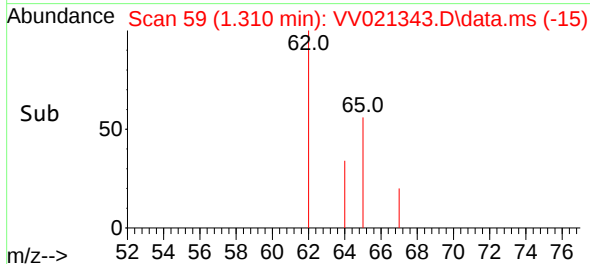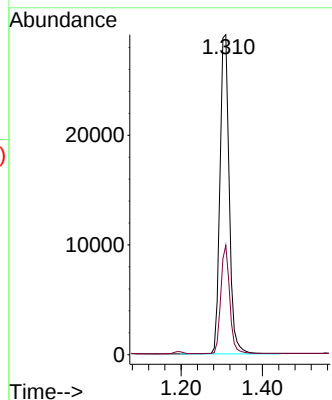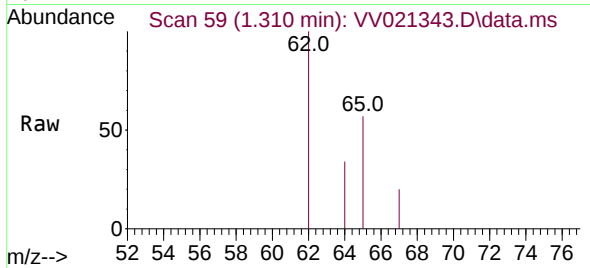

#6
 Trichloroethene
 Concen: 1.61 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. -0.000 min
 Lab File: VV021343.D
 Acq: 20 May 2021 12:04


Tgt Ion: 95 Resp: 40913
 Ion Ratio Lower Upper
 95 100
 97 66.0 47.5 88.1
 132 105.8 71.6 133.0
 130 108.7 74.5 138.3

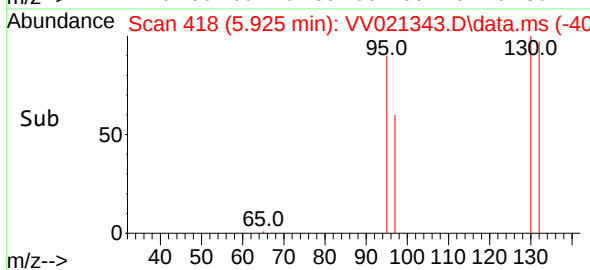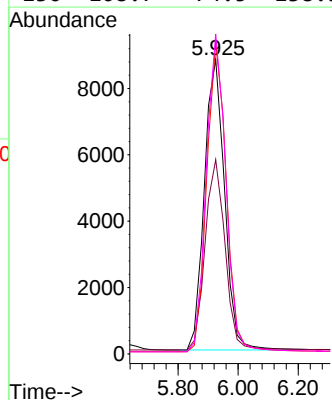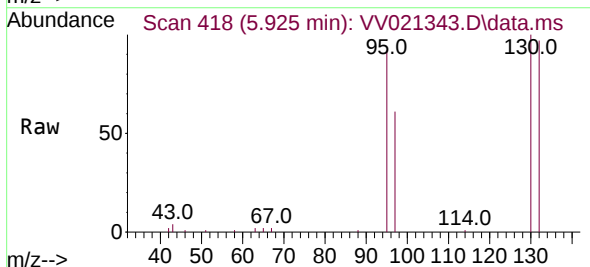



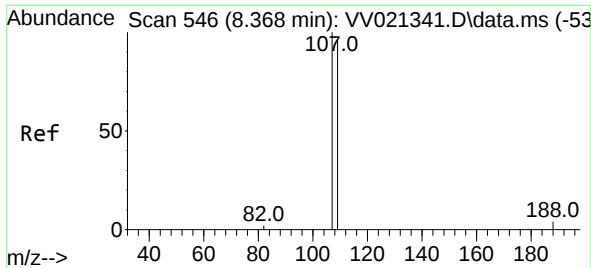


#9
1,2-Dibromoethane
Concen: 1.82 ug/L
RT: 8.353 min Scan# 545
Delta R.T. -0.016 min
Lab File: VV021343.D
Acq: 20 May 2021 12:04

Instrument :
MSVOA_V
ClientSampled :



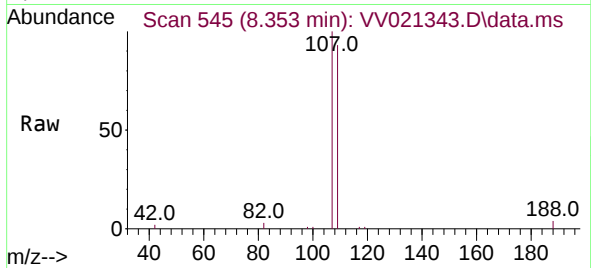



Tgt Ion:107 Resp: 27013
Ion Ratio Lower Upper
107 100
109 93.1 67.3 124.9
188 4.3 5.5 8.3#

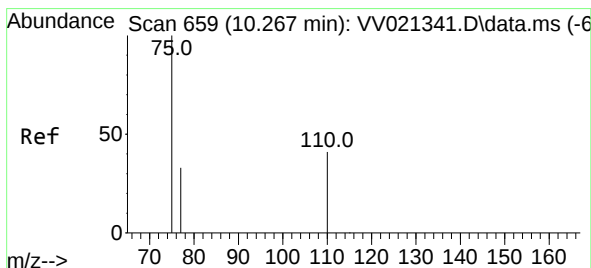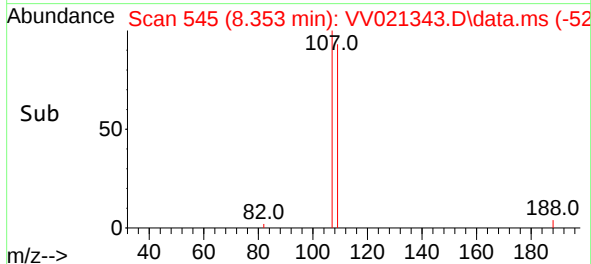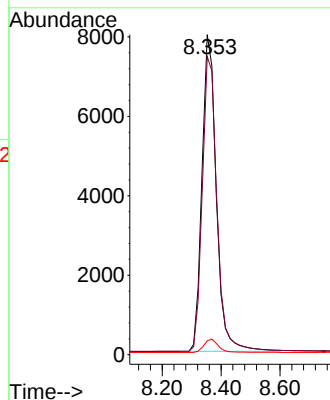

#12
1,2,3-Trichloropropane
Concen: 1.49 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV021343.D
Acq: 20 May 2021 12:04


Tgt Ion: 75 Resp: 22112
Ion Ratio Lower Upper
75 100
110 42.8 33.5 50.3
77 33.5 26.7 40.1

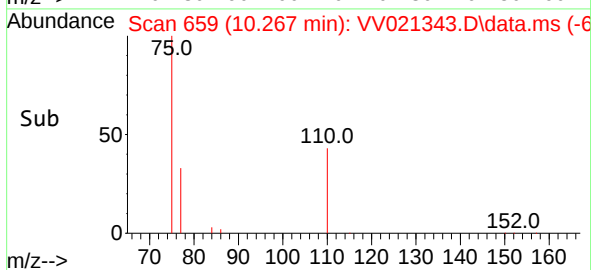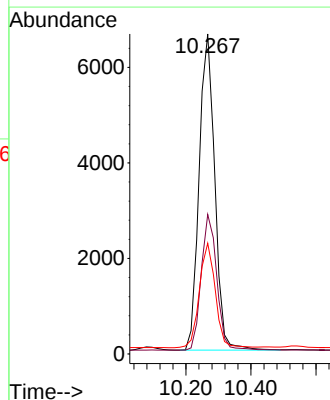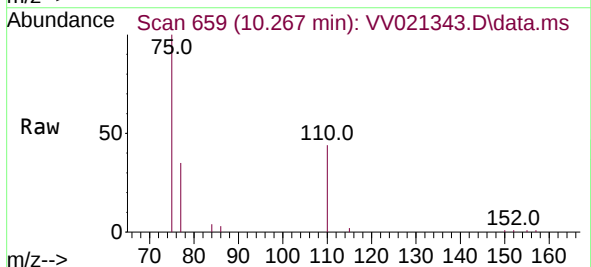

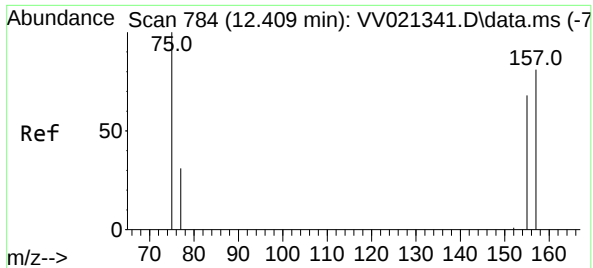

#13
 1,2-Dibromo-3-chloropropane
 Concen: 1.61 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. -0.000 min
 Lab File: VV021343.D
 Acq: 20 May 2021 12:04

Instrument :
 MSVOA_V
 ClientSampleId :

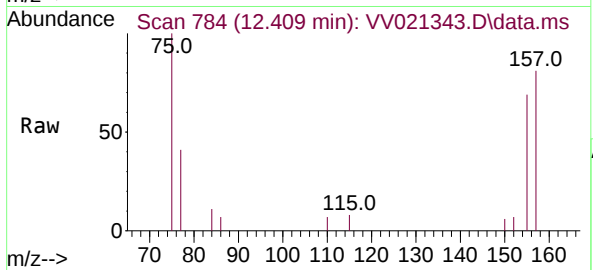

Tgt Ion: 75	Resp:	3520
Ion Ratio	Lower	Upper
75	100	
157	81.4	64.9 97.3
155	69.4	57.4 86.0

