

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
 Data File : VV021345.D
 Acq On : 20 May 2021 13:20
 Operator : SY/MD
 Sample : VV0520WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 21 05:08:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 21 05:04:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	29465	0.50	ug/L	-0.02
5) Chlorobenzene-d5	8.863	117	26773	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	14316	0.50	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	7813	0.43	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	86.00%		
4) 1,2-Dichloroethane-d4	5.042	65	7668	0.50	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.00%		
7) 1,2-Dichloropropane-d6	6.068	67	10674	0.52	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	104.00%		
8) Toluene-d8	7.317	98	29851	0.51	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.00%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	5594	0.49	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.00%		
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.426	75	23	0.01	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
Data File : VV021345.D
Acq On : 20 May 2021 13:20
Operator : SY/MD
Sample : VV0520WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: May 21 05:08:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 21 05:04:41 2021
Response via : Initial Calibration

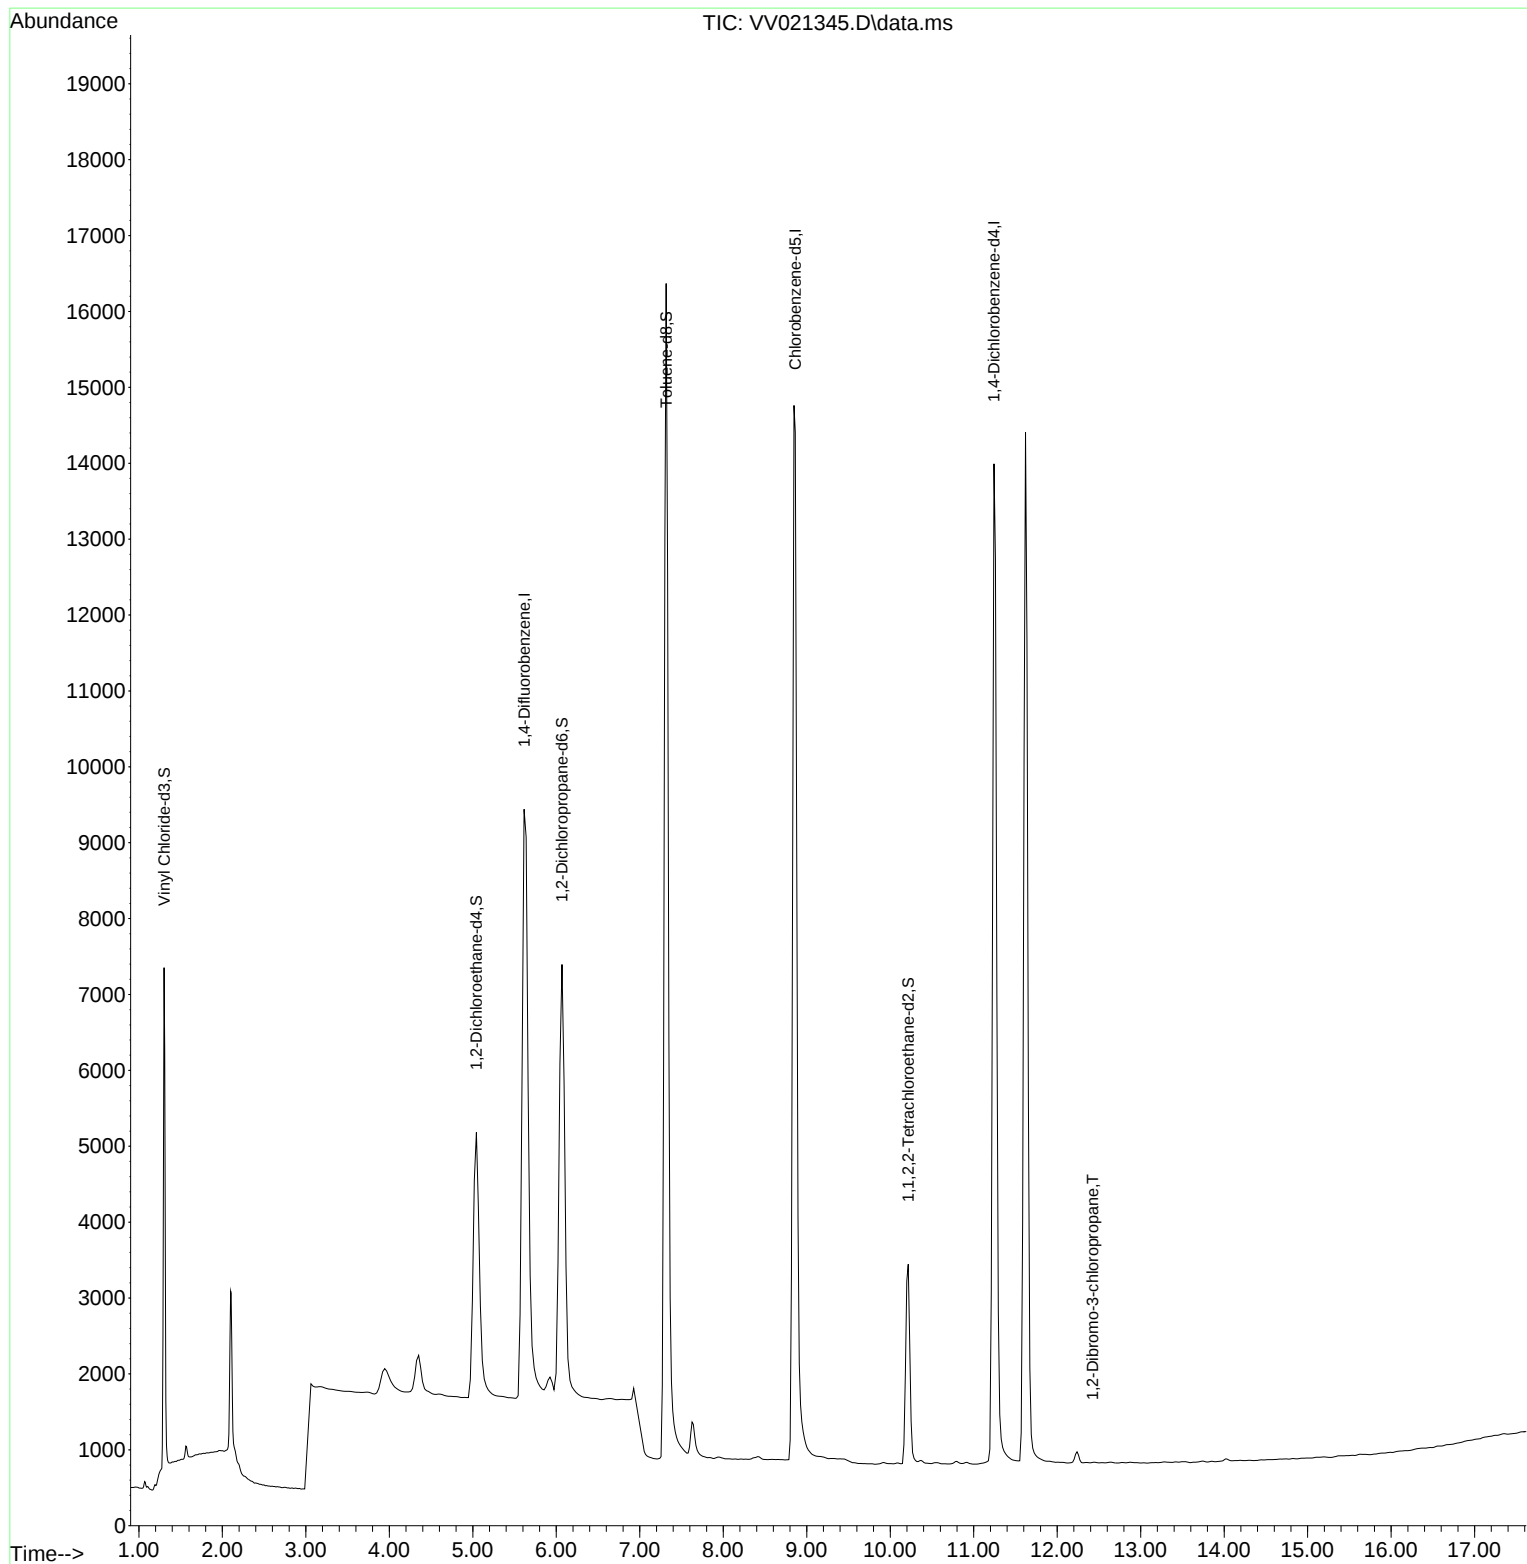

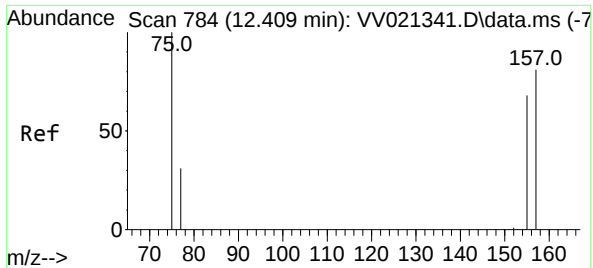

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.01 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.017 min
 Lab File: VV021345.D
 Acq: 20 May 2021 13:20

Instrument :
 MSVOA_V
 ClientSampleId :

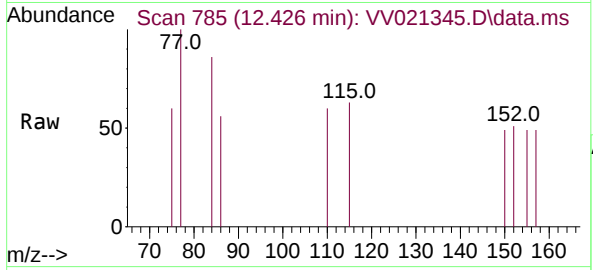

Tgt Ion:	75	Resp:	23
Ion	Ratio	Lower	Upper
75	100		
157	80.2	64.9	97.3
155	81.5	57.4	86.0

