
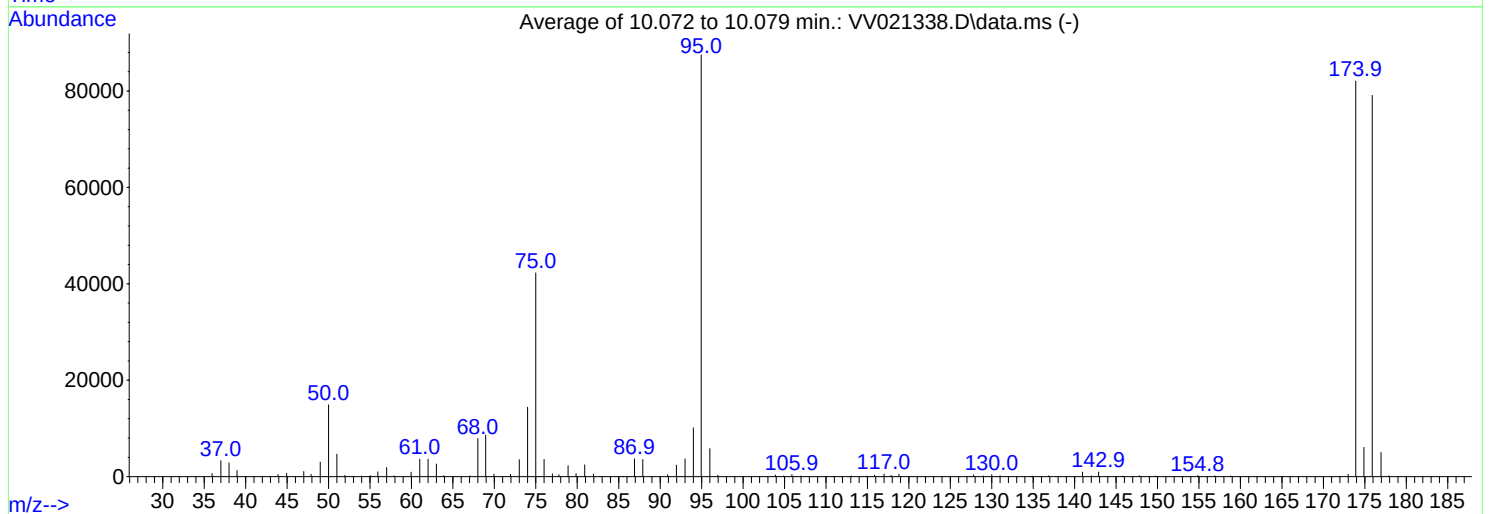


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052021\
 Data File : VV021338.D
 Acq On : 20 May 2021 09:23
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB197

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 21 05:04:41 2021

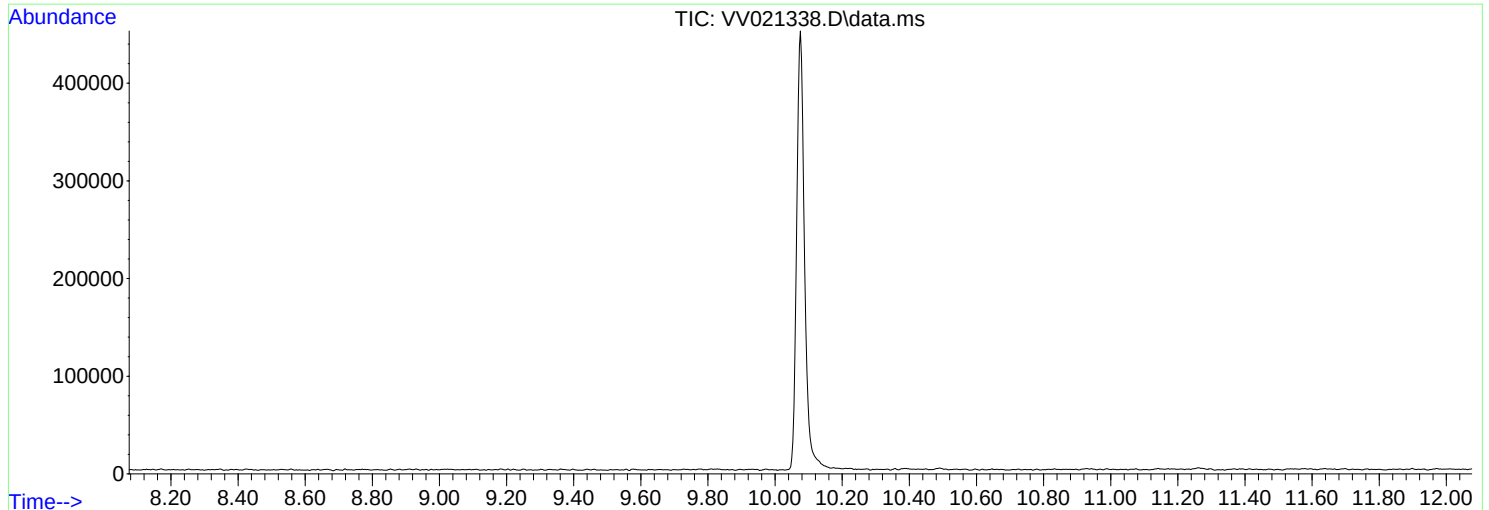

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	14889	PASS
75	95	30	80	48.3	42251	PASS
95	95	100	100	100.0	87494	PASS
96	95	5	9	6.6	5814	PASS
173	174	0.00	2	0.6	462	PASS
174	95	50	120	93.8	82053	PASS
175	174	5	9	7.4	6070	PASS
176	174	95	101	96.4	79093	PASS
177	176	5	9	6.3	5015	PASS

m/z	Abundance
36.00	635.0
37.00	3384.0
38.00	2924.0
39.00	1525.0
39.90	299.0
41.00	257.0
42.00	242.0
42.90	337.0
43.90	1585.0
45.00	712.0
46.00	110.0
47.00	1086.0
47.90	487.0
49.00	3071.0
50.00	15485.0
51.00	4785.0
51.90	239.0
52.90	116.0
54.00	139.0
54.90	325.0
55.10	327.0
56.00	1162.0
57.00	2172.0
57.90	171.0
60.00	976.0
61.00	3775.0
62.00	3768.0
63.00	2660.0
63.90	215.0
67.10	305.0
68.00	8178.0
69.00	9114.0
70.00	660.0
71.10	132.0
72.00	499.0
73.00	3609.0
74.00	14916.0
75.00	43568.0
76.00	3684.0
77.00	582.0
77.80	420.0
78.90	2320.0
79.90	652.0
80.90	2565.0
82.00	566.0
82.90	202.0
85.50	119.0
86.90	3770.0
87.90	3564.0
90.90	412.0
91.90	2513.0
93.00	3772.0
94.00	10466.0
95.00	90528.0
96.00	5920.0
96.90	281.0
103.90	339.0
104.90	175.0
105.90	454.0
107.00	127.0
111.90	116.0
113.10	181.0
115.00	115.0
115.80	309.0
117.00	558.0
117.80	278.0
118.80	490.0
127.80	342.0
129.00	173.0
130.00	450.0
131.00	218.0
134.90	163.0
136.80	161.0
140.90	930.0
142.00	179.0
142.90	1006.0
144.00	104.0
145.80	145.0
147.80	206.0
149.70	122.0
153.10	106.0
154.90	221.0
156.90	178.0
158.80	126.0
171.80	106.0
173.10	682.0
173.90	84896.0
174.90	6328.0
175.90	81808.0
177.00	5198.0
177.90	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
35.90	591.0
37.00	3537.0
38.00	2845.0
39.00	1480.0
39.90	301.0
41.00	304.0
42.00	255.0
42.90	366.0
43.90	1603.0
45.00	681.0
46.10	110.0
47.00	1061.0
47.90	505.0
49.00	3094.0
50.00	15170.0
51.00	4888.0
51.90	248.0
54.00	130.0
54.90	377.0
56.00	1236.0
57.00	2166.0
57.90	145.0
59.90	985.0
61.00	3621.0
62.00	3537.0
63.00	2580.0
63.90	246.0
67.10	305.0
68.00	8162.0
69.00	8917.0
70.00	678.0
71.00	127.0
71.90	459.0
73.00	3528.0
74.00	14548.0
75.00	42496.0
76.00	3691.0
77.00	603.0
77.80	444.0
78.90	2239.0
79.80	582.0
80.90	2534.0
82.00	581.0
82.90	148.0
85.60	133.0
86.90	3712.0
87.90	3799.0
90.90	418.0
92.00	2411.0
93.00	3634.0
94.00	10216.0
95.00	88848.0
96.00	5990.0
96.90	336.0
103.90	341.0
105.00	213.0
105.90	424.0
107.00	105.0
110.90	103.0
111.90	129.0
112.90	134.0
115.00	141.0
115.80	319.0
117.00	530.0
117.80	265.0
118.80	542.0
127.80	310.0
128.90	173.0
130.00	449.0
131.00	177.0
134.70	148.0
135.00	139.0
136.80	186.0
140.90	938.0
142.00	129.0
142.90	941.0
145.80	133.0
147.90	181.0
149.70	105.0
154.80	200.0
156.90	150.0
158.70	140.0
171.90	105.0
173.90	80024.0
174.90	6014.0
175.90	77200.0
177.00	5013.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
36.00	650.0
37.00	3010.0
38.00	2755.0
39.00	1414.0
40.00	275.0
40.90	242.0
42.00	224.0
43.00	315.0
43.90	1517.0
44.90	749.0
47.00	1015.0
47.90	419.0
49.00	2874.0
50.00	14013.0
51.00	4310.0
52.00	211.0
52.80	102.0
54.00	114.0
54.90	295.0
55.10	305.0
56.00	988.0
57.00	2048.0
57.90	183.0
60.00	852.0
61.00	3450.0
62.00	3569.0
63.00	2584.0
63.90	179.0
67.10	262.0
68.00	7353.0
69.00	8276.0
70.00	618.0
71.10	154.0
72.00	477.0
73.00	3427.0
74.00	13730.0
75.00	40688.0
76.00	3373.0
77.00	515.0
77.80	346.0
78.90	2180.0
79.90	696.0
80.90	2297.0
81.80	496.0
82.90	224.0
84.90	109.0
86.90	3543.0
87.90	3288.0
90.90	400.0
92.00	2271.0
93.00	3632.0
94.00	9674.0
95.00	83448.0
96.00	5532.0
97.00	237.0
103.90	314.0
104.80	123.0
105.90	425.0
107.00	131.0
113.10	190.0
114.90	119.0
115.90	272.0
117.00	536.0
117.90	271.0
118.80	425.0
127.80	322.0
129.00	174.0
130.00	373.0
131.00	230.0
134.80	172.0
136.90	170.0
141.00	904.0
142.00	202.0
142.90	935.0
145.80	142.0
147.70	228.0
149.80	121.0
154.90	249.0
156.90	183.0
158.90	119.0
160.70	105.0
172.90	705.0
173.90	81240.0
174.90	5867.0
175.90	78272.0
176.90	4833.0
177.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
38.90	200.0
39.90	289.0
41.00	302.0
42.10	171.0
43.00	267.0
43.90	1135.0
55.00	258.0
55.90	124.0
57.00	226.0
67.00	123.0
68.90	144.0
69.90	128.0
70.90	107.0
83.00	154.0
83.90	128.0
85.10	106.0
94.90	114.0
97.80	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197