


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052120\
Data File : VV016147.D
Acq On : 21 May 2020 12:47
Operator : SY/MD
Sample : L2725-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9B32

Manual Integrations
APPROVED

apatel
5/22/2020 11:26:01 AM

Quant Time: May 22 02:51:35 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 22 01:50:48 2020
Response via : Initial Calibration

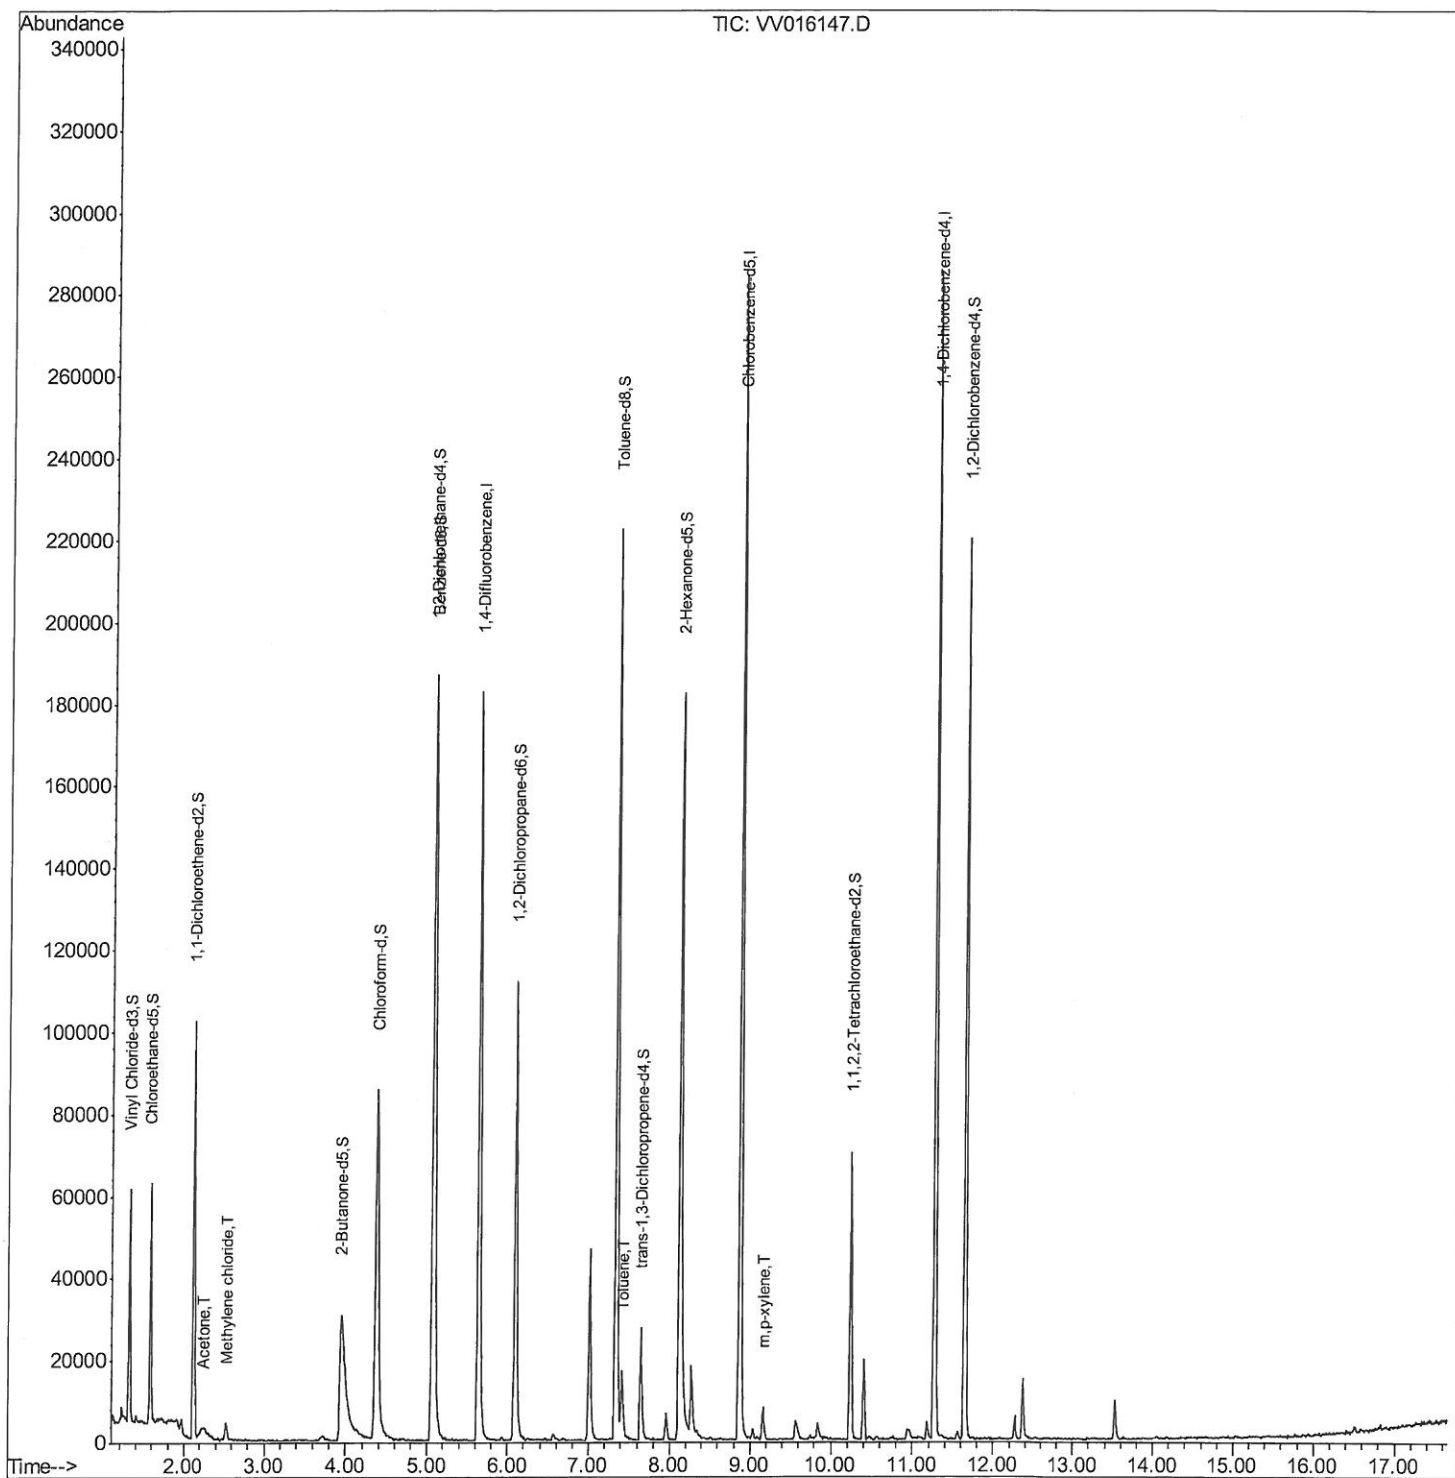

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052120\
Data File : VV016147.D
Acq On : 21 May 2020 12:47
Operator : SY/MD
Sample : L2725-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9B32

Manual Integrations
APPROVED

apatel
5/22/2020 11:26:01 AM

Quant Time: May 22 01:53:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 22 01:50:48 2020
Response via : Initial Calibration

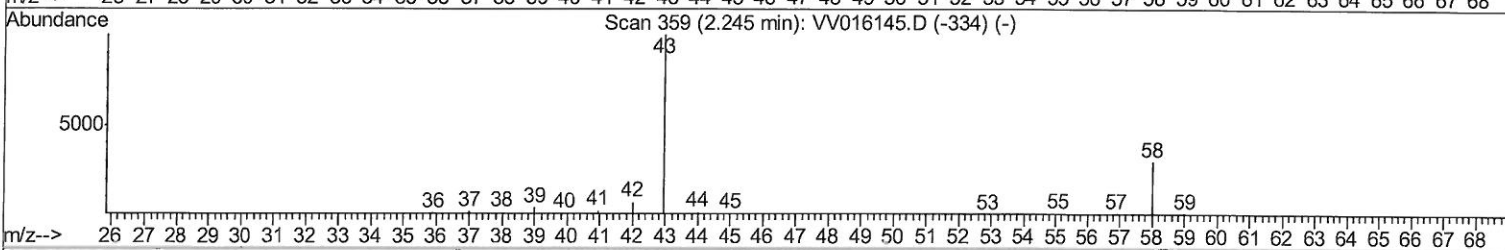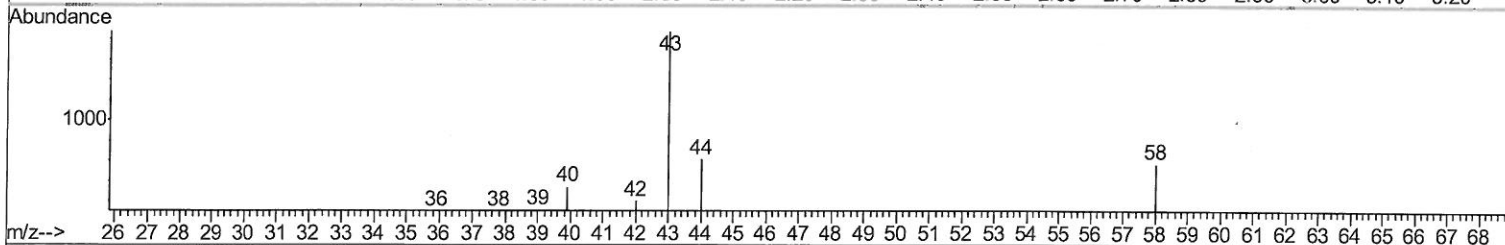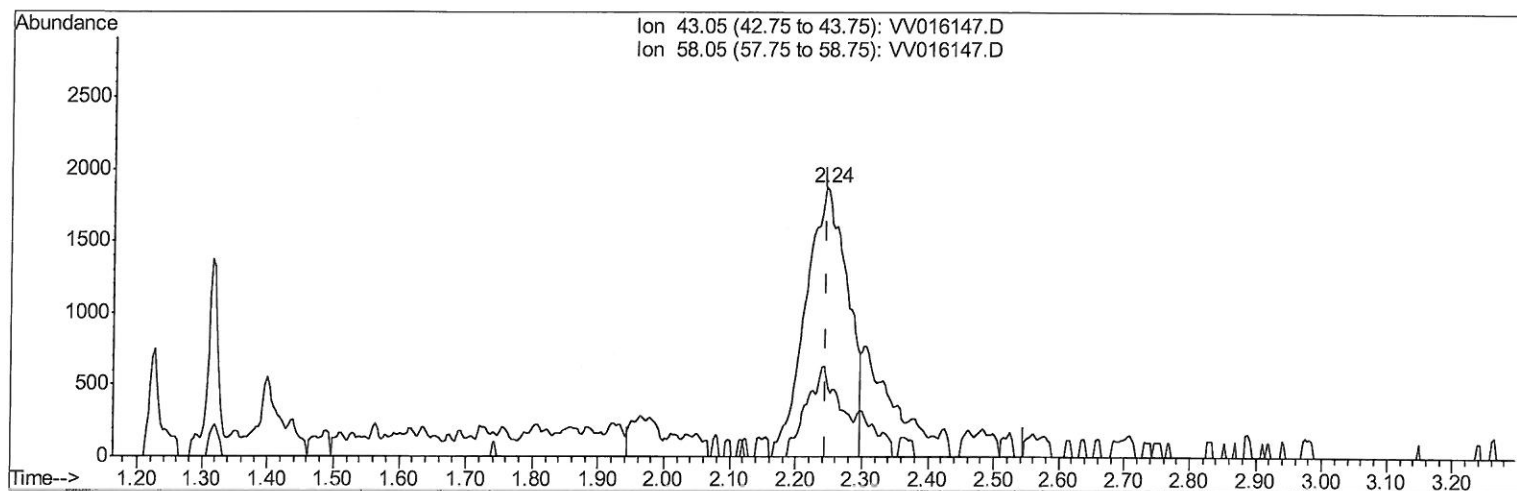

TIC: VV016147.D

(13) Acetone (T)

2.245min (+0.000) 5.47ug/L

response 8217

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	17.52
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052120\
 Data File : VV016147.D
 Acq On : 21 May 2020 12:47
 Operator : SY/MD
 Sample : L2725-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9B32

Manual Integrations
 APPROVED

apatel
 5/22/2020 11:26:01 AM

Quant Time: May 22 01:53:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 22 01:50:48 2020
 Response via : Initial Calibration

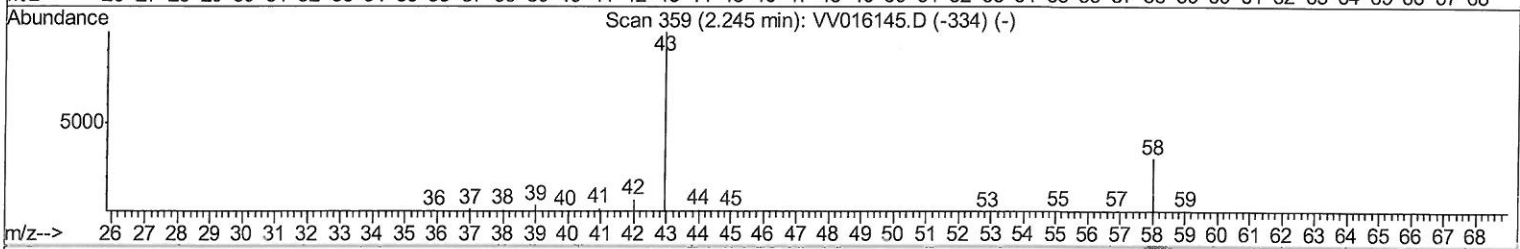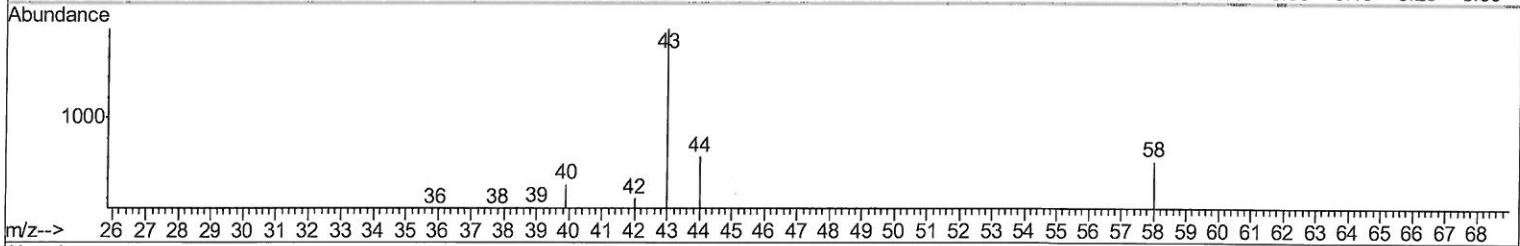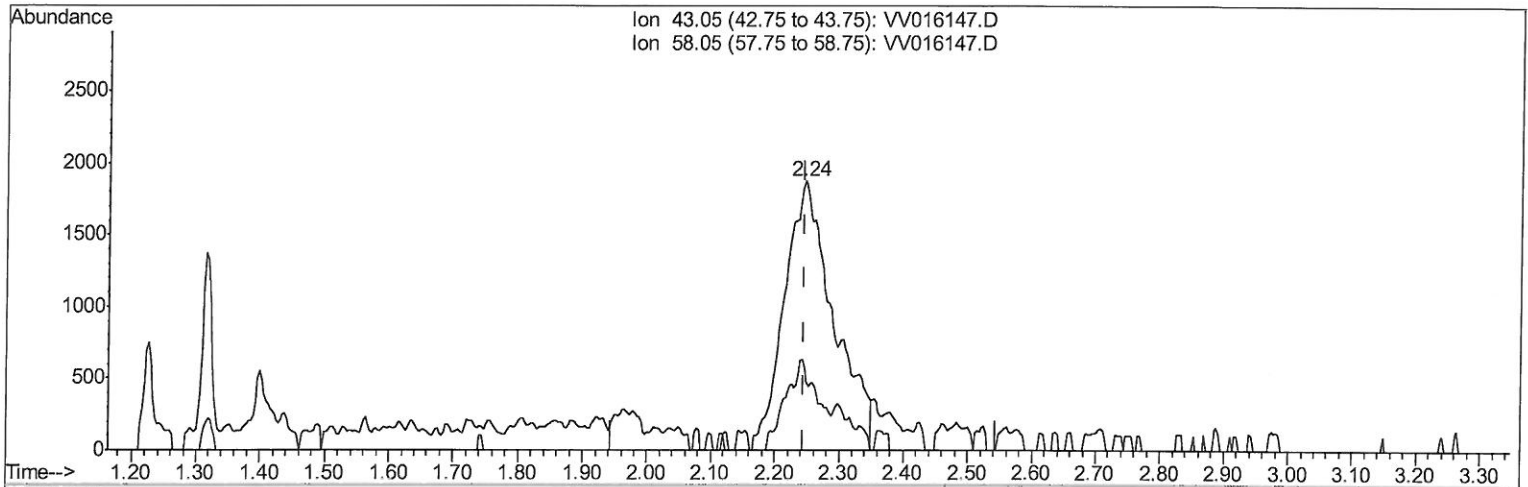

TIC: VV016147.D

(13) Acetone (T)

2.245min (+0.000) 6.61ug/L m

response 9938

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	14.49
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
 05/02/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052120\
 Data File : VV016147.D
 Acq On : 21 May 2020 12:47
 Operator : SY/MD
 Sample : L2725-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 F9B32

Manual Integrations
 APPROVED

apatel
 5/22/2020 11:26:01 AM

Quant Time: May 22 02:51:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 22 01:50:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	147235	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	142573	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	66821	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31231	3.91	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	78.20%		
7) Chloroethane-d5	1.58	69	35292	4.66	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	93.20%		
11) 1,1-Dichloroethene-d2	2.12	63	56855	3.31	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	66.20%		
20) 2-Butanone-d5	3.95	46	89461	39.26	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	78.52%		
24) Chloroform-d	4.38	84	85289	4.88	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.60%		
26) 1,2-Dichloroethane-d4	5.06	65	44304	4.43	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	88.60%		
32) Benzene-d6	5.08	84	160807	4.74	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.80%		
36) 1,2-Dichloropropane-d6	6.09	67	50402	4.87	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.40%		
41) Toluene-d8	7.34	98	139708	4.36	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	87.20%		
45) trans-1,3-Dichloropropene-	7.65	79	14820	3.65	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	73.00%		
48) 2-Hexanone-d5	8.12	63	68129	38.16	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	76.32%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	31998	4.39	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	87.80%		
65) 1,2-Dichlorobenzene-d4	11.65	152	51899	4.79	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	95.80%		

Target Compounds

					Ovalue
13) Acetone	2.24	43	9938m	6.612	ug/L
16) Methylene chloride	2.53	84	1579	0.163	ug/L
42) Toluene	7.41	91	11706	0.308	ug/L
55) m,p-xylene	9.16	106	2262	0.141	ug/L

7m8
 6/02/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed