


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052120\
 Data File : VV016144.D
 Acq On : 21 May 2020 08:51
 Operator : SY/MD
 Sample : BFB61
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 22 01:50:48 2020

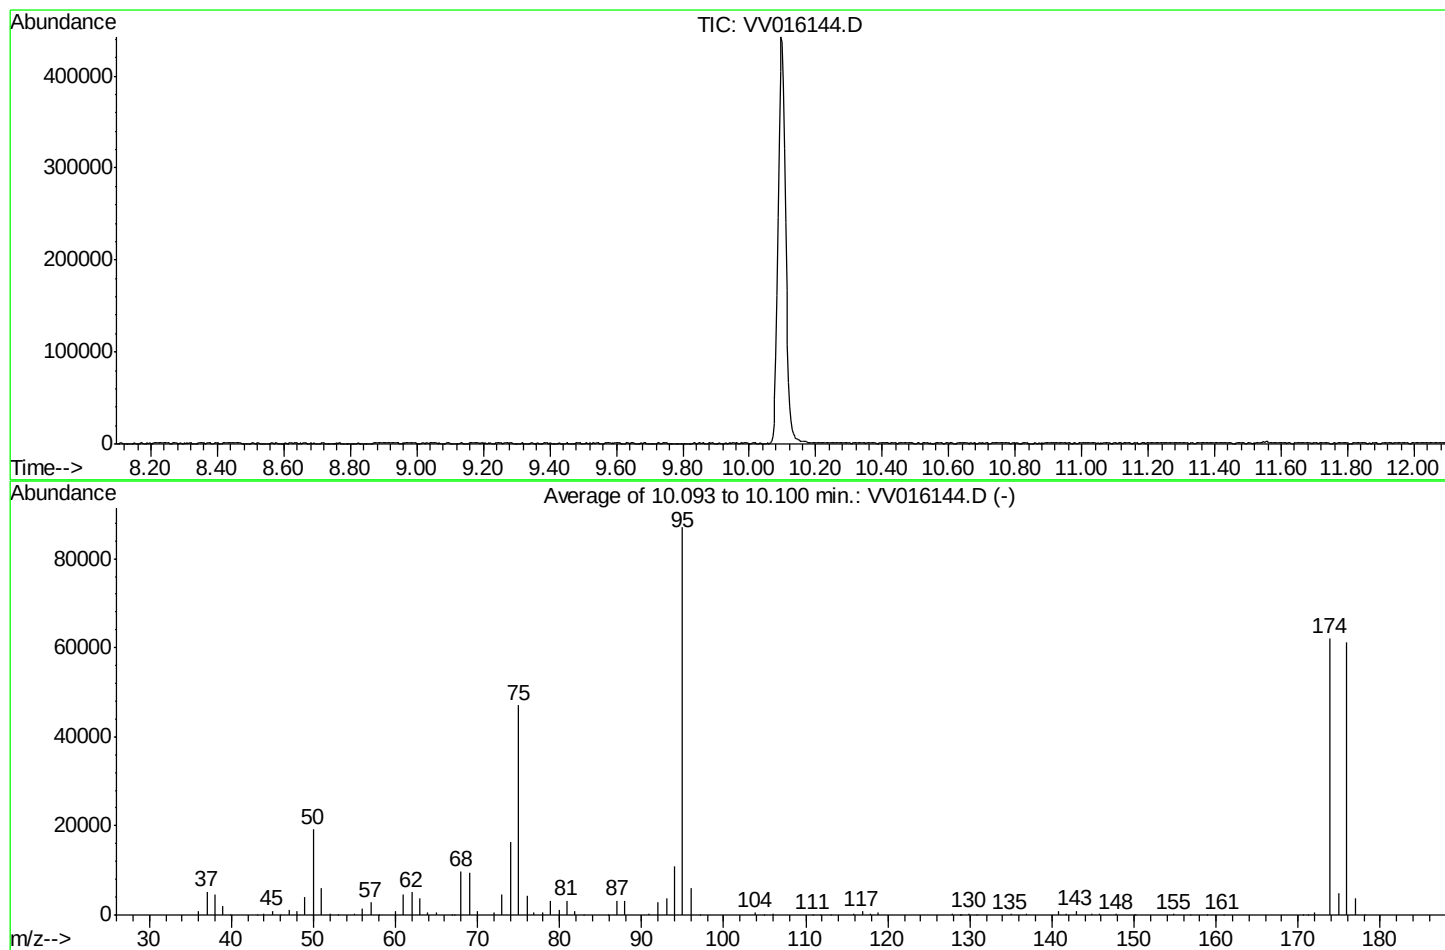

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	19250	PASS
75	95	30	80	54.1	47050	PASS
95	95	100	100	100.0	87013	PASS
96	95	5	9	6.9	6005	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.3	62029	PASS
175	174	5	9	7.9	4874	PASS
176	174	95	101	98.9	61338	PASS
177	176	5	9	6.2	3781	PASS

m/z	Abundance
36.00	942.0
37.00	5159.0
38.00	4470.0
39.00	1952.0
39.90	391.0
44.00	727.0
45.00	1007.0
45.90	119.0
47.00	1090.0
47.90	702.0
49.00	3987.0
50.00	18712.0
51.00	5923.0
52.00	280.0
55.00	302.0
56.00	1513.0
57.00	2720.0
60.00	926.0
61.00	4445.0
62.00	5002.0
63.00	3736.0
64.00	511.0
64.90	506.0
66.80	125.0
68.00	9353.0
69.00	9168.0
70.00	765.0
71.90	511.0
73.00	4352.0
74.00	15251.0
75.00	45064.0
76.00	4316.0
76.90	557.0
77.90	496.0
78.90	3203.0
79.90	1049.0
80.90	3161.0
81.90	770.0
82.90	109.0
86.00	132.0
87.00	3010.0
87.90	2976.0
90.90	317.0
92.00	2723.0
93.00	3583.0
94.00	10538.0
95.00	82368.0
96.00	5762.0
97.20	149.0
103.80	488.0
104.80	120.0
105.90	372.0
110.90	149.0
113.00	108.0
115.90	338.0
116.90	696.0
117.80	386.0
118.80	523.0
127.80	287.0
129.00	116.0
129.90	313.0
130.90	123.0
135.00	225.0
136.90	130.0
140.90	933.0
141.80	192.0
142.90	884.0
144.90	232.0
145.90	162.0
147.90	185.0
150.00	102.0
154.90	308.0
156.90	140.0
158.90	125.0
160.80	104.0
170.60	116.0
171.90	565.0
173.90	57544.0
174.90	4646.0
175.90	55976.0
177.00	3483.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	981.0
37.00	5501.0
38.00	4627.0
39.00	2143.0
39.90	385.0
43.10	111.0
44.00	808.0
45.00	1032.0
45.90	132.0
47.00	1150.0
48.00	793.0
49.00	4236.0
50.00	19840.0
51.00	6260.0
52.00	331.0
53.10	109.0
55.00	363.0
56.00	1580.0
57.00	2956.0
60.00	930.0
61.00	4736.0
62.00	5297.0
63.00	4004.0
63.90	560.0
64.90	535.0
68.00	9958.0
69.00	9783.0
70.00	770.0
71.90	552.0
73.00	4789.0
74.00	16752.0
75.00	48704.0
76.00	4599.0
76.90	627.0
77.90	466.0
78.90	3418.0
79.90	1079.0
80.90	3340.0
81.90	810.0
82.90	118.0
86.00	171.0
87.00	3297.0
88.00	3181.0
90.90	342.0
92.00	2957.0
93.00	3822.0
94.00	11321.0
95.00	89856.0
96.00	6168.0
97.00	129.0
103.90	503.0
104.80	128.0
105.90	392.0
110.80	148.0
111.80	108.0
115.90	393.0
116.90	806.0
117.80	446.0
118.80	605.0
127.80	316.0
128.90	133.0
129.90	365.0
130.90	122.0
134.90	265.0
136.80	167.0
140.80	1040.0
141.80	201.0
142.90	1043.0
144.90	232.0
145.90	175.0
147.80	220.0
154.90	297.0
156.90	155.0
158.90	127.0
160.80	112.0
170.70	125.0
171.20	137.0
171.90	652.0
173.90	64184.0
174.90	5002.0
175.90	63552.0
177.00	3875.0
178.10	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	926.0
37.00	5165.0
38.00	4334.0
39.00	2035.0
39.90	382.0
43.10	133.0
44.00	844.0
45.00	965.0
45.90	125.0
47.00	1122.0
48.00	779.0
49.00	4116.0
50.00	19200.0
51.00	5813.0
52.00	364.0
53.00	125.0
54.90	367.0
56.00	1591.0
57.00	2947.0
58.00	105.0
60.00	871.0
61.00	4596.0
62.00	4957.0
63.00	3788.0
63.90	565.0
65.00	555.0
67.10	205.0
68.00	9682.0
69.00	9511.0
70.00	726.0
72.00	546.0
73.00	4730.0
74.00	16760.0
75.00	47384.0
76.00	4203.0
76.90	655.0
78.00	387.0
78.90	3243.0
79.90	1004.0
80.90	3275.0
81.90	787.0
82.80	130.0
85.90	155.0
87.00	3286.0
88.00	3101.0
90.90	324.0
92.00	2808.0
93.00	3858.0
94.00	11109.0
95.00	88816.0
96.00	6086.0
97.00	142.0
103.90	449.0
104.90	140.0
106.00	396.0
110.80	131.0
111.80	126.0
115.90	385.0
116.90	804.0
117.80	398.0
118.80	620.0
127.80	329.0
128.70	156.0
129.90	372.0
130.80	131.0
134.90	236.0
136.80	189.0
140.80	1052.0
141.80	172.0
142.90	1097.0
144.80	222.0
145.80	169.0
147.80	247.0
150.20	104.0
154.90	222.0
156.90	152.0
158.90	143.0
160.90	134.0
170.70	115.0
171.20	130.0
172.00	729.0
173.90	64360.0
175.00	4974.0
175.90	64488.0
177.00	3987.0
178.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Scan 2788 (10.055 min): VV016144.D
BFB61

m/z	Abundance
35.70	101.0
39.90	313.0
43.90	410.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61