

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
 Data File : VV021370.D
 Acq On : 21 May 2021 19:49
 Operator : SY/MD
 Sample : M2494-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB429

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	126848	133584	13.71%	1.614%
2	1.413	111	116	126	rVB	33856	38624	3.97%	0.467%
3	1.568	157	164	182	rVB	112262	128462	13.19%	1.552%
4	2.108	322	332	345	rBV	205452	298338	30.63%	3.605%
5	3.899	876	889	947	rBV3	124848	479184	49.19%	5.790%
6	4.352	1013	1030	1050	rBV2	158408	399699	41.03%	4.829%
7	5.050	1231	1247	1272	rBV2	385060	955371	98.08%	11.543%
8	5.622	1412	1425	1452	rBV	299822	617450	63.39%	7.460%
9	5.911	1502	1515	1531	rBV	26116	56581	5.81%	0.684%
10	6.072	1552	1565	1595	rBV	218069	453383	46.54%	5.478%
11	6.992	1839	1851	1871	rBV	119120	226686	23.27%	2.739%
12	7.320	1940	1953	1971	rBV	481070	843640	86.61%	10.193%
13	7.400	1972	1978	1990	rVB2	8144	15965	1.64%	0.193%
14	7.628	2038	2049	2067	rBV	71215	131706	13.52%	1.591%
15	8.091	2181	2193	2238	rBV2	432429	974099	100.00%	11.769%
16	8.853	2419	2430	2459	rBV	441751	735408	75.50%	8.885%
17	10.217	2843	2854	2869	rBV	131587	210244	21.58%	2.540%
18	10.381	2896	2905	2915	rVB	11537	20365	2.09%	0.246%
19	11.249	3164	3175	3204	rBV	490202	783598	80.44%	9.467%
20	11.625	3279	3292	3312	rVV	481504	774365	79.50%	9.356%




Sum of corrected areas: 8276752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021370.D
Acq On : 21 May 2021 19:49
Operator : SY/MD
Sample : M2494-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB429

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

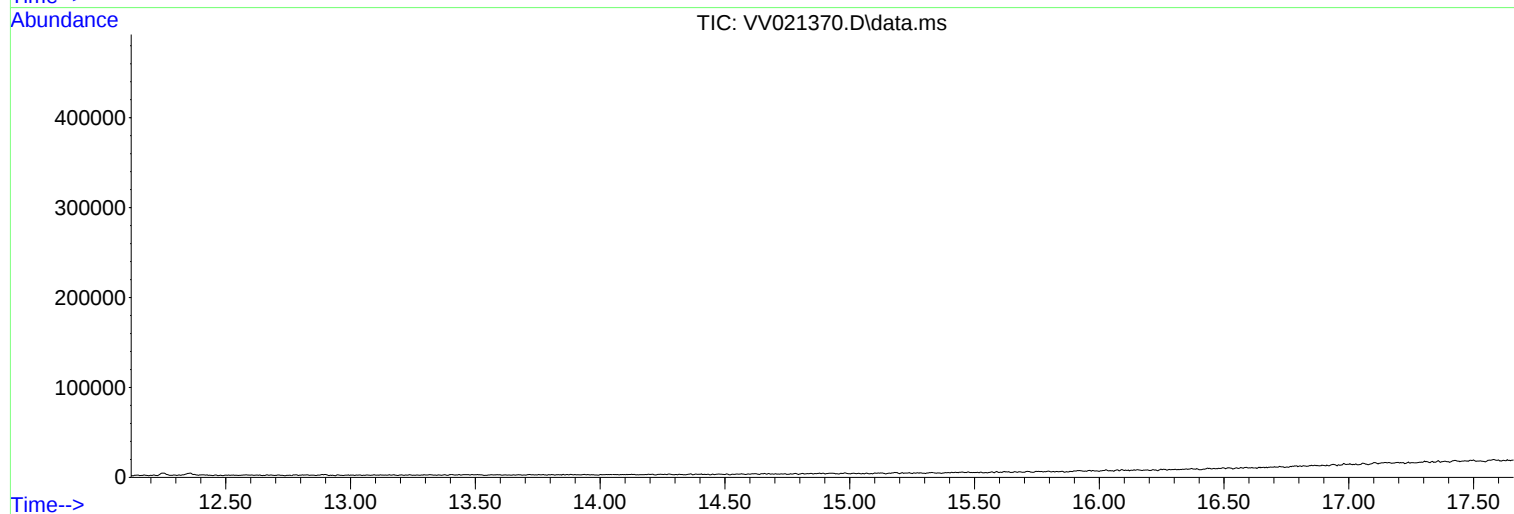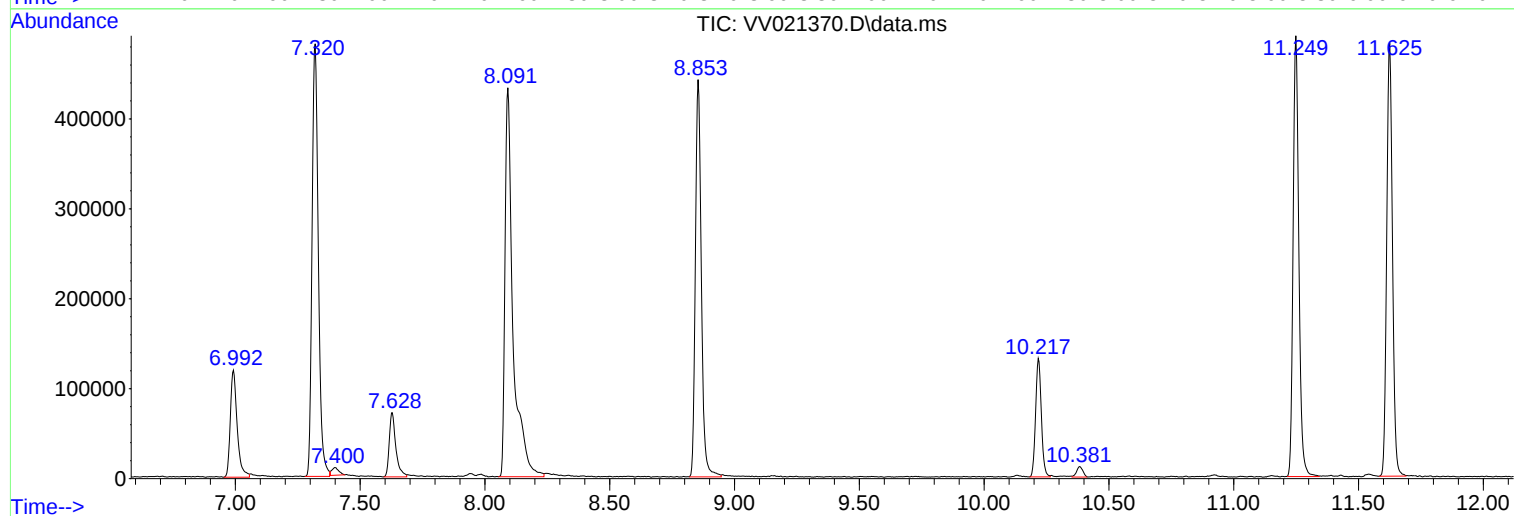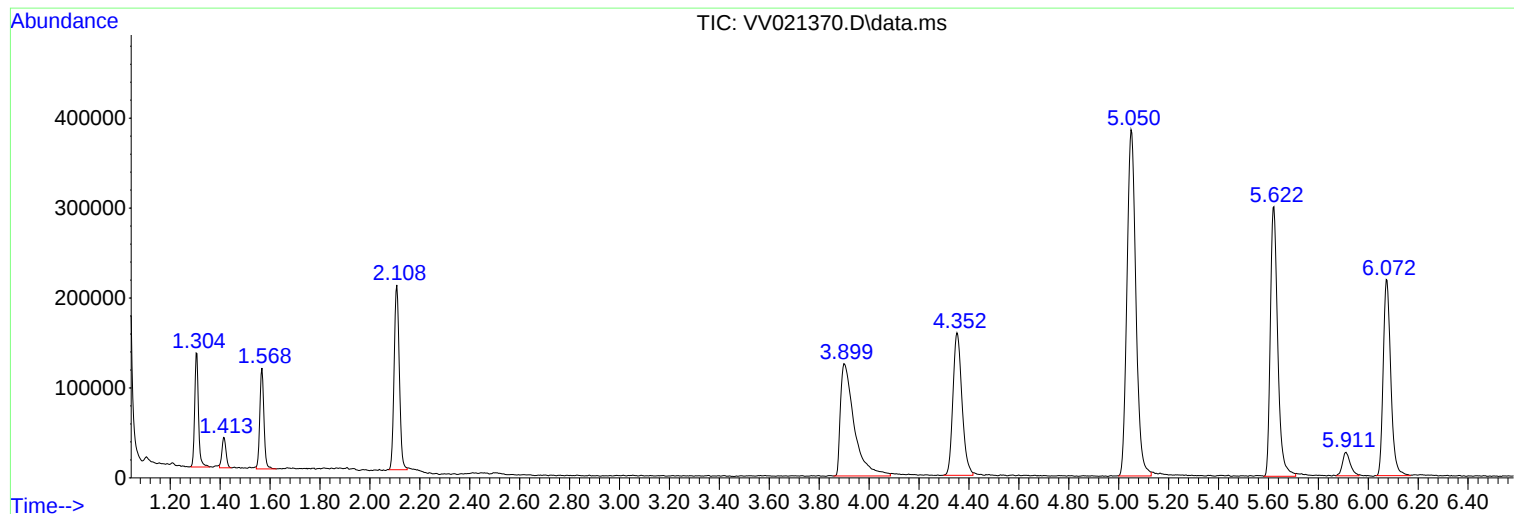

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021370.D
Acq On : 21 May 2021 19:49
Operator : SY/MD
Sample : M2494-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB429

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021370.D
Acq On : 21 May 2021 19:49
Operator : SY/MD
Sample : M2494-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB429

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
