

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
 Data File : VV021371.D
 Acq On : 21 May 2021 20:13
 Operator : SY/MD
 Sample : M2494-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB432

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV021371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	60	rVB3	16666	17389	1.88%	0.223%
2	1.304	75	82	97	rVB	121477	122823	13.29%	1.574%
3	1.565	156	163	177	rVB	103271	118669	12.84%	1.520%
4	2.108	320	332	350	rBV	199361	299216	32.38%	3.833%
5	3.905	880	891	928	rBV	94323	354631	38.38%	4.543%
6	4.352	1012	1030	1057	rBV	153603	381709	41.31%	4.890%
7	5.050	1228	1247	1276	rBV2	365396	908902	98.37%	11.644%
8	5.619	1412	1424	1457	rBV	292887	606534	65.64%	7.770%
9	5.908	1499	1514	1534	rBV3	24887	57817	6.26%	0.741%
10	6.072	1551	1565	1594	rBV	206567	431393	46.69%	5.527%
11	6.992	1838	1851	1872	rBV	112981	214211	23.18%	2.744%
12	7.320	1940	1953	1971	rBV	454995	801100	86.70%	10.263%
13	7.400	1973	1978	1992	rVB3	9291	17954	1.94%	0.230%
14	7.629	2036	2049	2074	rBV2	66323	127906	13.84%	1.639%
15	8.092	2182	2193	2229	rBV2	418168	923982	100.00%	11.837%
16	8.854	2418	2430	2452	rBV	435949	716620	77.56%	9.181%
17	10.217	2843	2854	2871	rBV	123665	198159	21.45%	2.539%
18	10.384	2897	2906	2917	rVB2	7614	12382	1.34%	0.159%
19	11.249	3161	3175	3202	rBV	480869	762709	82.55%	9.771%
20	11.625	3278	3292	3313	rBV	449450	731604	79.18%	9.373%




Sum of corrected areas: 7805710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021371.D
Acq On : 21 May 2021 20:13
Operator : SY/MD
Sample : M2494-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB432

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

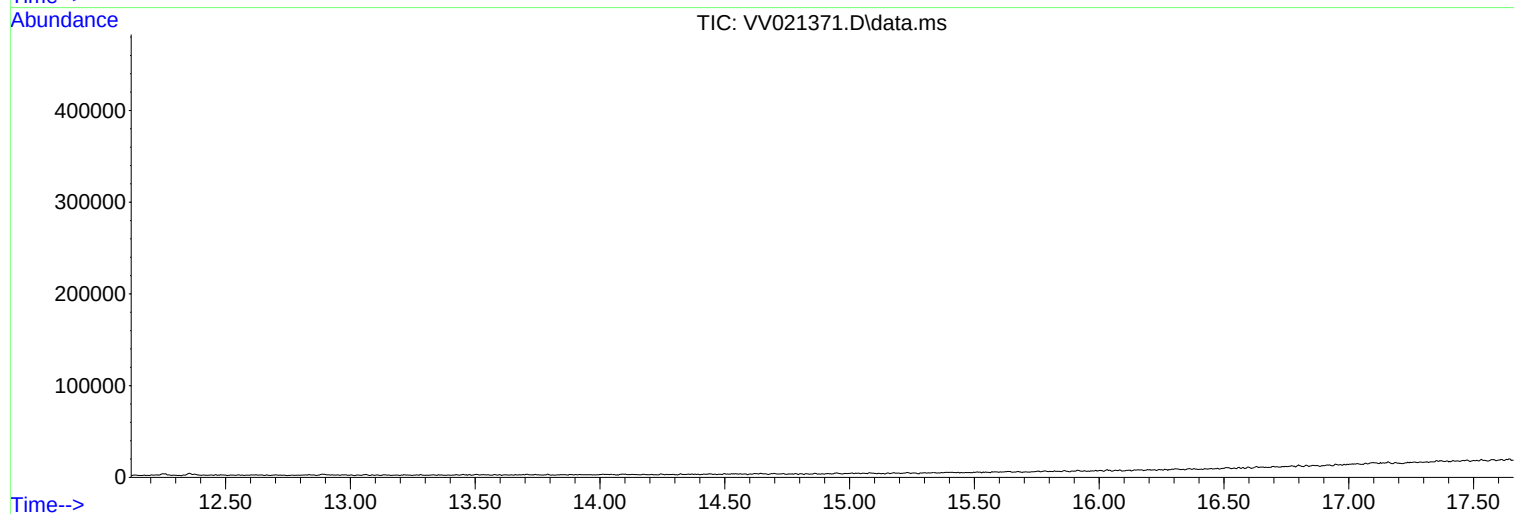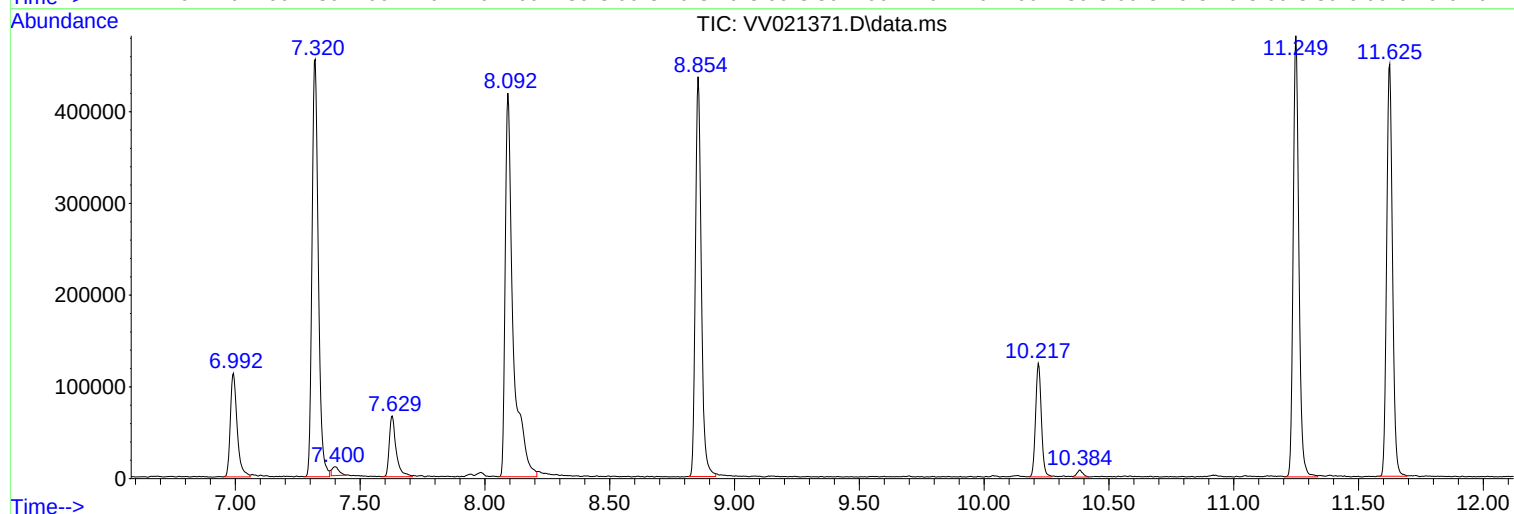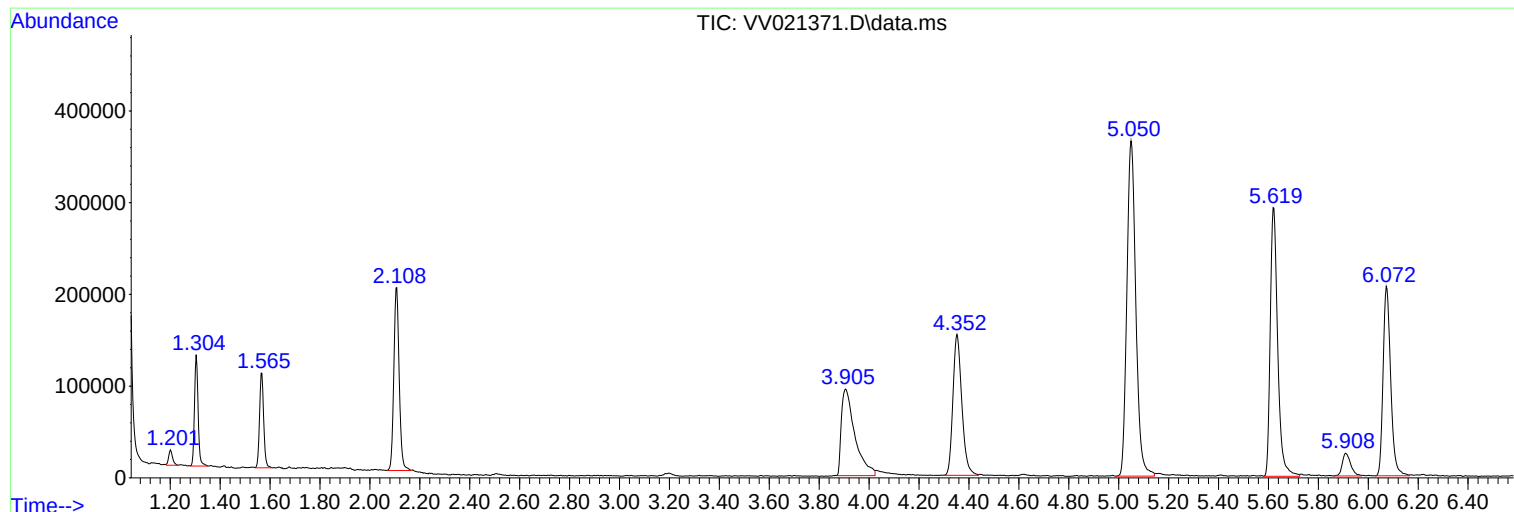

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021371.D
Acq On : 21 May 2021 20:13
Operator : SY/MD
Sample : M2494-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB432

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
Data File : VV021371.D
Acq On : 21 May 2021 20:13
Operator : SY/MD
Sample : M2494-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB432

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
