
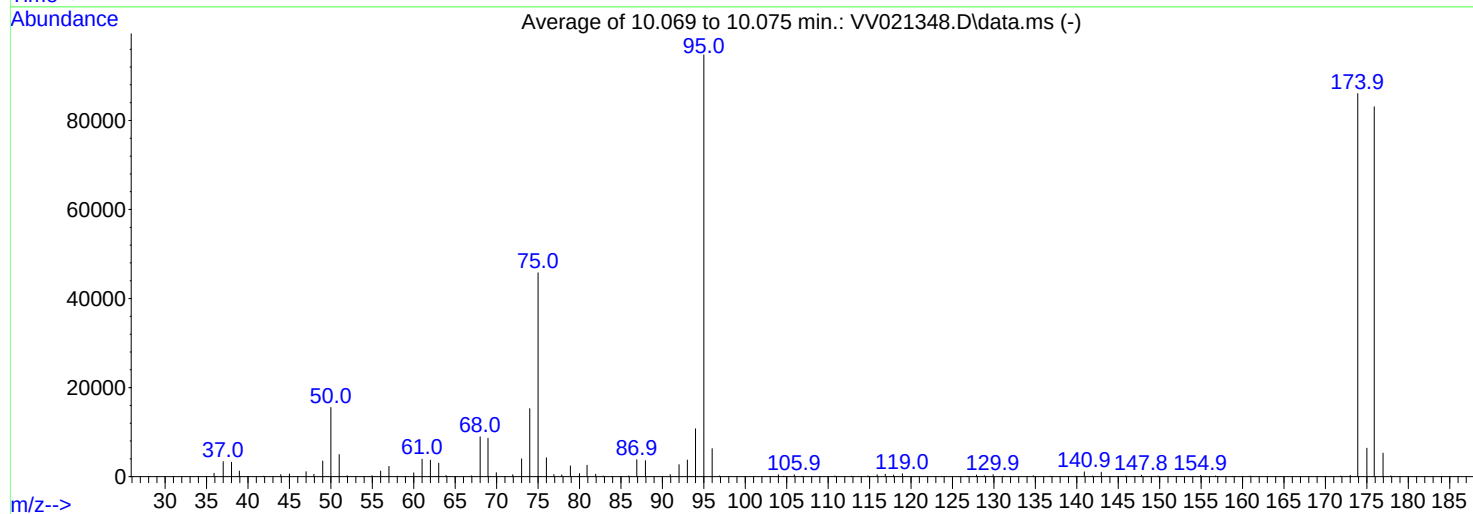


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052121\
 Data File : VV021348.D
 Acq On : 21 May 2021 09:25
 Operator : SY/MD
 Sample : BFB98
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB98

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 21 12:12:53 2021

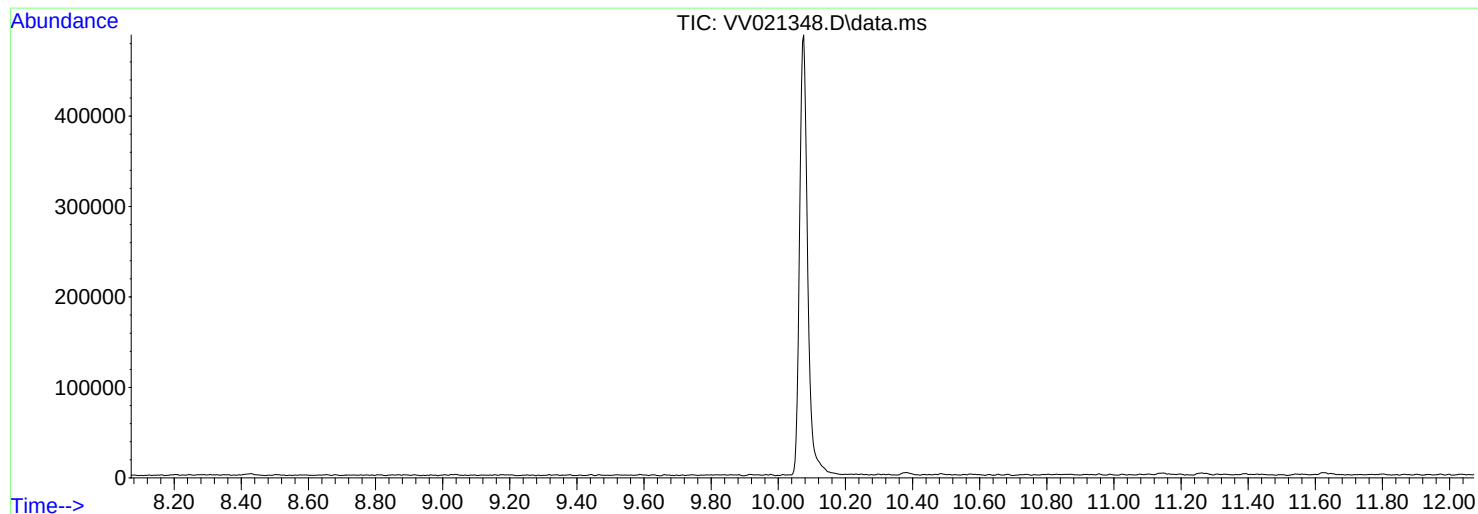

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	15534	PASS
75	95	30	80	48.3	45771	PASS
95	95	100	100	100.0	94741	PASS
96	95	5	9	6.6	6294	PASS
173	174	0.00	2	0.3	276	PASS
174	95	50	120	90.8	86035	PASS
175	174	5	9	7.4	6402	PASS
176	174	95	105	96.6	83077	PASS
177	176	5	10	6.3	5270	PASS

m/z	Abundance
35.90	808.0
37.00	3419.0
38.00	3211.0
39.00	1424.0
39.90	299.0
41.00	255.0
41.90	138.0
42.90	292.0
44.00	1317.0
45.00	780.0
46.00	104.0
47.00	1292.0
47.90	539.0
49.00	3586.0
50.00	16094.0
51.00	5210.0
51.90	257.0
54.90	443.0
56.00	1307.0
57.00	2487.0
58.00	122.0
60.10	898.0
61.00	4119.0
62.00	3617.0
63.00	3090.0
63.90	277.0
67.10	353.0
68.00	9213.0
69.00	8875.0
70.00	911.0
71.00	118.0
71.90	452.0
73.00	4248.0
74.00	15765.0
75.00	47384.0
76.00	4239.0
77.00	650.0
77.90	413.0
78.90	2510.0
80.00	681.0
80.90	2730.0
82.00	544.0
82.90	158.0
83.90	112.0
86.00	174.0
86.90	3929.0
88.00	3822.0
90.90	499.0
92.00	2850.0
93.00	3923.0
94.00	10977.0
95.00	97872.0
96.00	6414.0
96.90	268.0
104.00	448.0
104.80	131.0
105.90	464.0
106.90	110.0
110.80	144.0
111.90	110.0
112.80	114.0
114.80	193.0
115.90	394.0
116.90	559.0
117.90	397.0
119.00	597.0
127.90	386.0
128.90	257.0
129.90	533.0
131.10	115.0
134.80	193.0
136.70	109.0
139.90	151.0
140.90	1139.0
141.80	183.0
142.90	1057.0
145.80	170.0
146.80	130.0
147.80	333.0
149.80	145.0
154.90	318.0
156.70	187.0
159.10	110.0
160.90	165.0
171.90	146.0
173.00	828.0
173.90	92264.0
175.00	6925.0
175.90	88752.0
177.00	5708.0
177.90	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.90	800.0
37.00	3494.0
38.00	3365.0
39.00	1464.0
39.80	333.0
41.00	196.0
41.90	128.0
42.90	276.0
44.00	1294.0
45.00	712.0
47.00	1170.0
47.90	544.0
49.00	3646.0
50.00	16109.0
51.00	5112.0
51.90	241.0
52.90	115.0
55.00	400.0
56.00	1282.0
57.00	2570.0
58.00	125.0
60.00	862.0
61.00	4070.0
62.00	3799.0
63.00	3168.0
63.90	289.0
67.00	305.0
68.00	9354.0
69.00	9018.0
70.00	927.0
71.90	448.0
73.00	4121.0
74.00	15704.0
75.00	47472.0
76.00	4401.0
77.00	582.0
77.80	435.0
78.90	2471.0
80.00	719.0
80.90	2672.0
82.00	534.0
82.90	149.0
86.00	180.0
86.90	3876.0
88.00	3717.0
90.90	488.0
92.00	2803.0
93.00	3834.0
94.00	11075.0
95.00	97904.0
96.00	6509.0
96.90	302.0
104.00	435.0
104.70	148.0
105.90	457.0
106.90	110.0
110.80	174.0
112.00	110.0
112.80	117.0
114.80	203.0
115.90	452.0
116.90	548.0
117.90	352.0
118.90	721.0
123.70	105.0
126.80	114.0
127.90	343.0
128.90	250.0
129.90	504.0
131.10	113.0
134.80	208.0
136.80	109.0
137.10	110.0
139.90	126.0
140.90	1123.0
141.90	152.0
143.00	1030.0
143.90	108.0
145.90	131.0
147.80	335.0
149.80	165.0
155.00	317.0
156.80	208.0
158.80	105.0
160.90	163.0
171.80	143.0
173.90	89056.0
175.00	6554.0
175.90	85664.0
176.90	5364.0
177.90	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
38.90	158.0
40.00	254.0
41.00	381.0
42.30	119.0
43.10	294.0
43.90	823.0
45.10	104.0
53.90	102.0
55.10	199.0
57.00	144.0
66.90	118.0
68.10	111.0
68.90	113.0
76.90	108.0
85.10	126.0
96.90	100.0
207.00	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
35.90	690.0
37.00	3254.0
38.00	3107.0
39.00	1369.0
39.80	337.0
40.90	194.0
41.90	113.0
42.30	120.0
43.00	278.0
44.00	1225.0
45.00	633.0
47.00	906.0
48.00	499.0
49.00	3309.0
50.00	14400.0
51.00	4578.0
52.00	196.0
53.00	132.0
55.00	397.0
56.00	1202.0
57.00	2289.0
58.00	128.0
59.90	810.0
61.00	3523.0
62.00	3676.0
63.00	2809.0
63.90	246.0
66.90	293.0
68.00	8615.0
69.00	8322.0
69.90	834.0
72.00	427.0
73.00	3652.0
74.00	14320.0
75.00	42456.0
76.00	4052.0
76.90	508.0
77.80	389.0
78.90	2210.0
80.00	672.0
80.90	2309.0
81.90	511.0
82.80	124.0
85.90	146.0
86.90	3632.0
87.90	3255.0
91.00	429.0
92.00	2473.0
93.00	3436.0
94.00	10239.0
95.00	88448.0
96.00	5959.0
96.90	293.0
104.00	370.0
104.60	140.0
105.00	140.0
105.90	410.0
106.80	106.0
110.80	168.0
112.80	118.0
114.80	169.0
115.90	440.0
116.90	502.0
117.90	292.0
118.90	667.0
126.80	121.0
127.90	309.0
128.80	189.0
129.90	392.0
131.10	100.0
134.70	209.0
136.90	124.0
140.90	935.0
142.10	125.0
143.00	933.0
143.90	108.0
146.00	130.0
147.80	269.0
149.80	140.0
155.00	268.0
156.80	179.0
158.70	113.0
160.90	155.0
171.80	133.0
173.90	76784.0
175.00	5728.0
175.90	74816.0
176.90	4737.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98