

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
 Data File : VV035647.D
 Acq On : 21 May 2024 18:44
 Operator : SY/MD
 Sample : P2547-07
 Misc : 3.51g/10.0mL/MSVOA_V/SOIL/VIAL A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q0

Quant Time: May 22 02:38:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 22 02:35:18 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
 Supervised By :Semsettin Yesilyurt 05/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	252772	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	217776	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	58835	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	95664	24.486	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.960%		
7) Chloroethane-d5	1.529	69	87372	27.721	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	110.880%		
11) 1,1-Dichloroethene-d2	2.053	65	42288	24.449	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	97.800%		
21) 2-Butanone-d5	3.847	46	50304m	45.370	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.740%		
24) Chloroform-d	4.249	84	214398	28.530	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	114.120%		
26) 1,2-Dichloroethane-d4	4.944	65	111768	30.085	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	120.360%		
32) Benzene-d6	4.960	84	357471	29.987	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	119.960%		
36) 1,2-Dichloropropane-d6	5.989	67	126877	34.488	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	137.960%#		
41) Toluene-d8	7.243	98	246636	23.246	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.000%		
43) trans-1,3-Dichloroprop...	7.558	79	35288	22.428	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.720%		
47) 2-Hexanone-d5	8.037	63	23922	36.162	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.320%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	97114	27.394	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	109.560%		
66) 1,2-Dichlorobenzene-d4	11.561	152	52815	25.866	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.480%		
Target Compounds						Qvalue
16) Methylene chloride	2.445	84	45280	7.768	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
Data File : VV035647.D
Acq On : 21 May 2024 18:44
Operator : SY/MD
Sample : P2547-07
Misc : 3.51g/10.0mL/MSVOA_V/SOIL/VIAL A
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH5Q0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024


Quant Time: May 22 02:38:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 22 02:35:18 2024
Response via : Initial Calibration

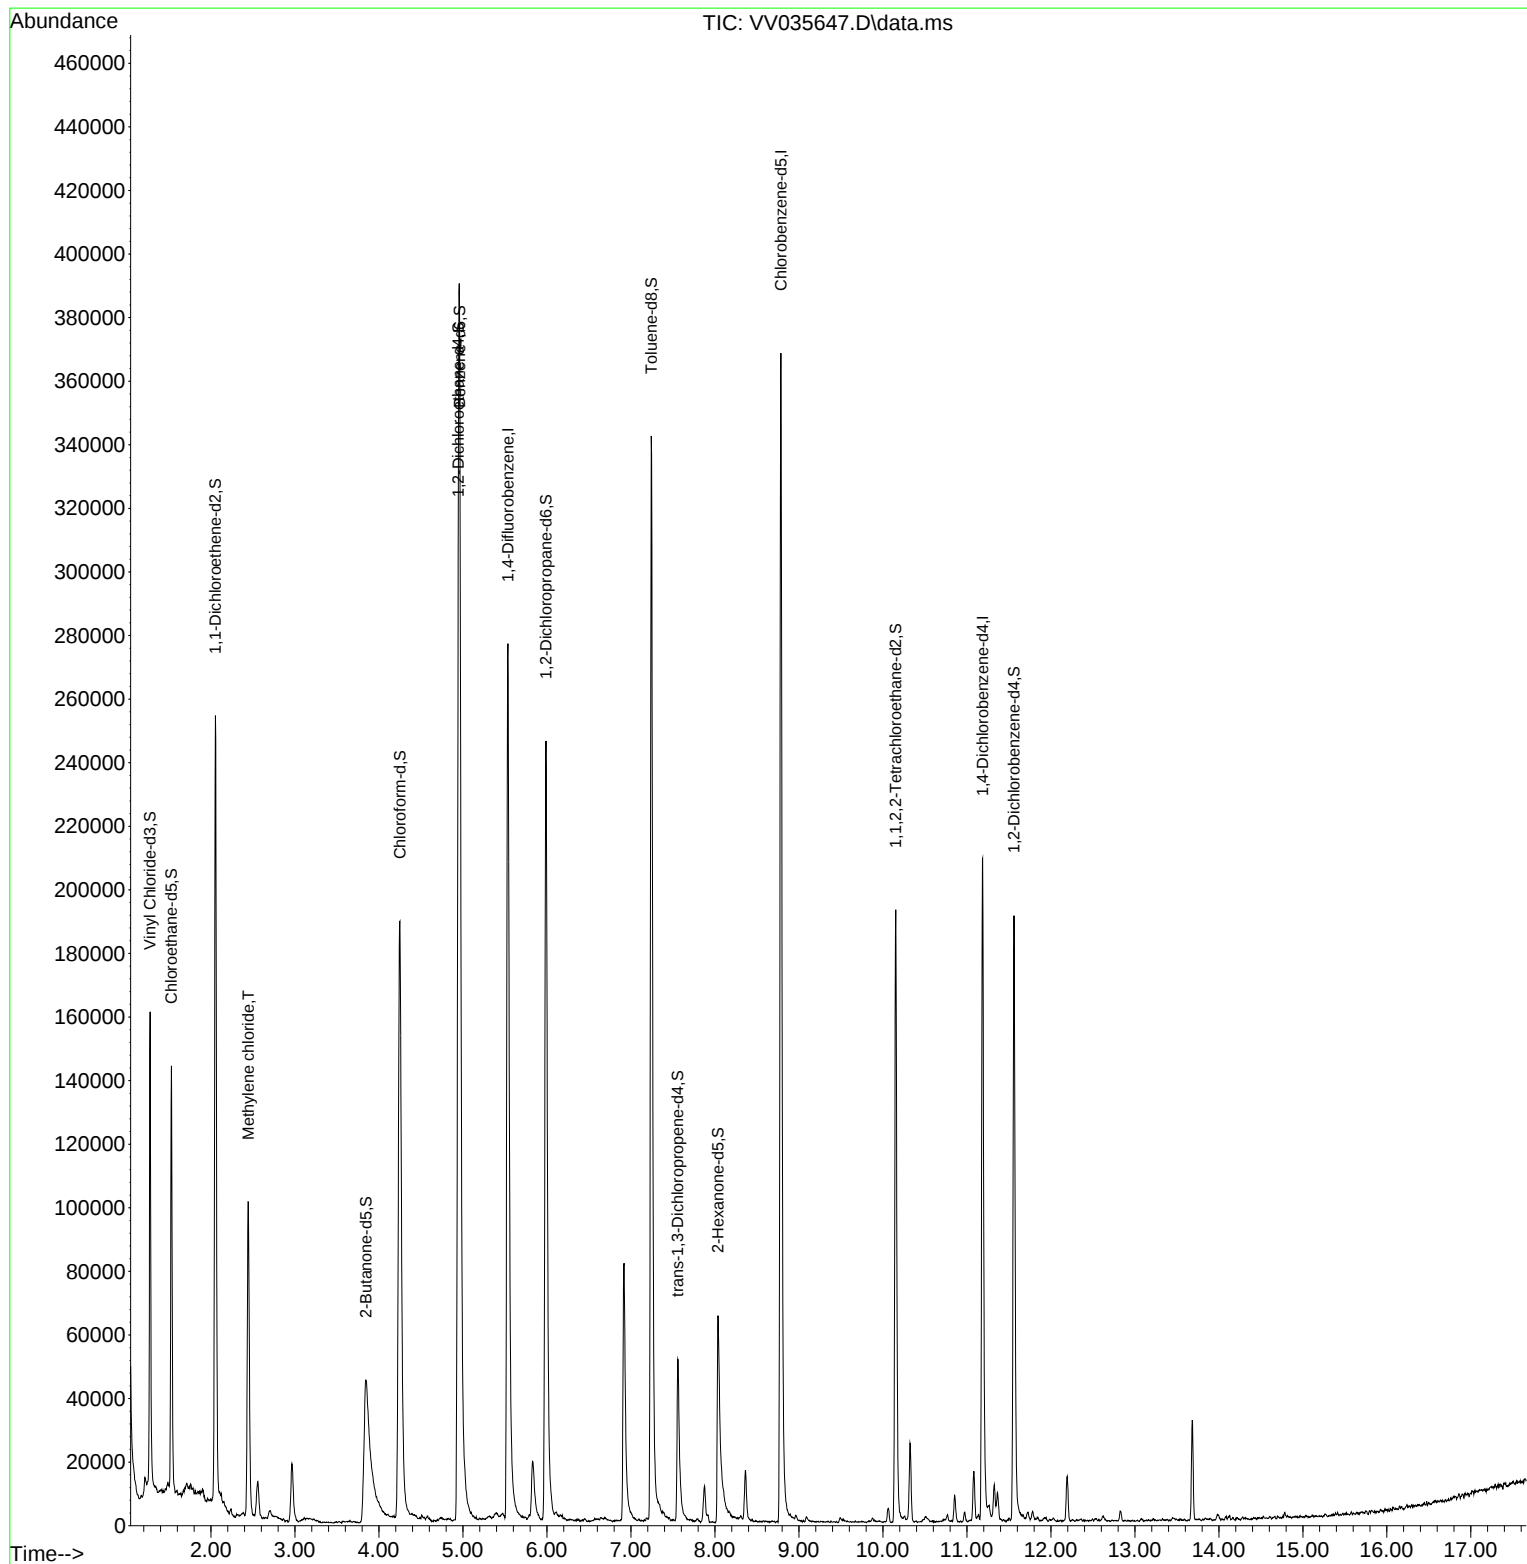

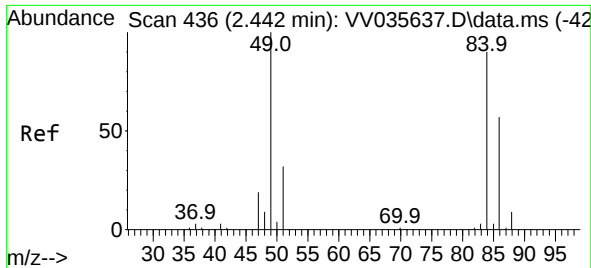

#16
Methylene chloride
Concen: 7.768 ug/L
RT: 2.445 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV035647.D
Acq: 21 May 2024 18:44

Instrument :
MSVOA_V
ClientSampleId :
BH5Q0

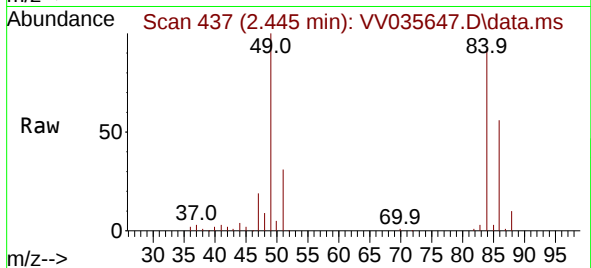

Tgt Ion: 84 Resp: 45280
Ion Ratio Lower Upper
84 100
86 61.0 43.8 81.3
49 109.2 75.3 139.9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024

