

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
 Data File : VV035648.D
 Acq On : 21 May 2024 19:07
 Operator : SY/MD
 Sample : P2547-08
 Misc : 5.59g/10.0mL/MSVOA_V/SOIL/VIAL A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q1

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
 Supervised By :Semsettin Yesilyurt 05/24/2024

Quant Time: May 22 02:38:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 22 02:35:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	243884	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	210955	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	56653	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	91815	24.357	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.440%		
7) Chloroethane-d5	1.526	69	85448	28.099	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	112.400%		
11) 1,1-Dichloroethene-d2	2.053	65	41198	24.687	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	98.760%		
21) 2-Butanone-d5	3.854	46	55908m	52.262	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.520%		
24) Chloroform-d	4.246	84	215516	29.724	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	118.880%		
26) 1,2-Dichloroethane-d4	4.940	65	117248	32.711	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	130.840%#		
32) Benzene-d6	4.956	84	355857	30.816	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	123.280%		
36) 1,2-Dichloropropane-d6	5.989	67	132802	37.266	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	149.080%#		
41) Toluene-d8	7.243	98	245294	23.867	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	95.480%		
43) trans-1,3-Dichloroprop...	7.558	79	38467	25.239	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	100.960%		
47) 2-Hexanone-d5	8.037	63	27987	43.675	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.340%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	111526	32.477	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	129.920%#		
66) 1,2-Dichlorobenzene-d4	11.561	152	52831	26.871	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.480%		
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	47892	8.516	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
Data File : VV035648.D
Acq On : 21 May 2024 19:07
Operator : SY/MD
Sample : P2547-08
Misc : 5.59g/10.0mL/MSVOA_V/SOIL/VIAL A
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH5Q1

Quant Time: May 22 02:38:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 22 02:35:18 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024

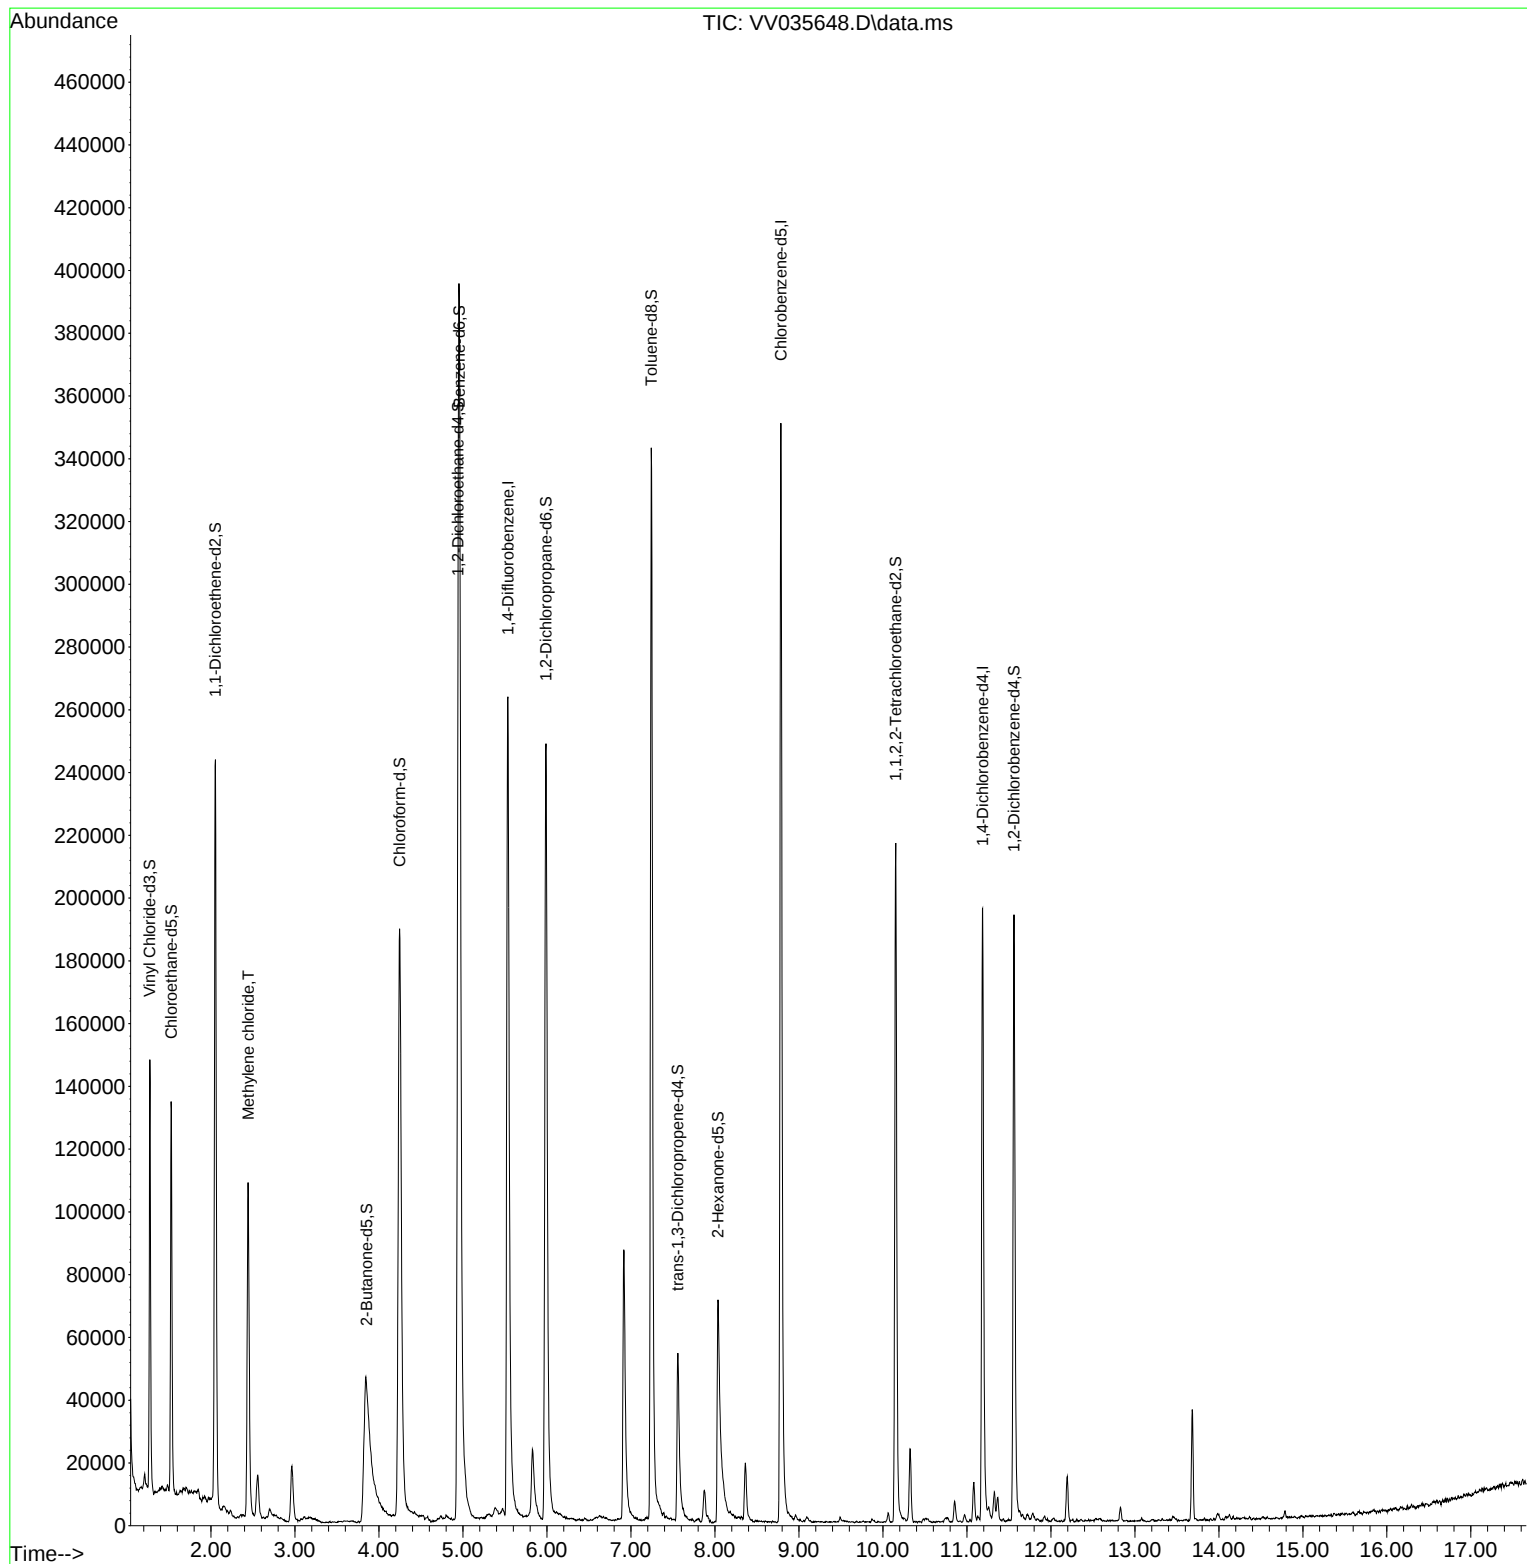

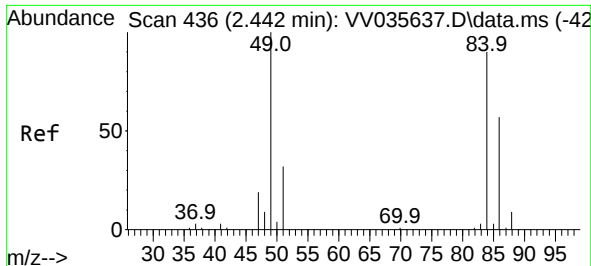

#16
Methylene chloride
Concen: 8.516 ug/L
RT: 2.442 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV035648.D
Acq: 21 May 2024 19:07

Instrument :
MSVOA_V
ClientSampleId :
BH5Q1

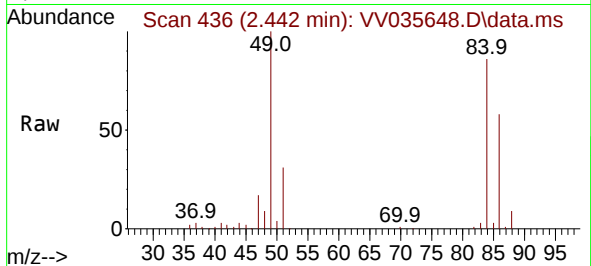

Tgt Ion: 84 Resp: 47892
Ion Ratio Lower Upper
84 100
86 66.5 43.8 81.3
49 115.6 75.3 139.9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024

