

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
 Data File : VV035655.D
 Acq On : 21 May 2024 21:47
 Operator : SY/MD
 Sample : P2547-15
 Misc : 5.25g/10.0mL/MSVOA_V/SOIL/VIAL A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5X2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
 Supervised By :Semsettin Yesilyurt 05/24/2024

Quant Time: May 22 02:40:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 22 02:35:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	277541	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	315469	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	140741	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	88920	20.729	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.920%		
7) Chloroethane-d5	1.526	69	84524	24.424	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.680%		
11) 1,1-Dichloroethene-d2	2.053	65	43236	22.766	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	91.080%		
21) 2-Butanone-d5	3.847	46	60337m	49.563	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.120%		
24) Chloroform-d	4.246	84	223732	27.115	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	108.480%		
26) 1,2-Dichloroethane-d4	4.941	65	116439	28.546	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	114.200%		
32) Benzene-d6	4.957	84	386993	22.410	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.640%		
36) 1,2-Dichloropropane-d6	5.986	67	136893	25.687	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.760%		
41) Toluene-d8	7.243	98	303401	19.741	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.960%		
43) trans-1,3-Dichloroprop...	7.558	79	46078	20.217	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.880%		
47) 2-Hexanone-d5	8.037	63	30565	31.896	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	63.800%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	121701	23.699	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.800%		
66) 1,2-Dichlorobenzene-d4	11.558	152	129927	26.601	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	106.400%		
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	76385	11.935	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052124\
Data File : VV035655.D
Acq On : 21 May 2024 21:47
Operator : SY/MD
Sample : P2547-15
Misc : 5.25g/10.0mL/MSVOA_V/SOIL/VIAL A
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH5X2

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024


Quant Time: May 22 02:40:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 22 02:35:18 2024
Response via : Initial Calibration

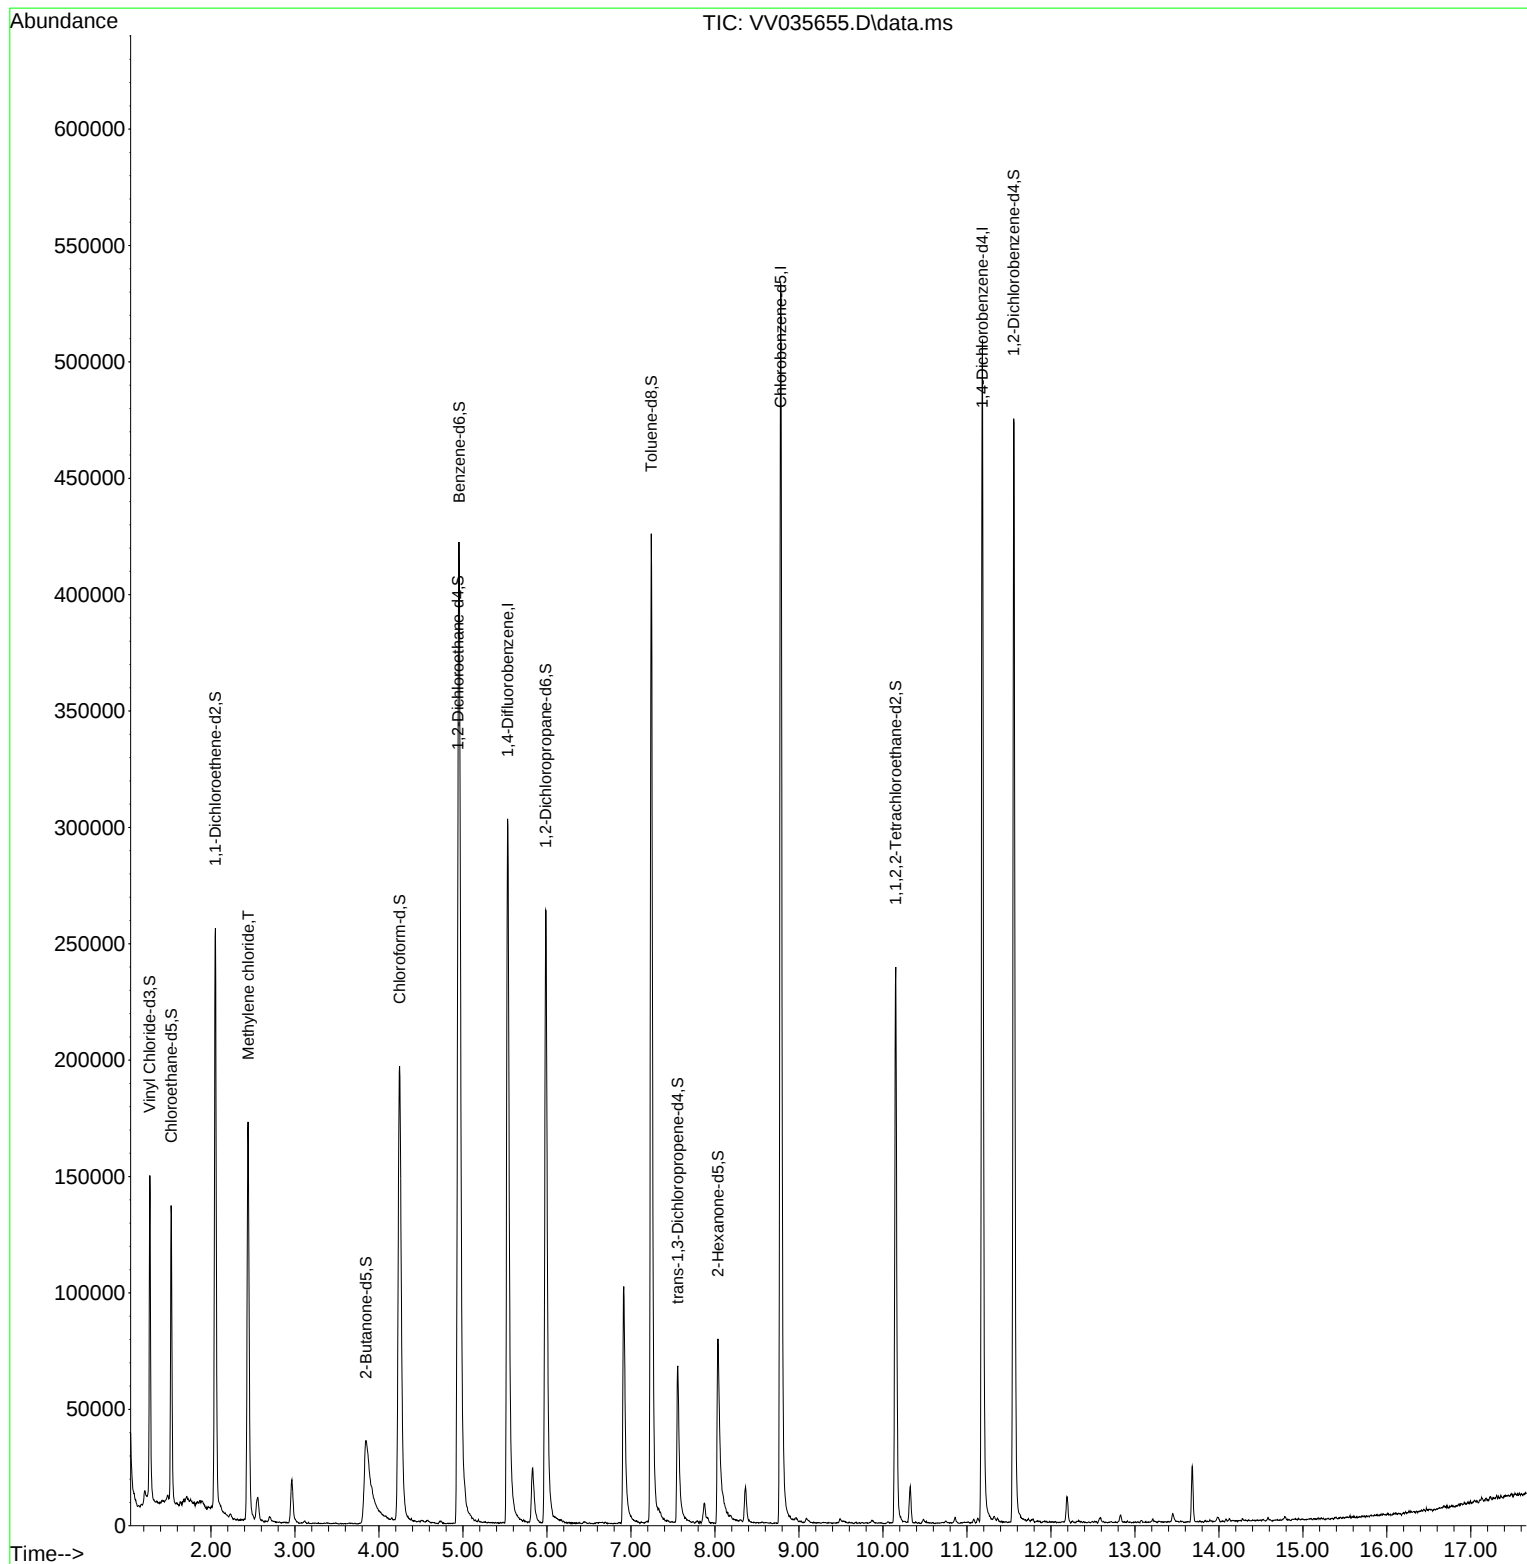

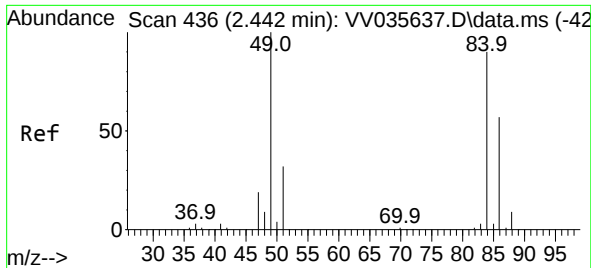

#16
Methylene chloride
Concen: 11.935 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV035655.D
Acq: 21 May 2024 21:47

Instrument :
MSVOA_V
ClientSampleId :
BH5X2

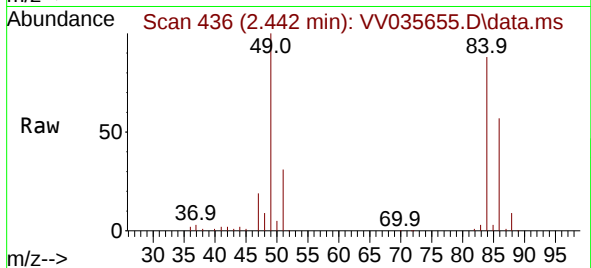

Tgt Ion: 84 Resp: 7638
Ion Ratio Lower Upper
84 100
86 64.7 43.8 81.3
49 113.5 75.3 139.9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 05/24/2024
Supervised By :Semsettin Yesilyurt 05/24/2024

