


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052219\
Data File : VV011006.D
Acq On : 22 May 2019 09:02
Operator : SY/MD
Sample : BFB61
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
Title : VOC Analysis
Last Update : Thu May 23 08:00:26 2019

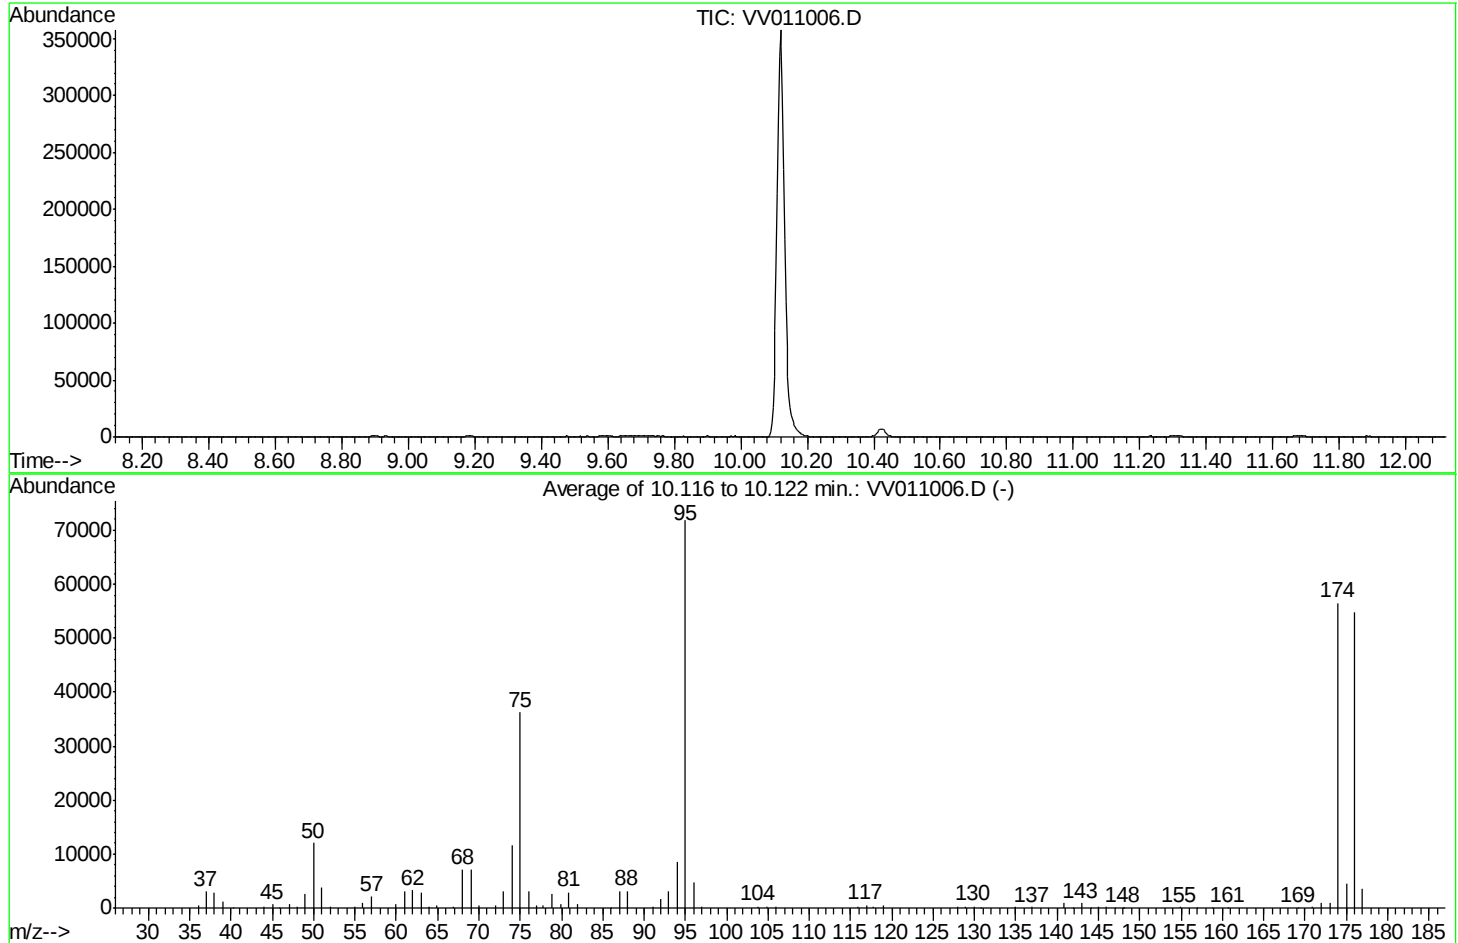

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	11989	PASS
75	95	30	80	50.4	36192	PASS
95	95	100	100	100.0	71837	PASS
96	95	5	9	6.7	4780	PASS
173	174	0.00	2	1.5	843	PASS
174	95	50	120	78.6	56482	PASS
175	174	5	9	7.8	4397	PASS
176	174	95	101	97.2	54898	PASS
177	176	5	9	6.7	3672	PASS

Scan 2795 (10.077 min): VV011006.D
BFB61

m/z	Abundance
39.90	132.0
44.00	178.0
168.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	516.0
37.00	2904.0
38.00	2836.0
39.00	1234.0
39.90	180.0
44.00	524.0
45.00	704.0
45.80	117.0
47.00	792.0
47.90	333.0
49.00	2545.0
50.00	11697.0
51.00	3837.0
52.00	193.0
54.90	222.0
55.90	1070.0
57.00	2153.0
60.00	725.0
61.10	3094.0
62.00	3318.0
63.00	2809.0
63.90	265.0
64.90	616.0
67.00	177.0
68.00	6816.0
69.00	7076.0
70.00	600.0
71.90	408.0
73.00	3188.0
74.00	11445.0
75.00	35280.0
76.00	3060.0
77.00	410.0
77.80	373.0
78.90	2407.0
79.90	849.0
80.90	2902.0
81.90	719.0
86.00	172.0
87.00	2956.0
88.00	3011.0
91.00	268.0
92.00	1697.0
93.00	2963.0
94.00	8272.0
95.00	69856.0
96.00	4747.0
97.00	160.0
103.80	339.0
104.80	111.0
105.90	288.0
115.90	253.0
116.90	497.0
117.80	284.0
119.00	525.0
127.90	233.0
128.90	128.0
130.00	258.0
130.80	107.0
135.00	133.0
137.00	191.0
140.80	779.0
142.90	885.0
144.00	103.0
145.00	242.0
146.00	188.0
147.00	112.0
147.90	129.0
154.90	161.0
158.90	104.0
169.20	146.0
171.00	184.0
172.00	898.0
173.00	877.0
174.00	53544.0
175.00	4125.0
176.00	52216.0
177.00	3745.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	521.0
37.00	3191.0
38.00	2888.0
39.00	1226.0
40.00	145.0
44.00	511.0
45.00	691.0
47.00	844.0
47.90	370.0
49.00	2787.0
50.00	12448.0
51.00	3995.0
52.00	215.0
55.00	199.0
56.00	1098.0
57.00	2209.0
60.00	802.0
61.00	3308.0
62.00	3299.0
63.00	2975.0
63.90	268.0
65.00	579.0
67.00	195.0
68.00	7387.0
69.00	7371.0
70.00	606.0
72.00	382.0
73.00	3312.0
74.00	11996.0
75.00	37664.0
76.00	3307.0
77.00	479.0
77.80	419.0
78.90	2637.0
79.80	816.0
80.90	3055.0
81.90	760.0
86.00	143.0
87.00	3106.0
87.90	3232.0
91.00	302.0
92.00	1817.0
93.00	3244.0
94.00	8861.0
95.00	74528.0
96.00	4953.0
97.00	219.0
103.80	369.0
104.80	140.0
105.90	315.0
115.80	273.0
116.90	556.0
117.80	314.0
119.00	502.0
127.90	263.0
128.90	151.0
130.00	295.0
130.80	126.0
134.90	129.0
137.00	193.0
140.90	907.0
143.00	910.0
144.10	104.0
145.00	217.0
146.00	188.0
147.00	108.0
148.10	133.0
154.90	193.0
158.90	122.0
160.70	117.0
171.00	147.0
172.00	862.0
173.00	856.0
174.00	58384.0
175.00	4571.0
176.00	57104.0
177.00	3785.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	466.0
37.00	3045.0
38.00	2667.0
39.00	1152.0
40.20	147.0
44.00	481.0
45.00	585.0
47.00	786.0
48.00	380.0
49.00	2695.0
50.00	11822.0
51.00	3668.0
52.00	202.0
55.00	195.0
56.00	1002.0
57.00	1932.0
60.00	716.0
61.00	3108.0
62.00	3064.0
63.00	2847.0
63.90	294.0
65.00	464.0
66.90	227.0
68.00	7134.0
69.00	6883.0
70.00	590.0
72.00	312.0
73.00	3100.0
74.00	11532.0
75.00	35632.0
76.00	3196.0
77.00	454.0
77.80	366.0
78.90	2713.0
79.80	760.0
80.90	2777.0
81.90	663.0
87.00	3085.0
87.90	3131.0
91.00	305.0
92.00	1748.0
93.00	3178.0
94.00	8834.0
95.00	71128.0
96.00	4642.0
97.00	215.0
103.90	375.0
104.80	163.0
105.90	307.0
115.80	286.0
116.90	534.0
117.80	312.0
119.00	466.0
127.90	251.0
129.00	159.0
129.90	296.0
130.80	105.0
134.80	144.0
137.00	177.0
140.90	886.0
141.90	121.0
143.00	899.0
145.00	192.0
145.90	178.0
148.10	132.0
154.80	208.0
156.90	107.0
158.80	125.0
160.70	129.0
170.80	121.0
172.00	833.0
173.00	796.0
174.00	57520.0
175.00	4496.0
176.00	55376.0
177.00	3487.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61