

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016179.D
 Acq On : 22 May 2020 18:33
 Operator : SY/MD
 Sample : L2751-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y27

Manual Integrations
 APPROVED

Quant Time: May 23 07:52:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.65	114	127833	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	121482	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	56762	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43633	6.29	ug/L	0.00	MMDadoda
Spiked Amount 5.000	Range 40 - 130	Recovery =	125.80%				
7) Chloroethane-d5	1.58	69	38529	5.86	ug/L	0.00	
Spiked Amount 5.000	Range 65 - 130	Recovery =	117.20%				
11) 1,1-Dichloroethene-d2	2.13	63	69879	4.69	ug/L	0.00	5/26/2020 9:35:11 AM
Spiked Amount 5.000	Range 60 - 125	Recovery =	93.80%				
20) 2-Butanone-d5	3.95	46	86602	43.78	ug/L	-0.03	
Spiked Amount 50.000	Range 40 - 130	Recovery =	87.56%				
24) Chloroform-d	4.38	84	80442	5.31	ug/L	0.00	
Spiked Amount 5.000	Range 70 - 125	Recovery =	106.20%				
26) 1,2-Dichloroethane-d4	5.06	65	42287	4.87	ug/L	0.00	
Spiked Amount 5.000	Range 70 - 130	Recovery =	97.40%				
32) Benzene-d6	5.08	84	164477	5.69	ug/L	0.00	
Spiked Amount 5.000	Range 70 - 125	Recovery =	113.80%				
36) 1,2-Dichloropropane-d6	6.10	67	49792	5.64	ug/L	0.00	
Spiked Amount 5.000	Range 60 - 140	Recovery =	112.80%				
41) Toluene-d8	7.34	98	149753	5.48	ug/L	0.00	
Spiked Amount 5.000	Range 70 - 130	Recovery =	109.60%				
45) trans-1,3-Dichloropropene-	7.65	79	15563	4.49	ug/L	0.00	
Spiked Amount 5.000	Range 55 - 130	Recovery =	89.80%				
48) 2-Hexanone-d5	8.12	63	66863	43.95	ug/L	0.00	
Spiked Amount 50.000	Range 45 - 130	Recovery =	87.90%				
59) 1,1,2,2-Tetrachloroethane-	10.24	84	29853	4.81	ug/L	0.00	
Spiked Amount 5.000	Range 65 - 120	Recovery =	96.20%				
65) 1,2-Dichlorobenzene-d4	11.65	152	51765	5.62	ug/L	0.00	
Spiked Amount 5.000	Range 80 - 120	Recovery =	112.40%				

Target Compounds					Ovalue
3) Chloromethane	1.25	50	4862	0.490 ug/L	98
13) Acetone	2.23	43	3529m	2.704 ug/L	
25) Chloroform	4.41	83	3425	0.208 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016179.D
Acq On : 22 May 2020 18:33
Operator : SY/MD
Sample : L2751-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0Y27

Manual Integrations
APPROVED

Quant Time: May 23 07:52:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration



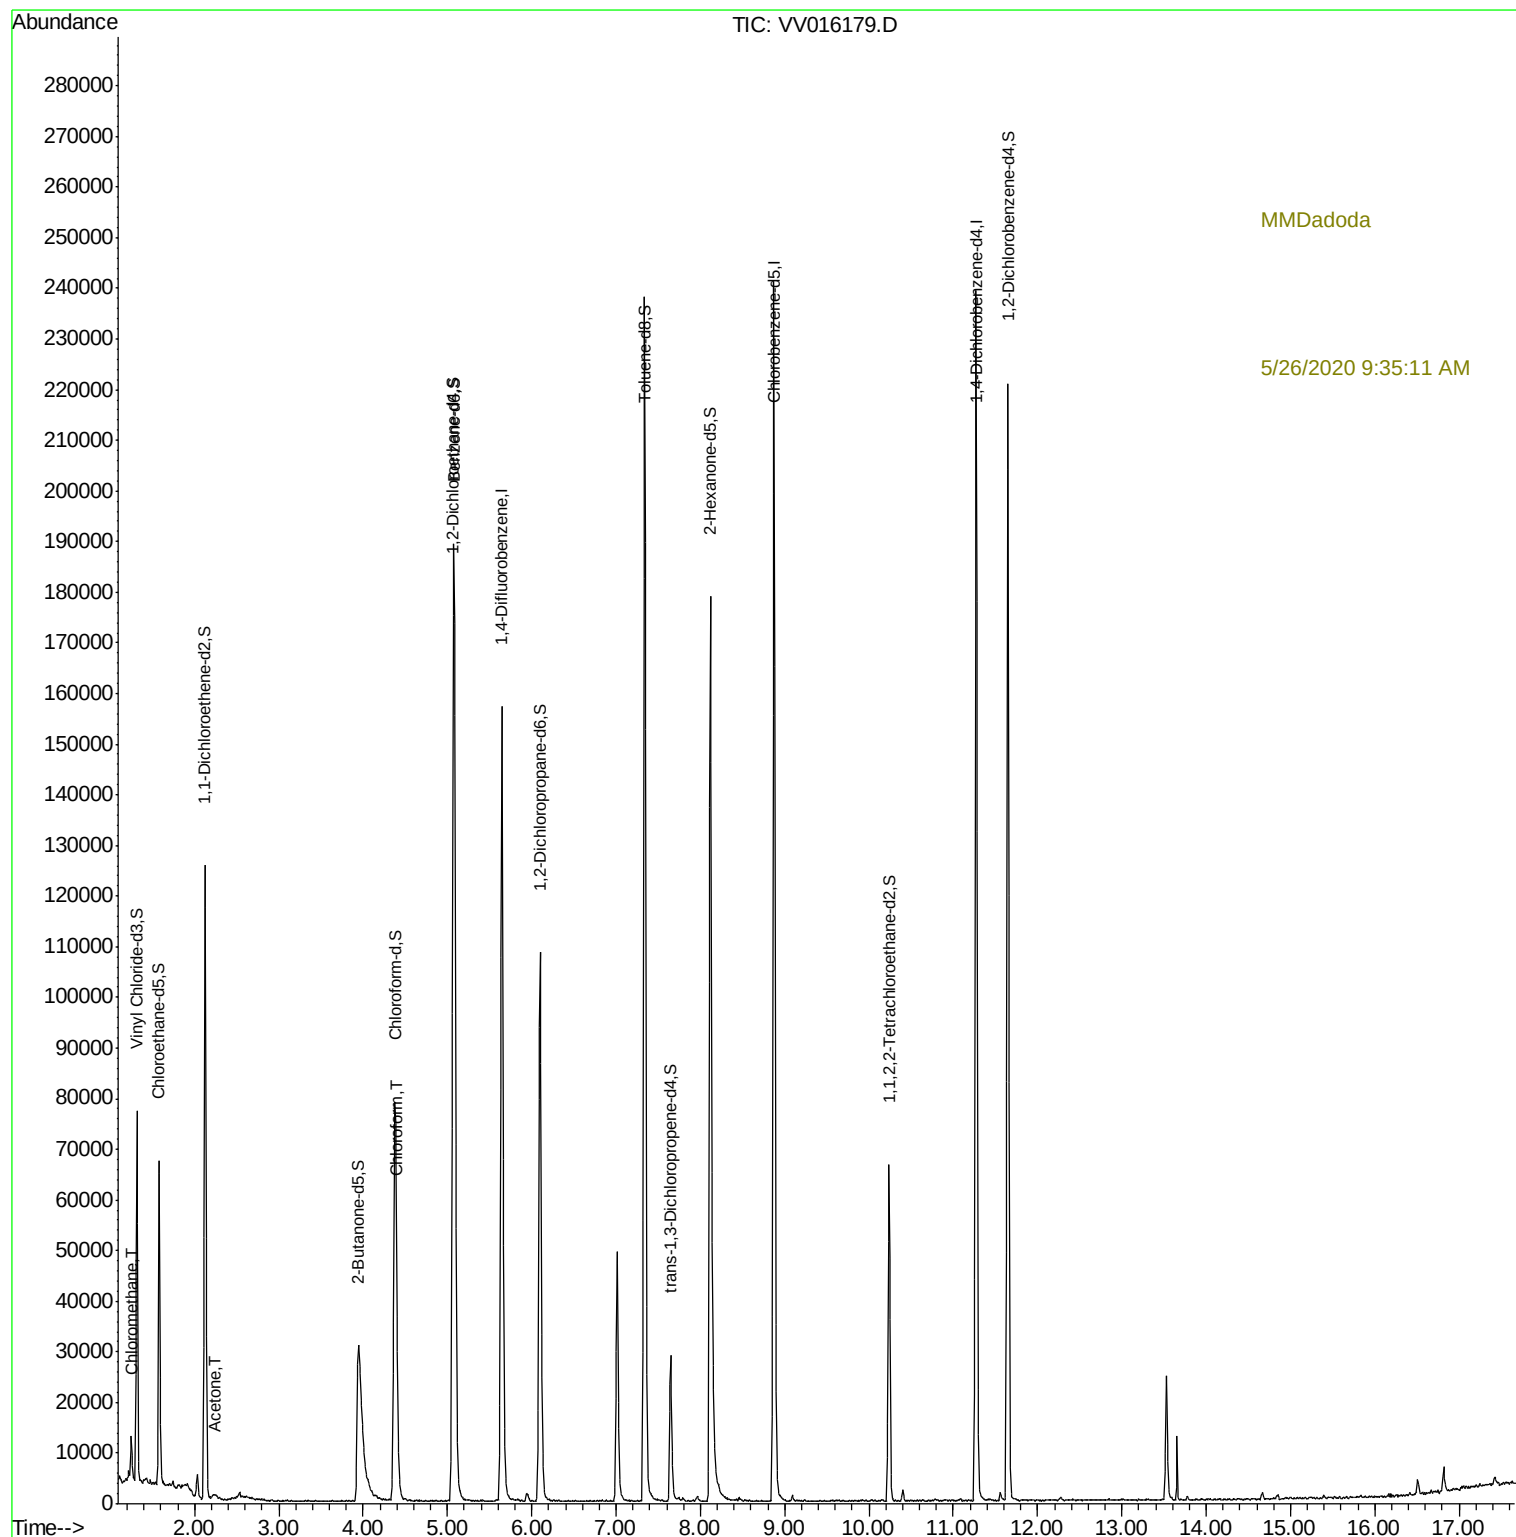


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016179.D
 Acq On : 22 May 2020 18:33
 Operator : SY/MD
 Sample : L2751-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y27

Manual Integrations
 APPROVED

Quant Time: May 23 05:11:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

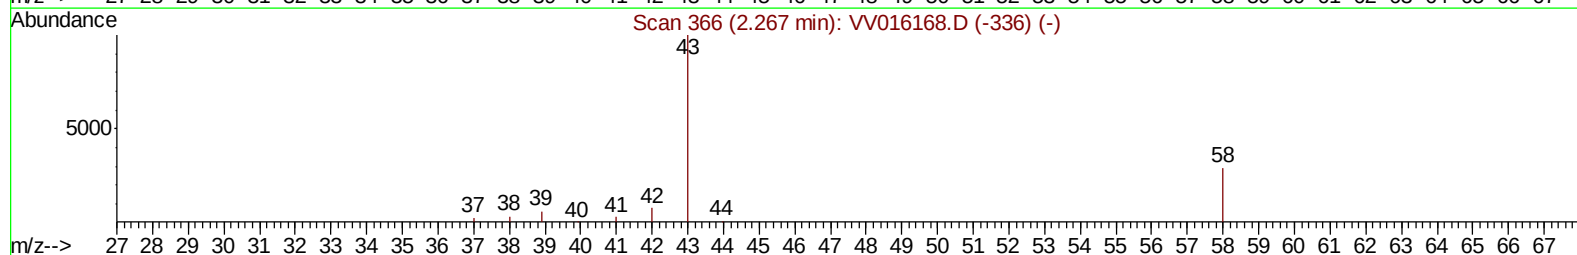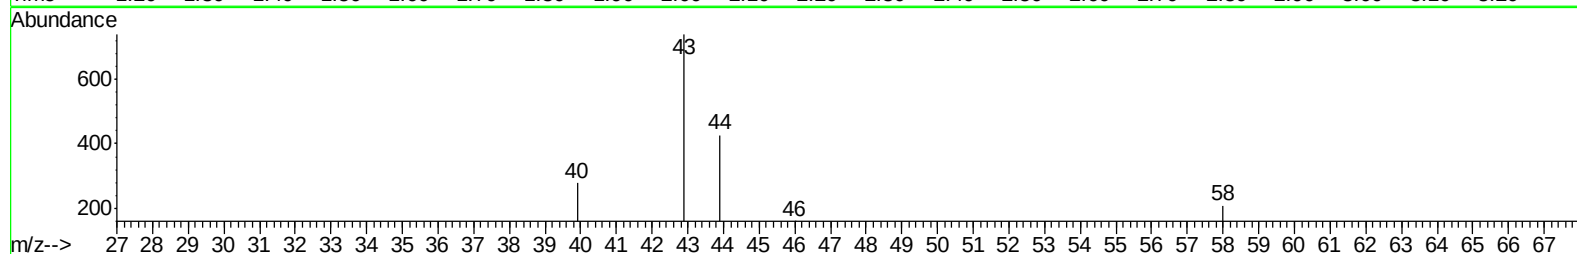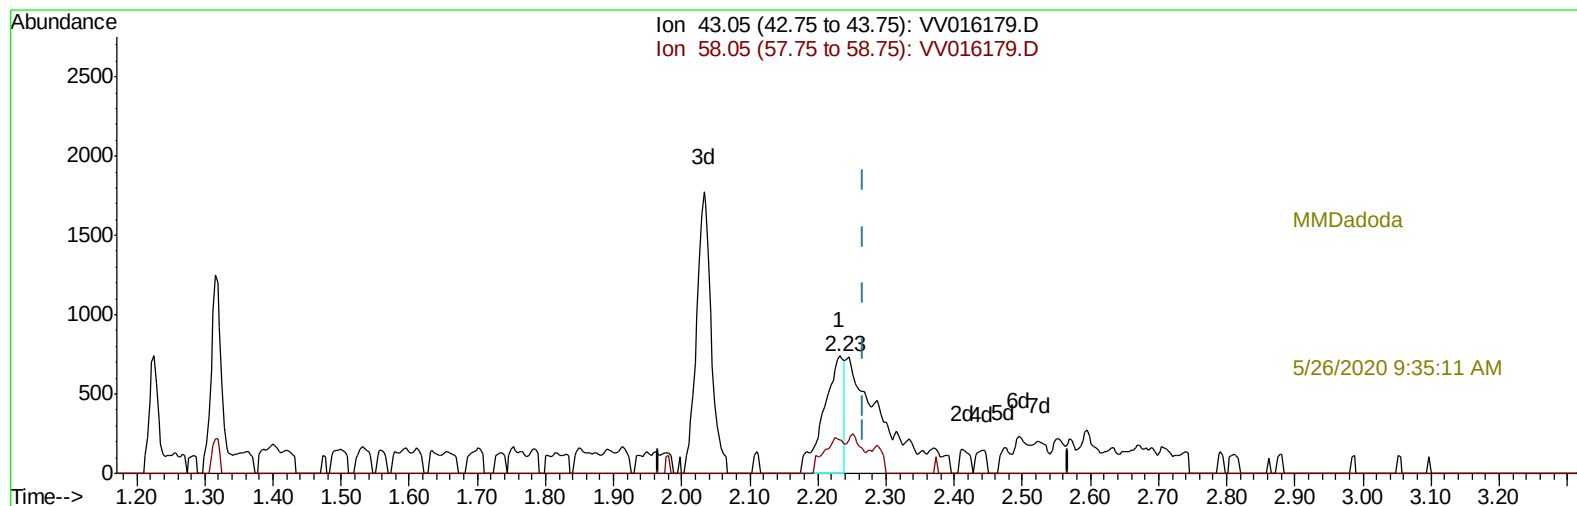

TIC: VV016179.D

(13) Acetone (T)

2.232min (-0.035) 1.18ug/L

response 1535




Ion	Exp%	Act%
43.05	100	100
58.05	15.40	29.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016179.D
 Acq On : 22 May 2020 18:33
 Operator : SY/MD
 Sample : L2751-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y27

Manual Integrations
 APPROVED

Quant Time: May 23 05:11:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

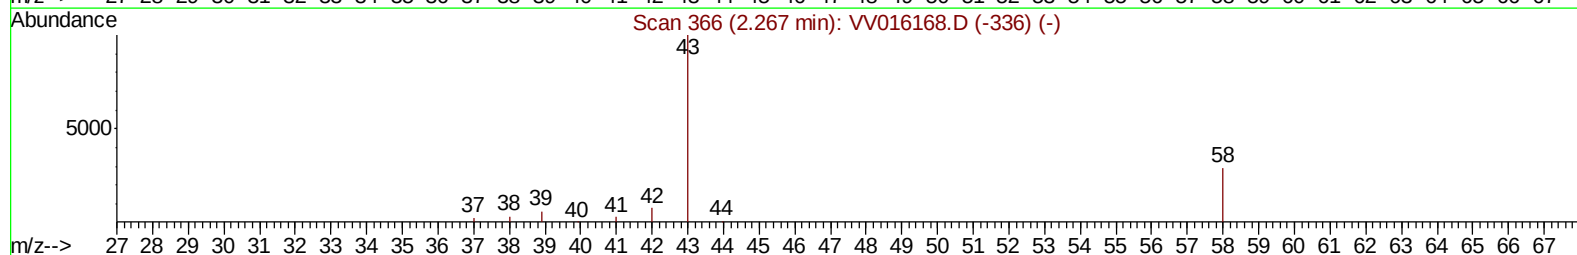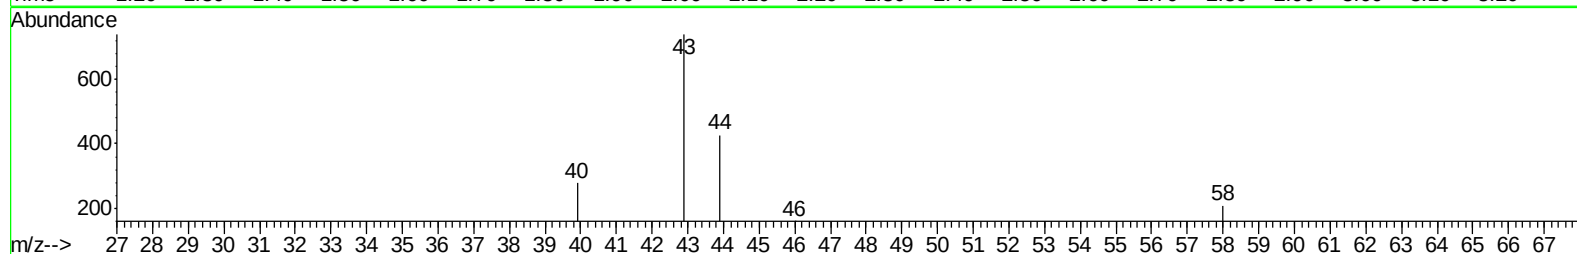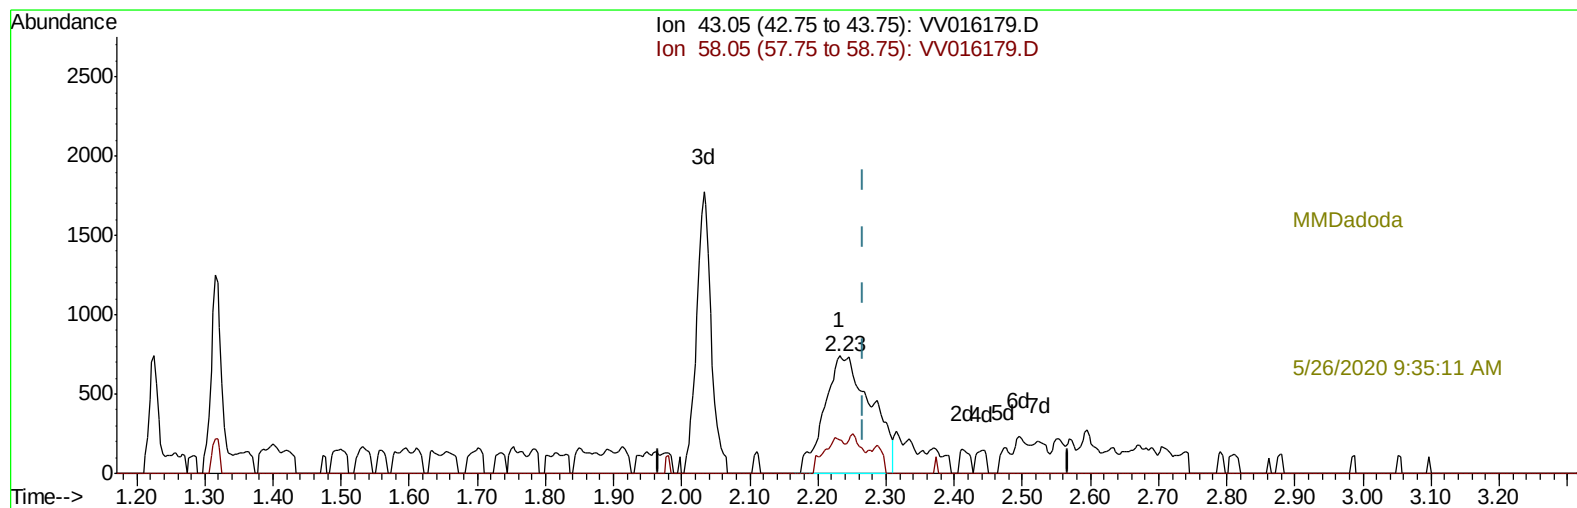

TIC: VV016179.D

(13) Acetone (T)

2.232min (-0.035) 2.70ug/L m

response 3529

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	12.64
0.00	0.00	0.00
0.00	0.00	0.00