




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

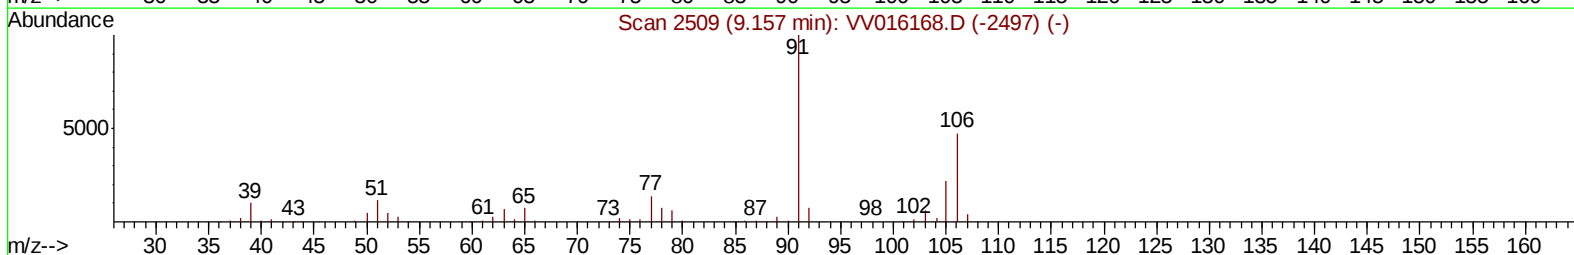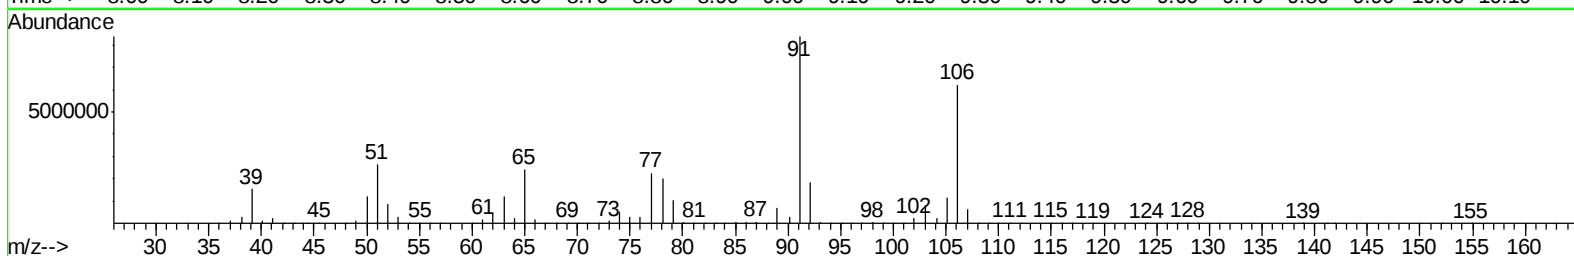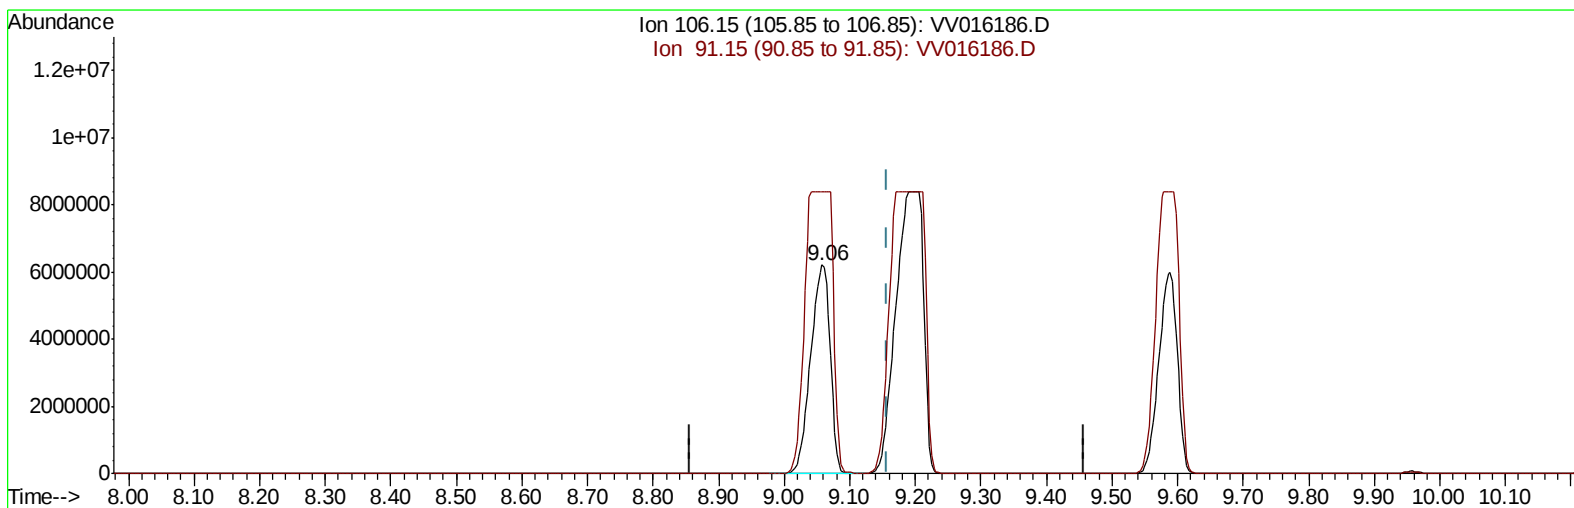

TIC: VV016186.D

(55) m,p-xylene (T)

9.058min (-0.100) 735.95ug/L

response 12720041

Ion	Exp%	Act%
106.15	100	100
91.15	214.10	135.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

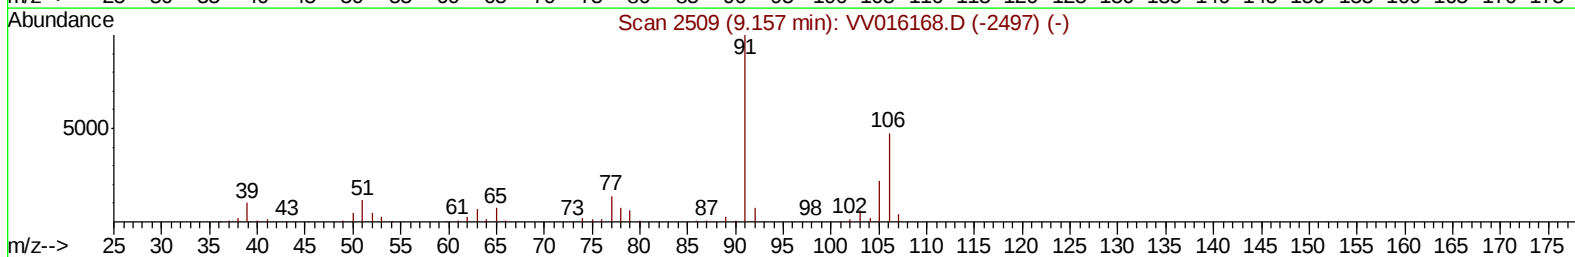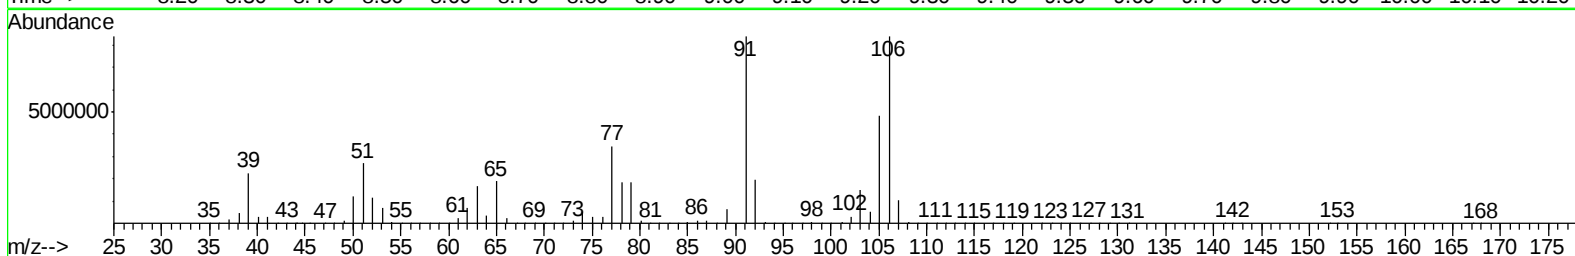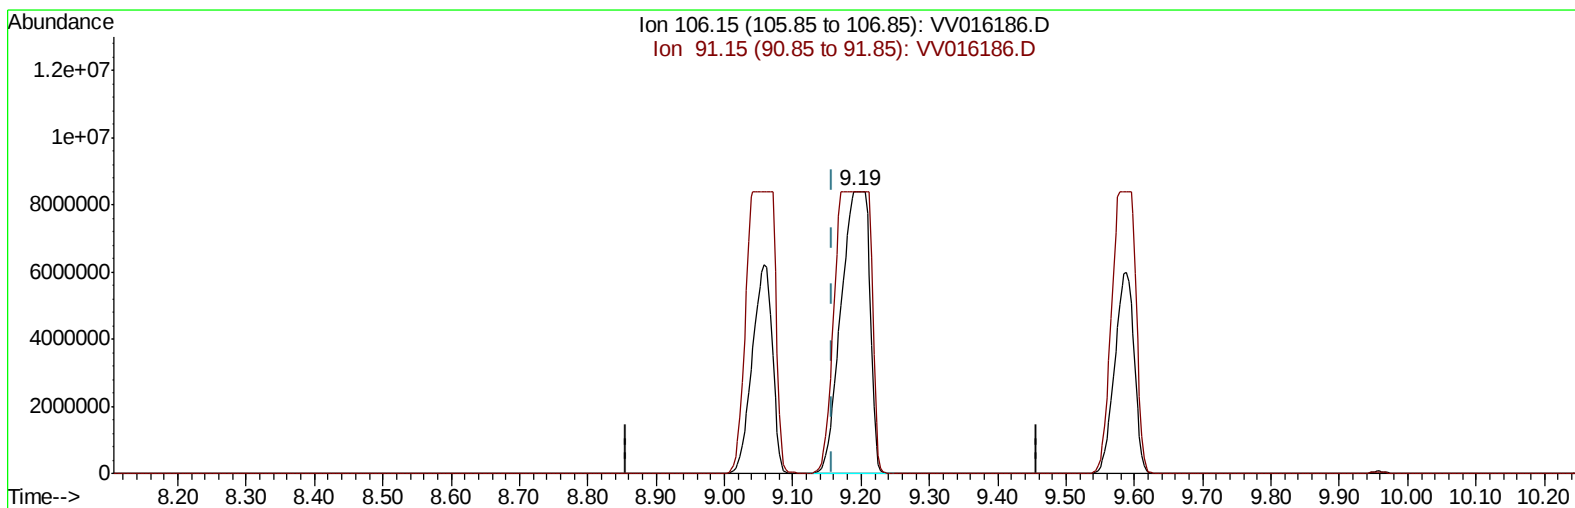

TIC: VV016186.D

(55) m,p-xylene (T)

9.190min (+0.032) 1414.86ug/L m

response 24454413

Ion	Exp%	Act%
106.15	100	100
91.15	214.10	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:18:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	165512	5.00	ug/L	0.02
28) Chlorobenzene-d5	8.88	117	153931	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.28	152	78796	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	55239	6.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	123.00%
7) Chloroethane-d5	1.58	69	40959	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.20%
11) 1,1-Dichloroethene-d2	2.14	63	3666268	189.88	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	3797.60%#
20) 2-Butanone-d5	4.05	46	50003	19.52	ug/L	0.07
Spiked Amount	50.000	Range	40 - 130	Recovery	=	39.04%#
24) Chloroform-d	4.40	84	99880	5.09	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.08	65	46009	4.09	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.80%
32) Benzene-d6	5.10	84	191641	5.23	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
36) 1,2-Dichloropropane-d6	6.11	67	58144	5.20	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.36	98	204162m	5.90	ug/L	0.03
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.00%
45) trans-1,3-Dichloropropene-	7.66	79	21421	4.88	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.60%
48) 2-Hexanone-d5	8.13	63	93184	48.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.68%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	37457	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	64829	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	1.14	85	1380	0.109	ug/L	98
3) Chloromethane	1.24	50	1703	0.133	ug/L	95
5) Vinyl chloride	1.32	62	1122917	91.454	ug/L	100
8) Chloroethane	1.60	64	18380	2.101	ug/L	92
9) Trichlorofluoromethane	1.77	101	41668	2.474	ug/L	100
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	435987	45.830	ug/L	98
12) 1,1-Dichloroethene	2.14	96	6213821	682.211	ug/L #	58
14) Carbon disulfide	2.32	76	31243	1.039	ug/L	99
16) Methylene chloride	2.52	84	13287605	1219.173	ug/L	98
18) trans-1,2-Dichloroethene	2.79	96	1028720	102.198	ug/L	99
19) 1,1-Dichloroethane	3.23	63	21241000	1095.590	ug/L	94
22) cis-1,2-Dichloroethene	3.94	96	74293374m	7050.549	ug/L	
25) Chloroform	4.42	83	99447	4.658	ug/L	100
29) 1,1,1-Trichloroethane	4.66	97	50929301m	3000.260	ug/L	
30) Cyclohexane	4.75	56	1391413	81.797	ug/L	92
33) Benzene	5.14	78	7681656	198.348	ug/L	100
34) Trichloroethene	5.95	95	2501290	226.282	ug/L	95

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:18:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) Methylcyclohexane	6.17	83	1778662	106.374	uq/L	99
40) 4-Methyl-2-pentanone	7.30	43	2780675	453.418	uq/L	97
42) Toluene	7.41	91	51665781m	1258.583	uq/L	
47) 1,1,2-Trichloroethane	7.87	97	60369	9.188	uq/L	96
49) Tetrachloroethene	8.01	164	219909	28.512	uq/L	99
50) 2-Hexanone	8.18	43	130392	30.066	uq/L #	89
53) Chlorobenzene	8.91	112	180250	6.827	uq/L	99
54) Ethylbenzene	9.04	91	24588211m	526.753	uq/L	
55) m,p-xylene	9.19	106	24454413m	1414.863	uq/L	
56) o-xylene	9.59	106	11846290	716.896	uq/L #	47
57) Styrene	9.60	104	5579361	201.862	uq/L	83
58) Isopropylbenzene	9.96	105	1065884	23.479	uq/L	99
63) 1,3-Dichlorobenzene	11.21	146	10095	0.476	uq/L	89
64) 1,4-Dichlorobenzene	11.30	146	96241	4.512	uq/L	98
66) 1,2-Dichlorobenzene	11.67	146	563125	29.309	uq/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:18:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

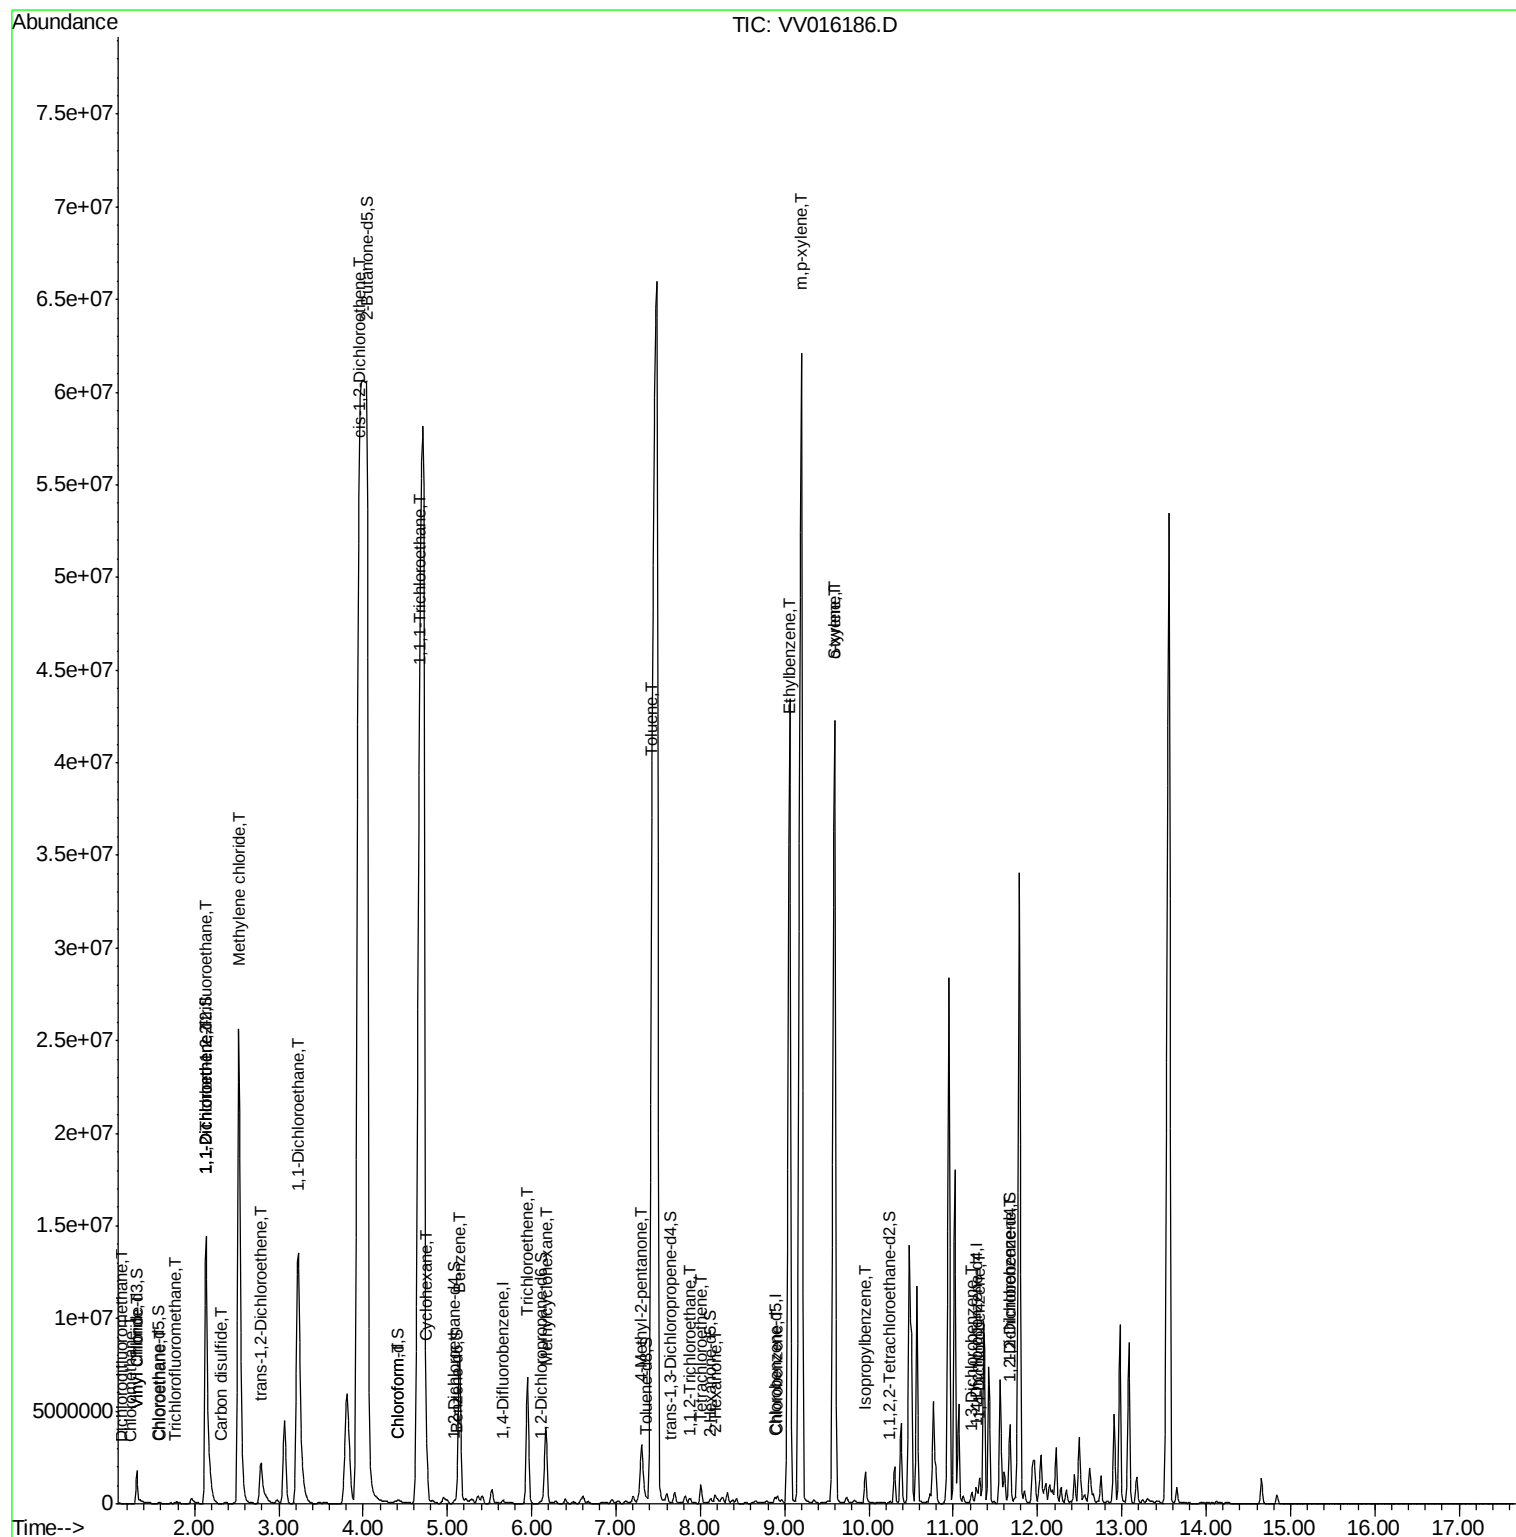




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:13:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

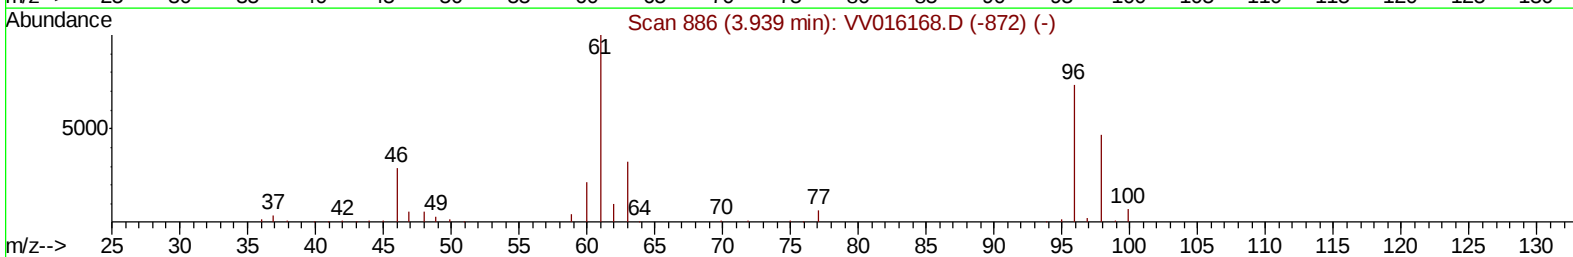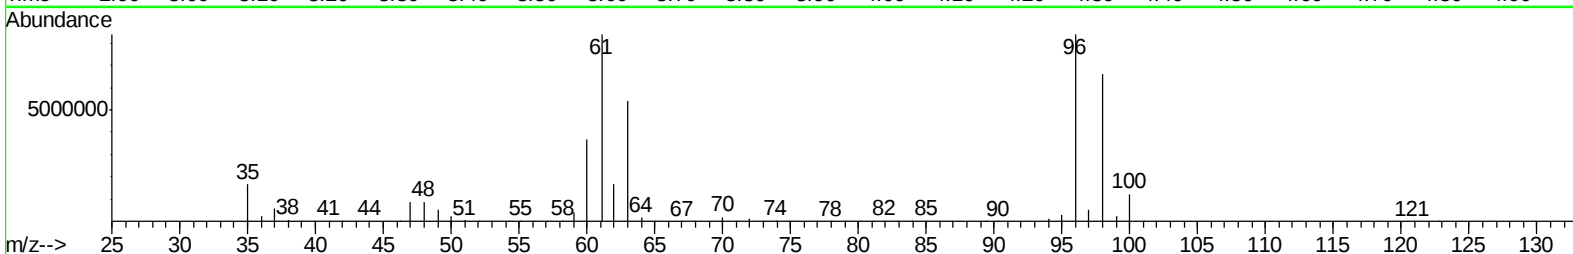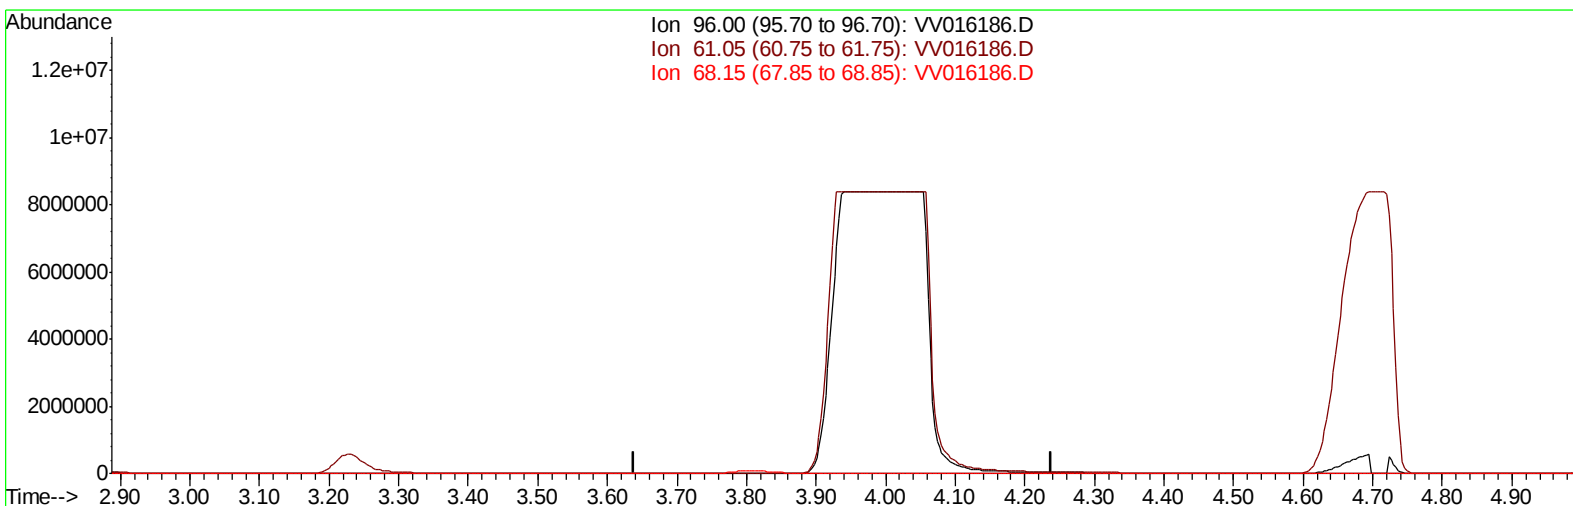

TIC: VV016186.D

(22) cis-1,2-Dichloroethene (T)

3.939min (-3.939) 0.00ug/L

response 0

Ion	Exp%	Act%
96.00	100	0.00
61.05	138.90	0.00#
68.15	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:13:36 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

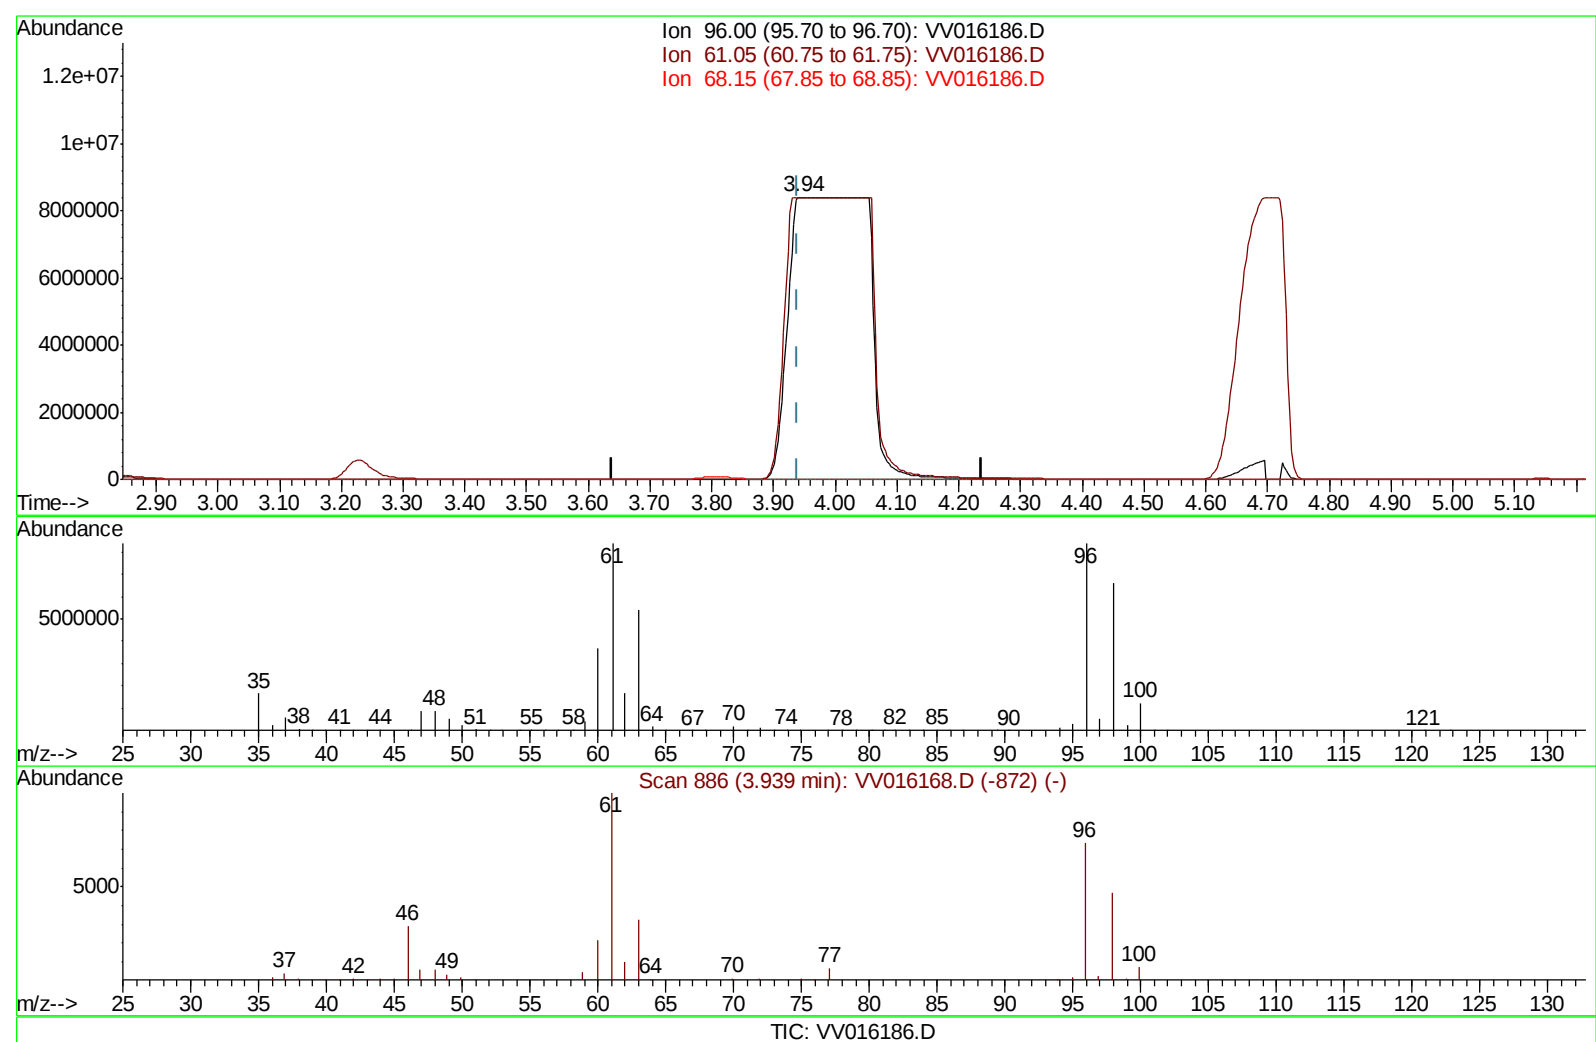

(22) cis-1,2-Dichloroethene (T)

3.939min (+0.000) 7050.55ug/L m

response 74293374

Ion	Exp%	Act%
96.00	100	100
61.05	138.90	100.00
68.15	0.00	0.00#
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:13:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

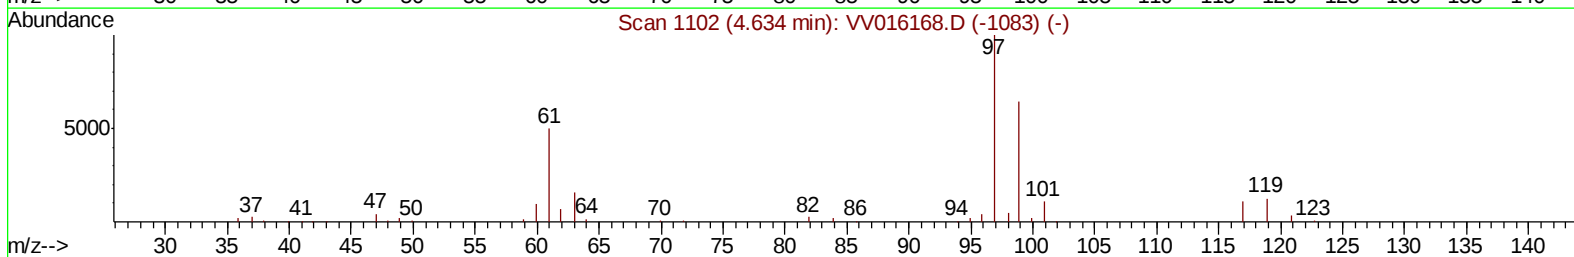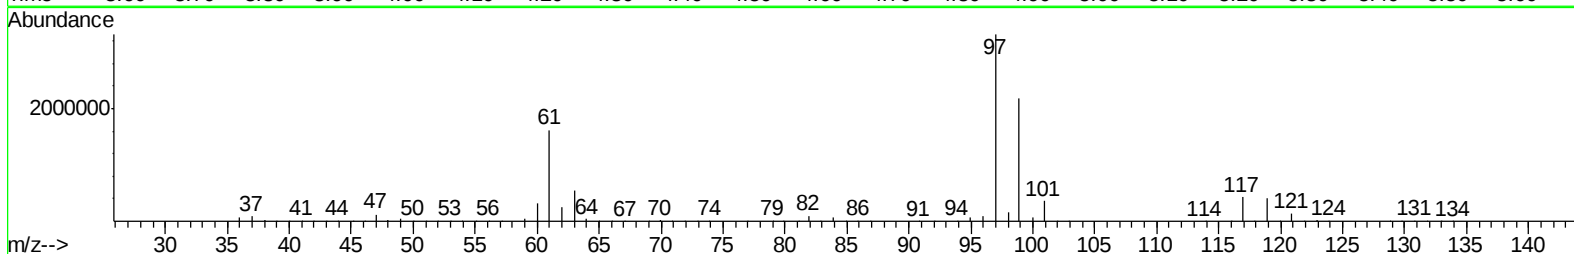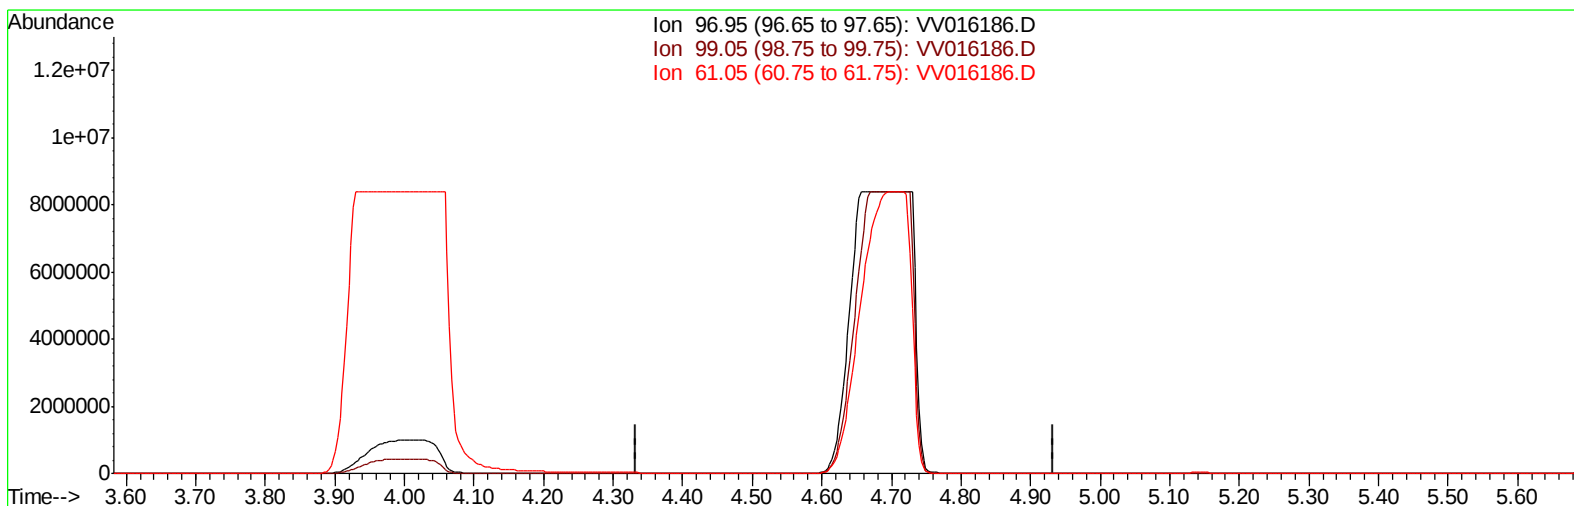

TIC: VV016186.D

(29) 1,1,1-Trichloroethane (T)

4.634min (-4.634) 0.00ug/L

response 0

Ion	Exp%	Act%
96.95	100	0.00
99.05	63.40	0.00#
61.05	48.50	0.00#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:13:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

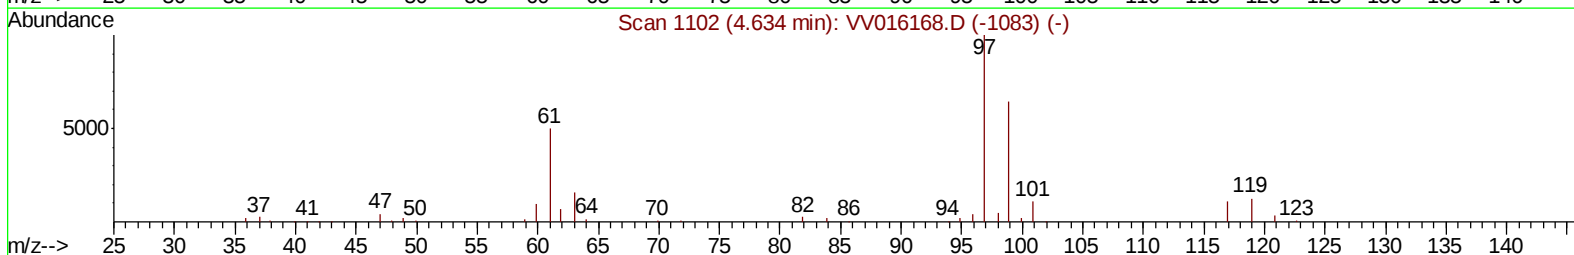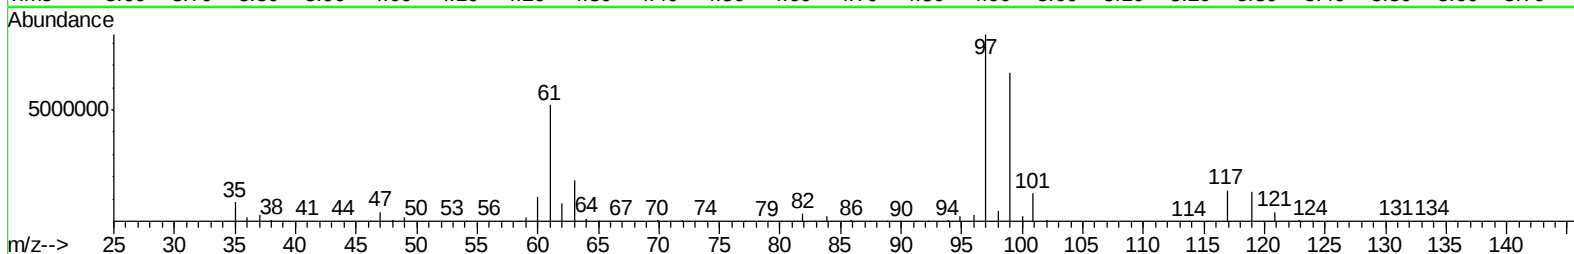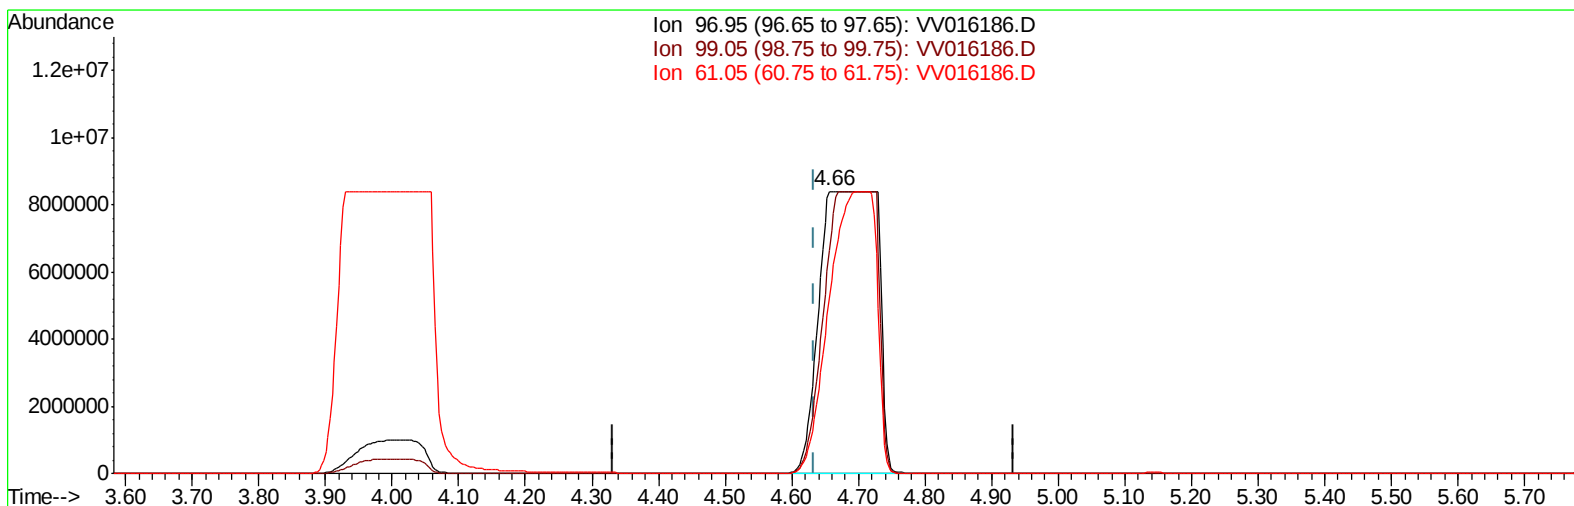

TIC: VV016186.D

(29) 1,1,1-Trichloroethane (T)

4.656min (+0.023) 3000.26ug/L m

response 50929301

Ion	Exp%	Act%
96.95	100	100
99.05	63.40	0.00#
61.05	48.50	0.00#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

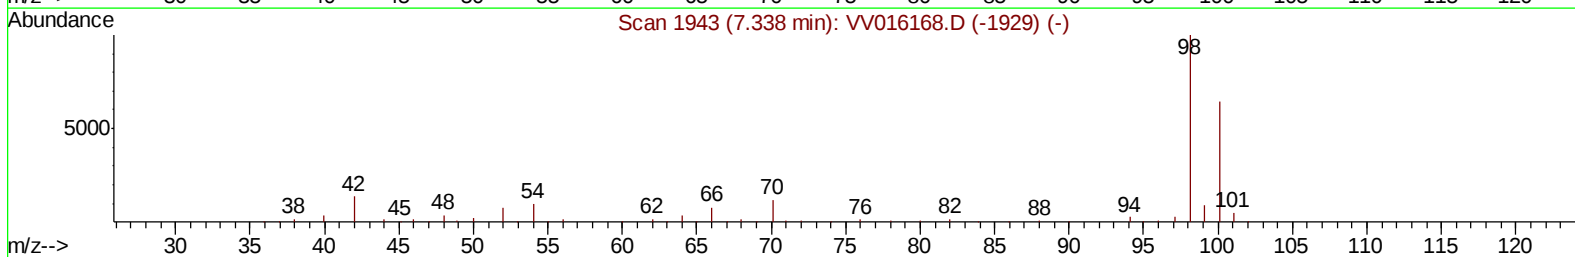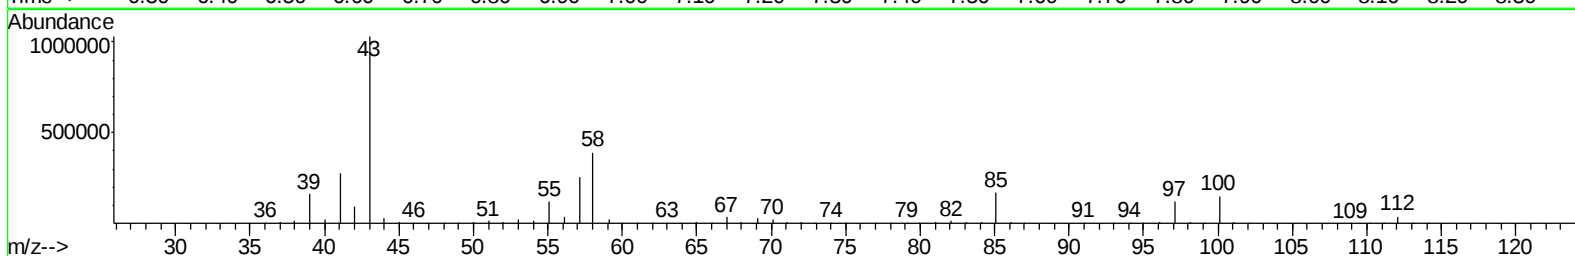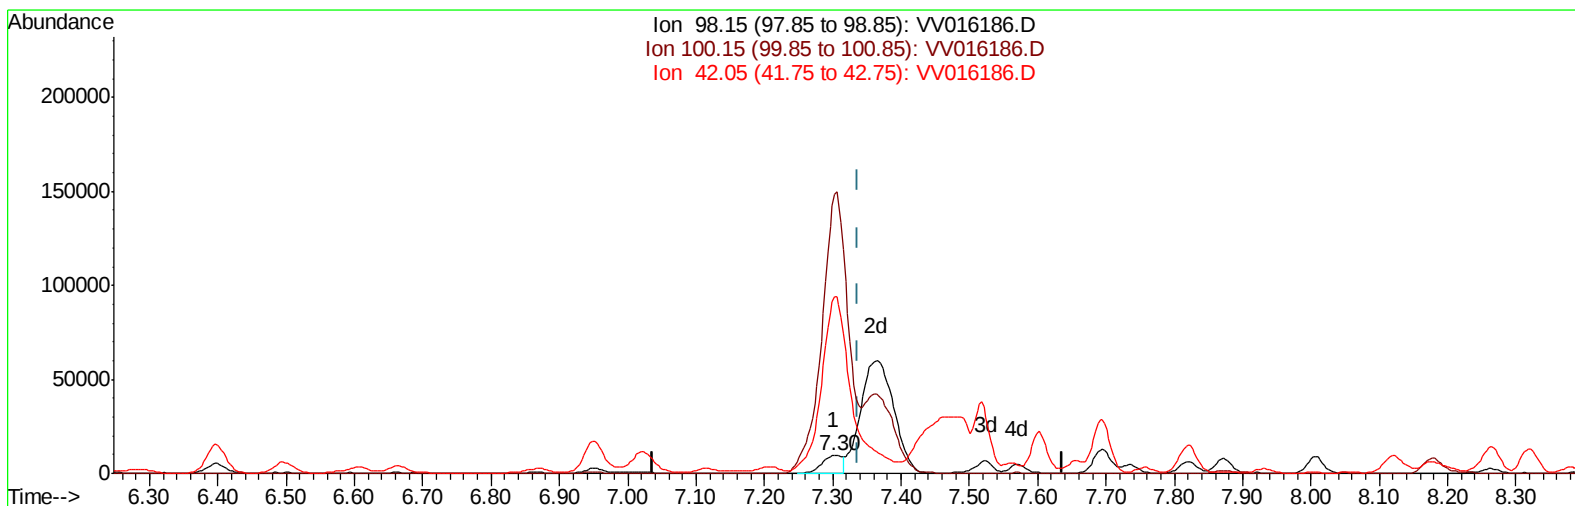

TIC: VV016186.D

(41) Toluene-d8 (S)

7.302min (-0.035) 0.56ug/L

response 19485

Ion	Exp%	Act%
98.15	100	100
100.15	66.10	2075.41#
42.05	14.70	1446.74#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

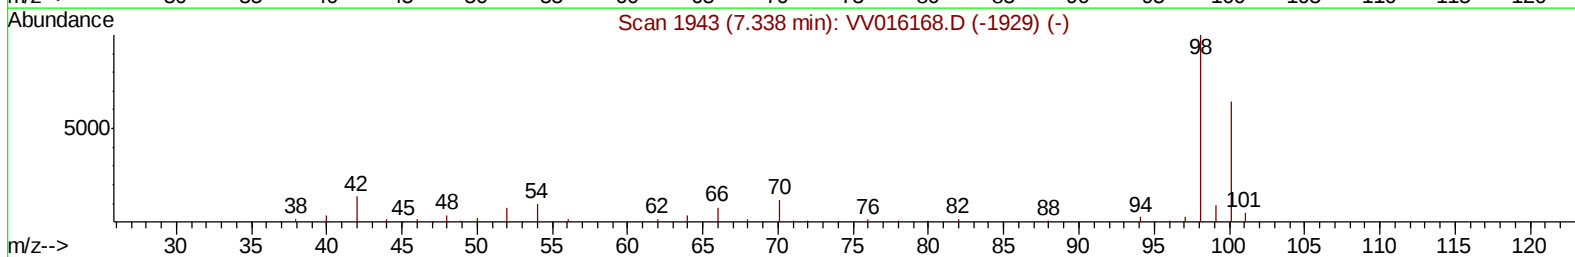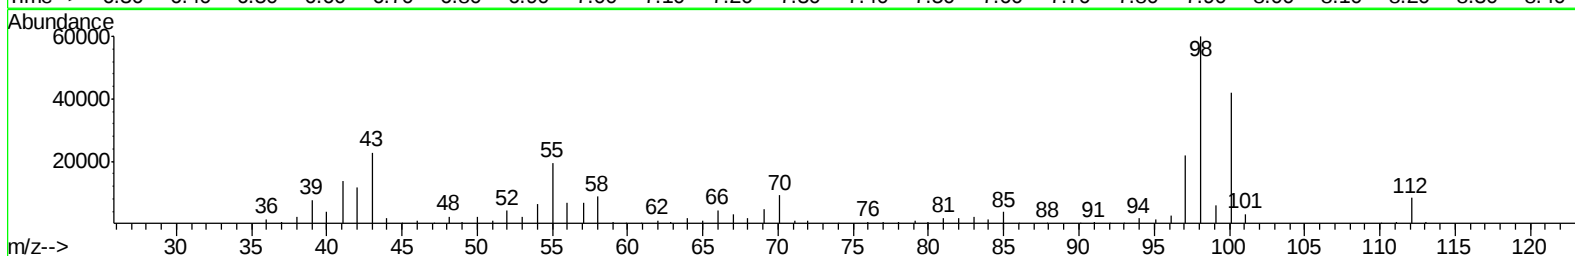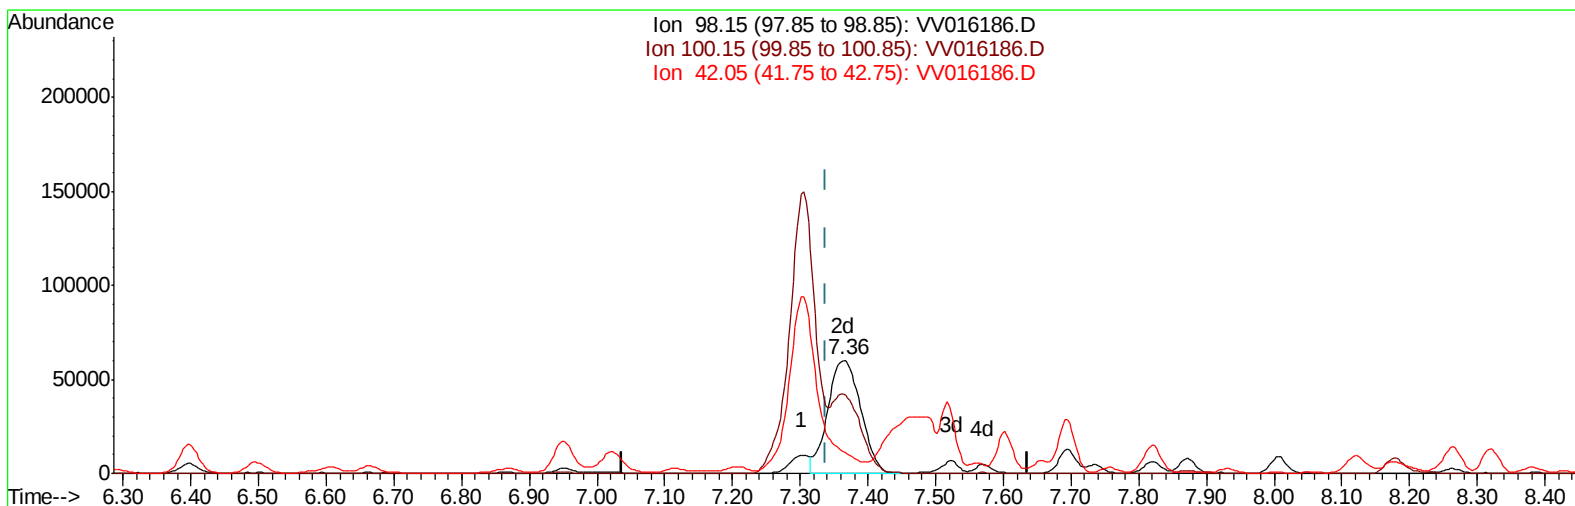

TIC: VV016186.D

(41) Toluene-d8 (S)

7.363min (+0.026) 5.90ug/L m

response 204162

Ion	Exp%	Act%
98.15	100	100
100.15	66.10	198.08#
42.05	14.70	138.08#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016186.D
Acq On : 22 May 2020 21:14
Operator : SY/MD
Sample : L2756-05MS
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW8MS

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

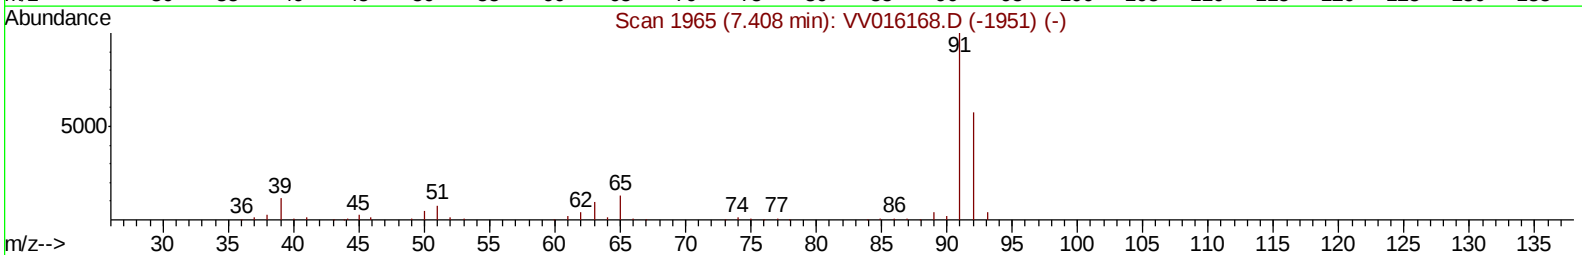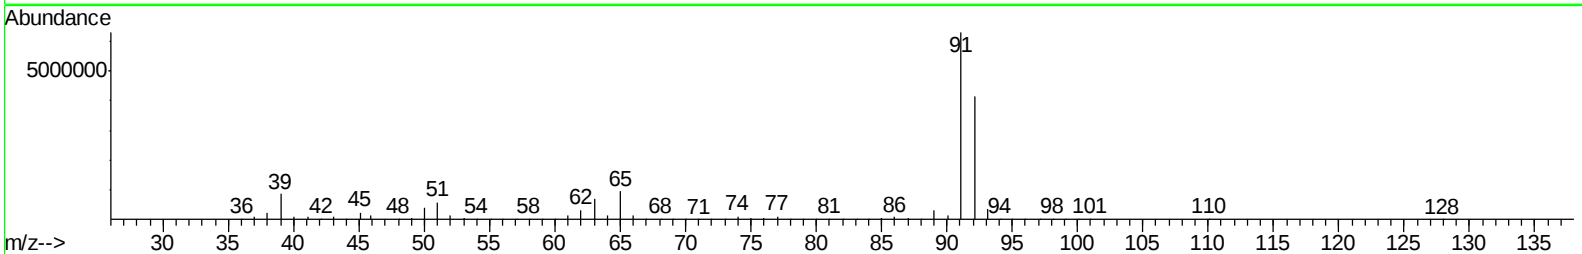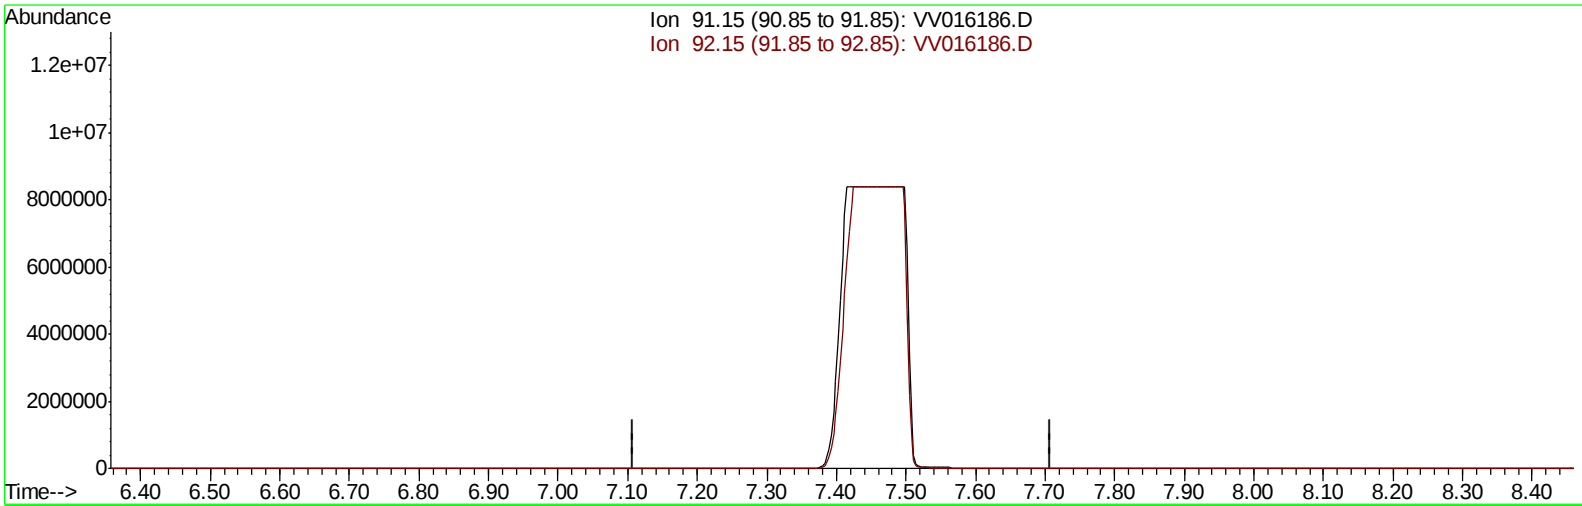

TIC: VV016186.D

(42) Toluene (T)

7.408min (-7.408) 0.00ug/L

response 0

Ion	Exp%	Act%
91.15	100	0.00
92.15	57.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

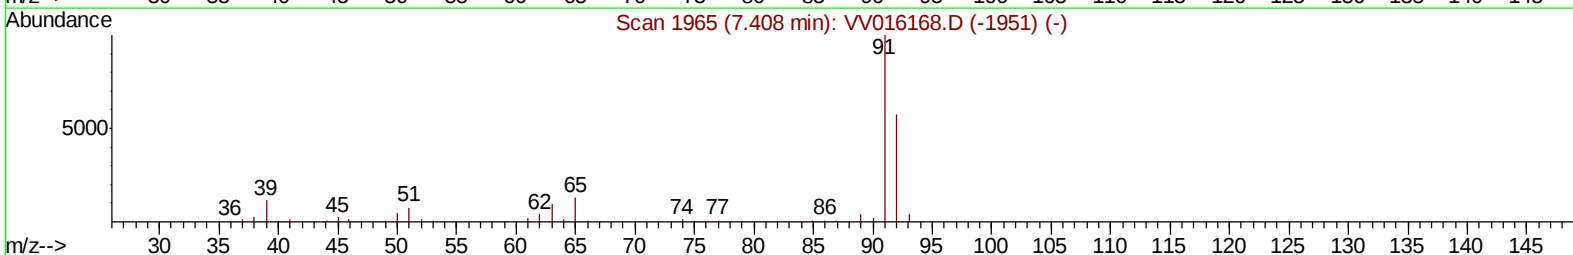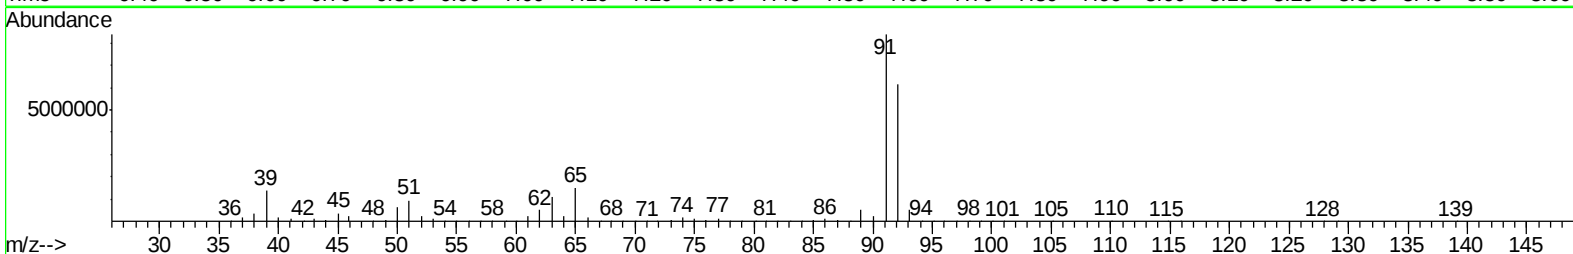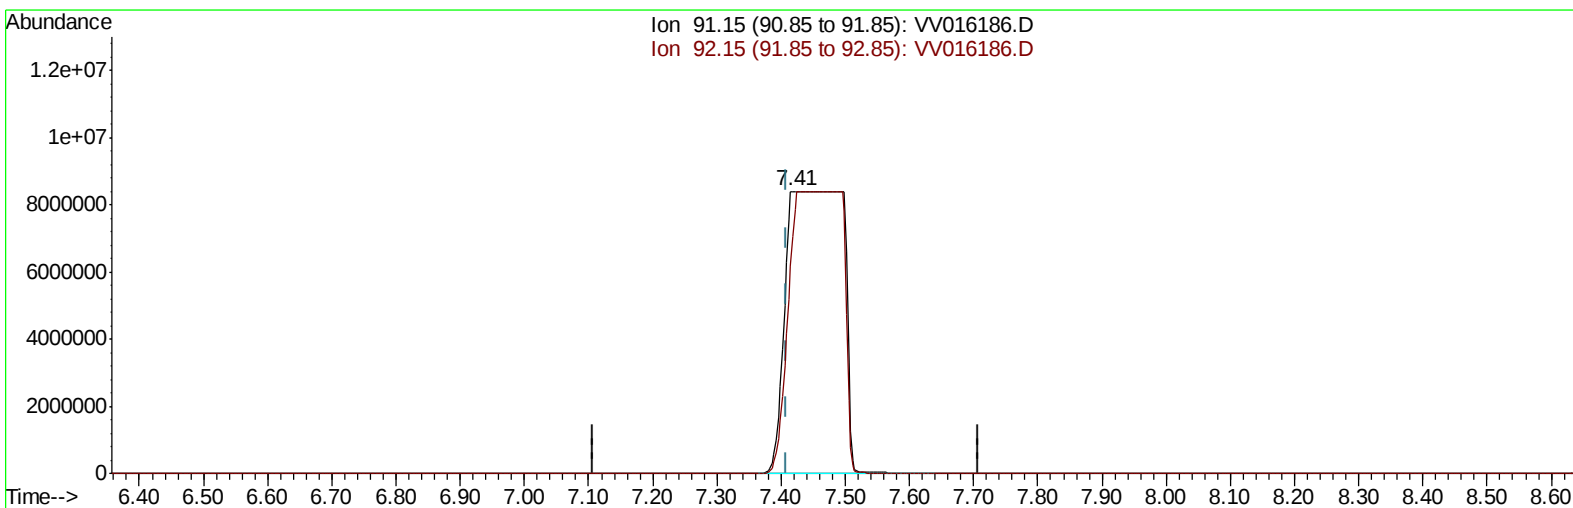

TIC: VV016186.D

(42) Toluene (T)

7.415min (+0.007) 1258.58ug/L m

response 51665781

Ion	Exp%	Act%
91.15	100	100
92.15	57.30	73.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

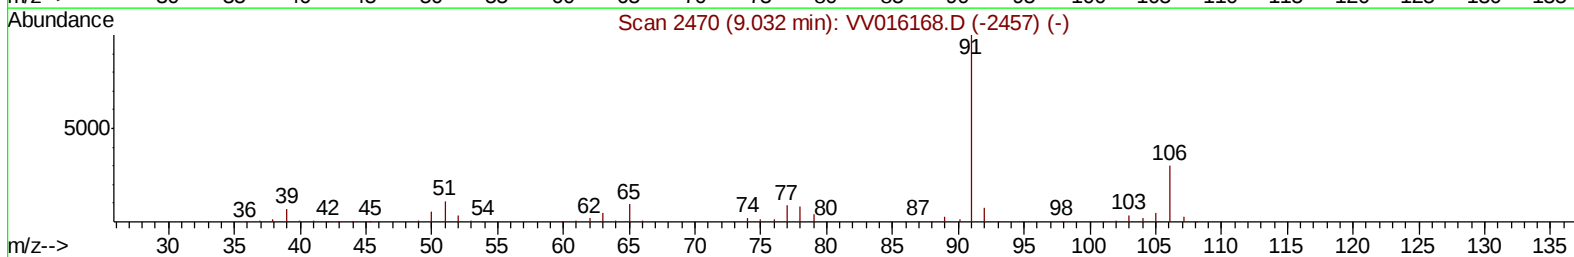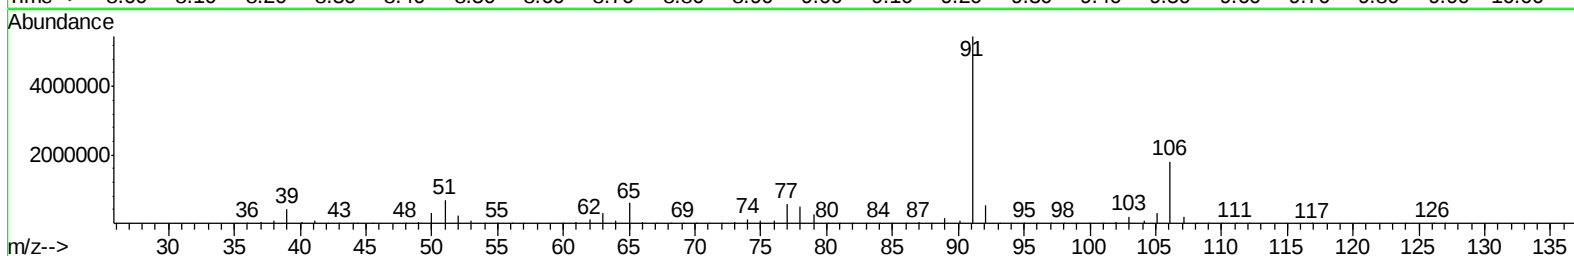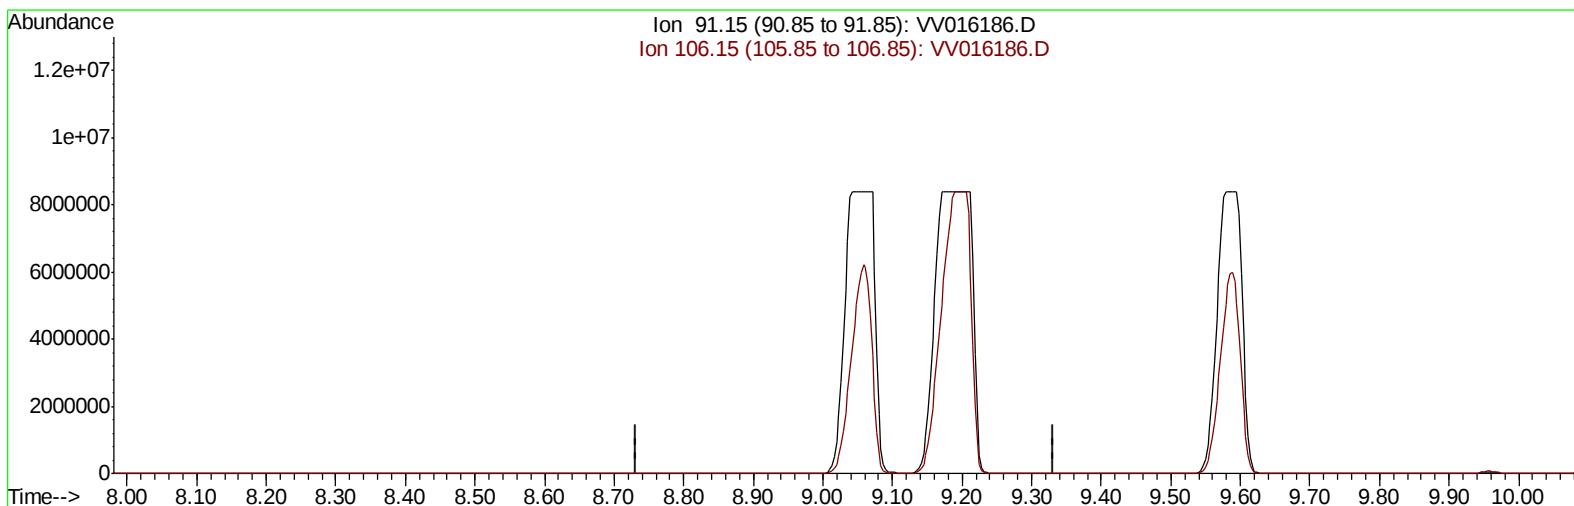

TIC: VV016186.D

(54) Ethylbenzene (T)

9.032min (-9.032) 0.00ug/L

response 0

Ion	Exp%	Act%
91.15	100	0.00
106.15	29.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016186.D
 Acq On : 22 May 2020 21:14
 Operator : SY/MD
 Sample : L2756-05MS
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW8MS

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:25 AM

Quant Time: May 23 08:15:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

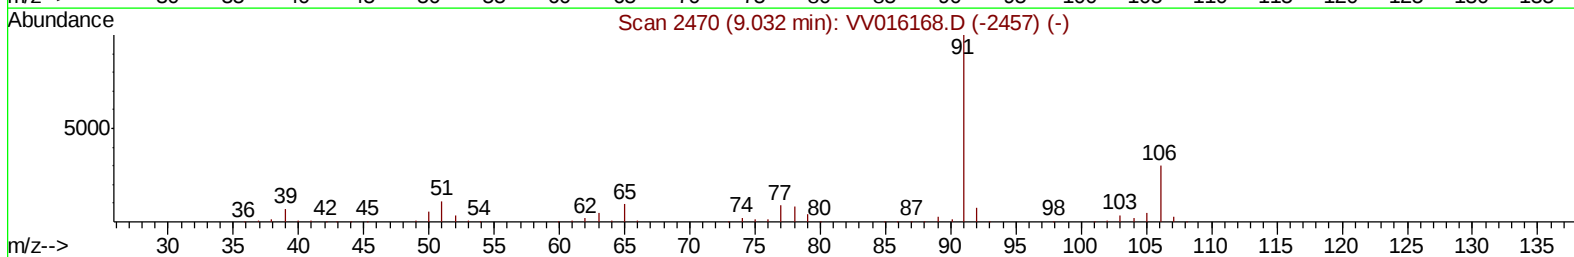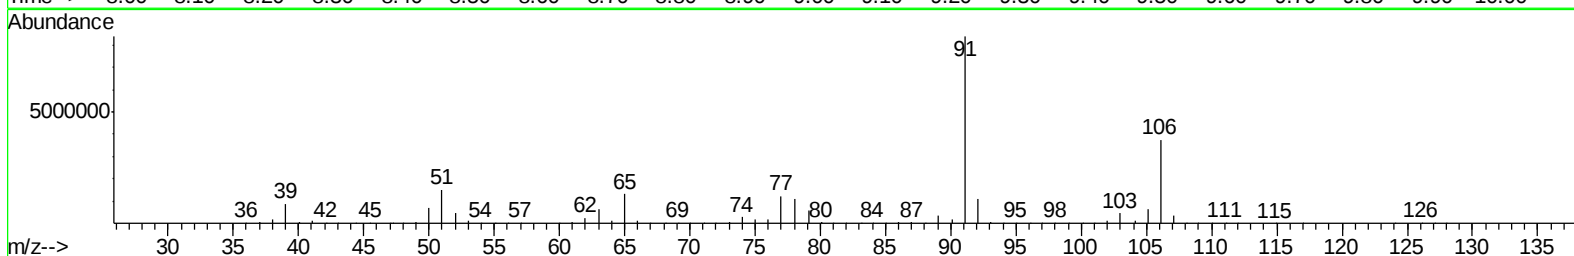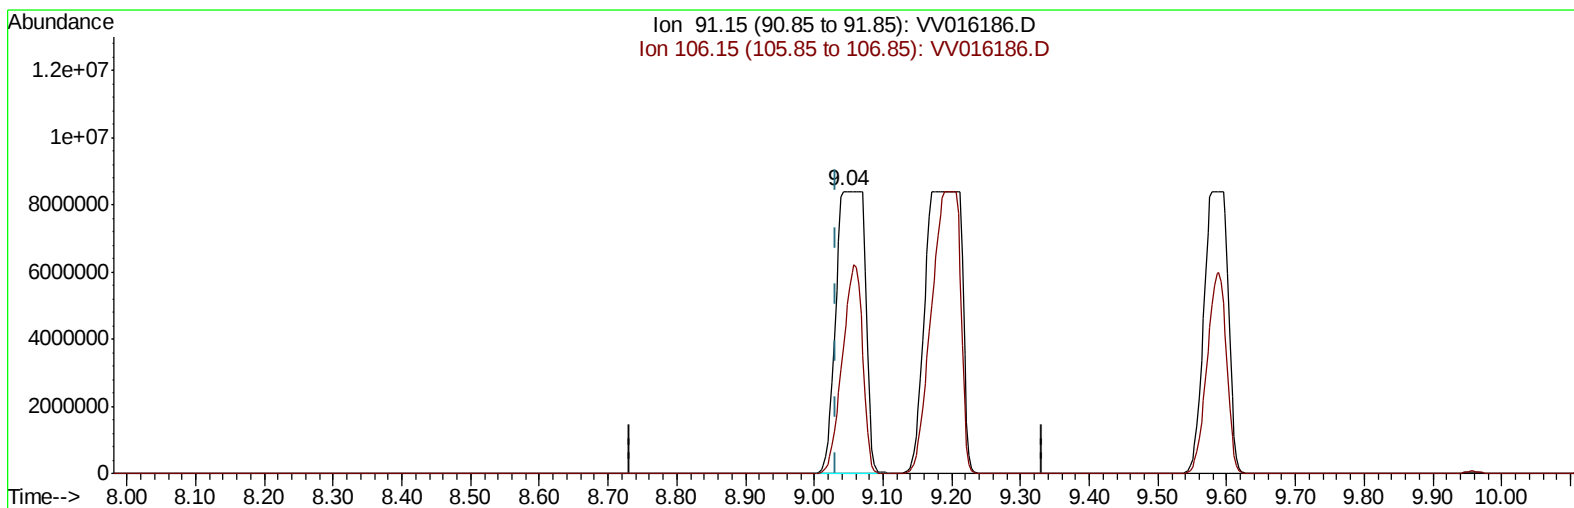

TIC: VV016186.D

(54) Ethylbenzene (T)

9.042min (+0.010) 526.75ug/L m

response 24588211

Ion	Exp%	Act%
91.15	100	100
106.15	29.50	44.75#
0.00	0.00	0.00
0.00	0.00	0.00