

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016175.D
 Acq On : 22 May 2020 17:00
 Operator : SY/MD
 Sample : L2731-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX5

Quant Time: May 25 01:16:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	144820	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	138633	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	66142	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42467	5.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.20%
7) Chloroethane-d5	1.58	69	37557	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.13	63	65568	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.93	46	87442	39.02	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.04%
24) Chloroform-d	4.38	84	76558	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.06	65	39766	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.80%
32) Benzene-d6	5.08	84	159306	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.10	67	47071	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.34	98	146250	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
45) trans-1,3-Dichloropropene-	7.65	79	14911	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
48) 2-Hexanone-d5	8.12	63	65039	37.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.92%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	29316	4.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	49282	4.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	29123	19.699 ug/L	70
30) Cyclohexane	4.71	56	6197	0.405 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016175.D
Acq On : 22 May 2020 17:00
Operator : SY/MD
Sample : L2731-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Time: May 25 01:16:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

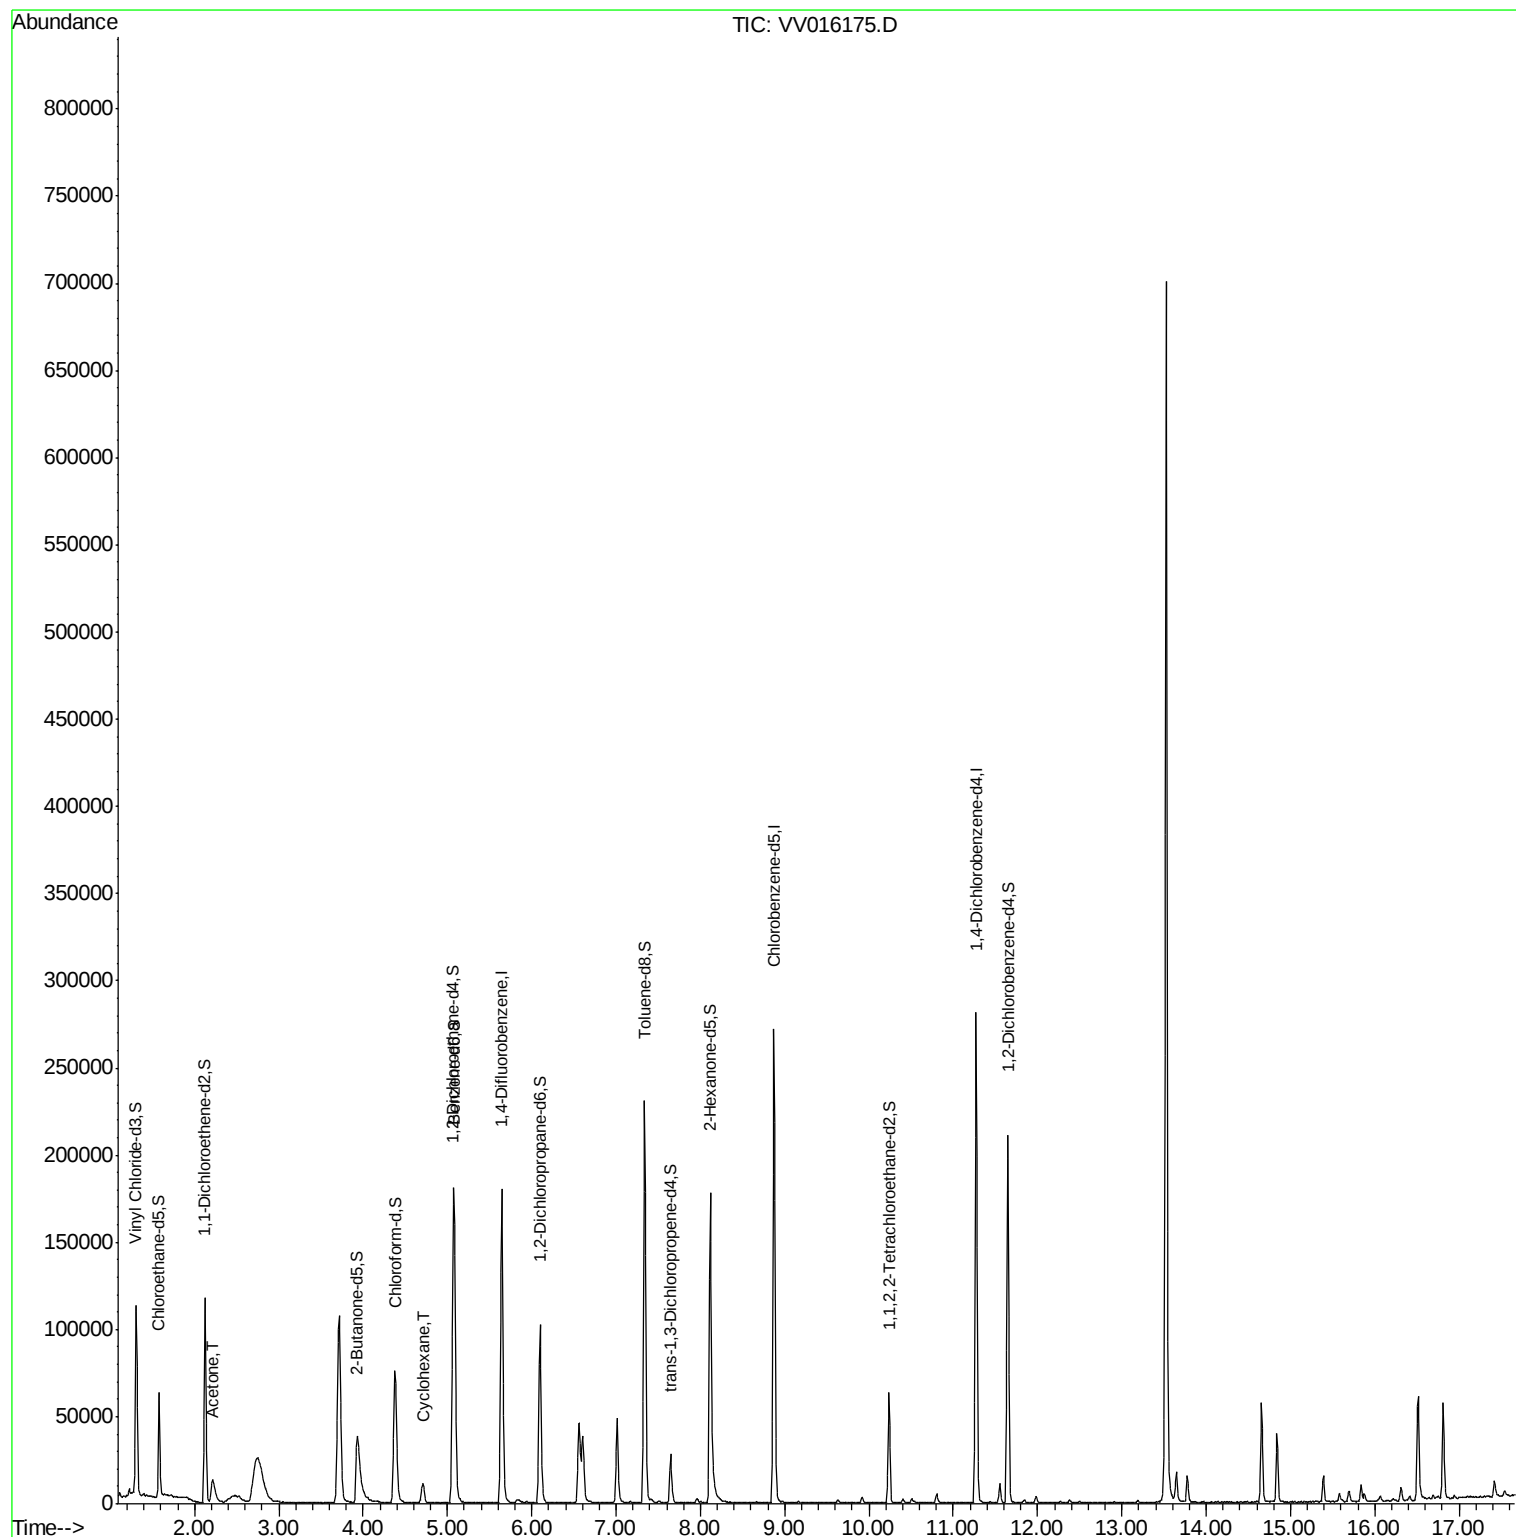

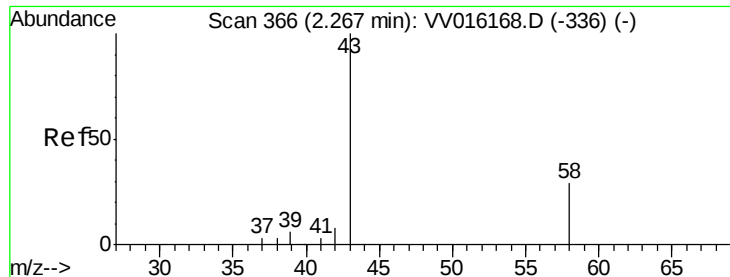

#13

Acetone

Concen: 19.699 ug/L

RT: 2.22 min Scan# 350

Delta R.T. -0.05 min

Lab File: VV016175.D

Acq: 22 May 2020 17:00

Instrument :

MSVOA_V

ClientSampleId :


C0AX5

Tot Ion: 43 Resp: 29123

Ion Ratio Lower Upper




43 100

58 28.0 0.0 30.8

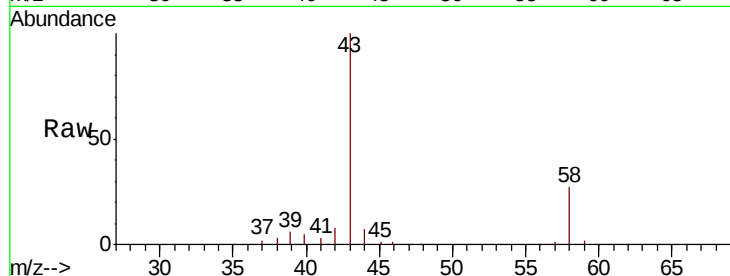

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

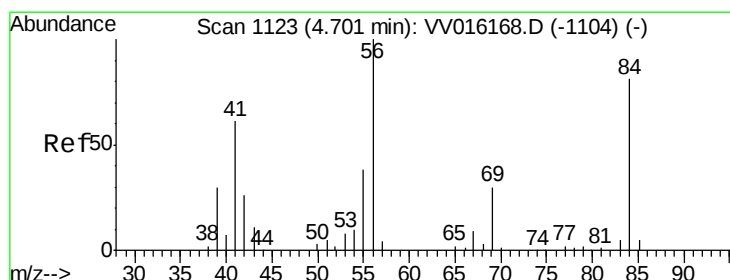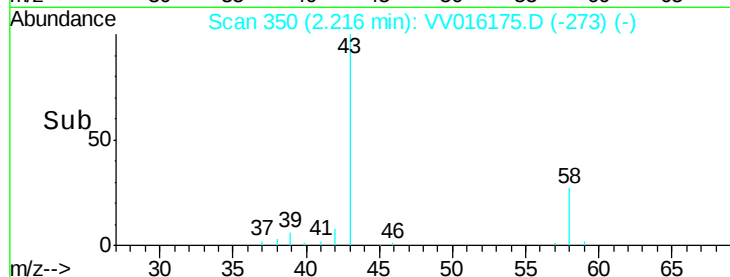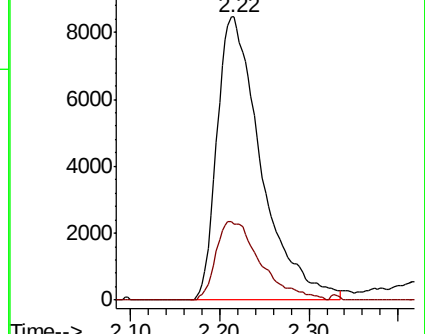

#30

Cyclohexane

Concen: 0.405 ug/L

RT: 4.71 min Scan# 1127

Delta R.T. 0.01 min

Lab File: VV016175.D

Acq: 22 May 2020 17:00


Tgt Ion: 56 Resp: 6197

Ion Ratio Lower Upper

56 100

69 32.3 24.2 36.2

84 85.6 68.3 102.5

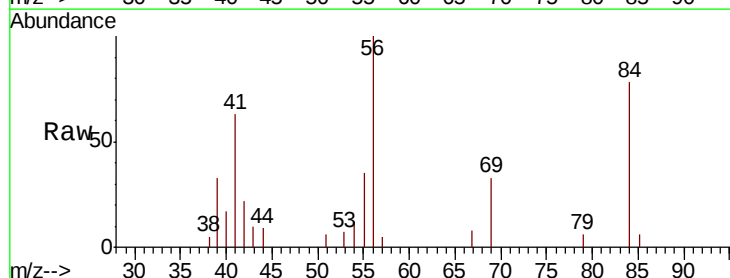

Abundance Ion 56.10 (55.80 to 56.80): VV0

Ion 69.15 (68.85 to 69.85): VV0

Ion 84.15 (83.85 to 84.85): VV0

