

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
 Data File : VV016181.D
 Acq On : 22 May 2020 19:19
 Operator : SY/MD
 Sample : L2751-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y33

Manual Integrations
 APPROVED

MMDadoda
 5/26/2020 9:35:15 AM

Quant Time: May 25 01:45:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 23 05:08:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	129813	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	125889	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	58368	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	40023	5.68	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.60%
7) Chloroethane-d5	1.58	69	35071	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.00%
11) 1,1-Dichloroethene-d2	2.12	63	65546	4.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.60%
20) 2-Butanone-d5	3.96	46	68300	34.00	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	68.00%
24) Chloroform-d	4.38	84	75877	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.06	65	40796	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	5.08	84	154176	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.10	67	46213	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.34	98	142022	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
45) trans-1,3-Dichloropropene-	7.65	79	15711	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
48) 2-Hexanone-d5	8.12	63	64018	40.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.22%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	29457	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	49545	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%

Target Compounds				Ovalue
13) Acetone	2.28	43	10815m	8.161 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052220\
Data File : VV016181.D
Acq On : 22 May 2020 19:19
Operator : SY/MD
Sample : L2751-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0Y33

Manual Integrations
APPROVED

MMDadoda
5/26/2020 9:35:15 AM

Quant Time: May 25 01:45:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 23 05:08:14 2020
Response via : Initial Calibration

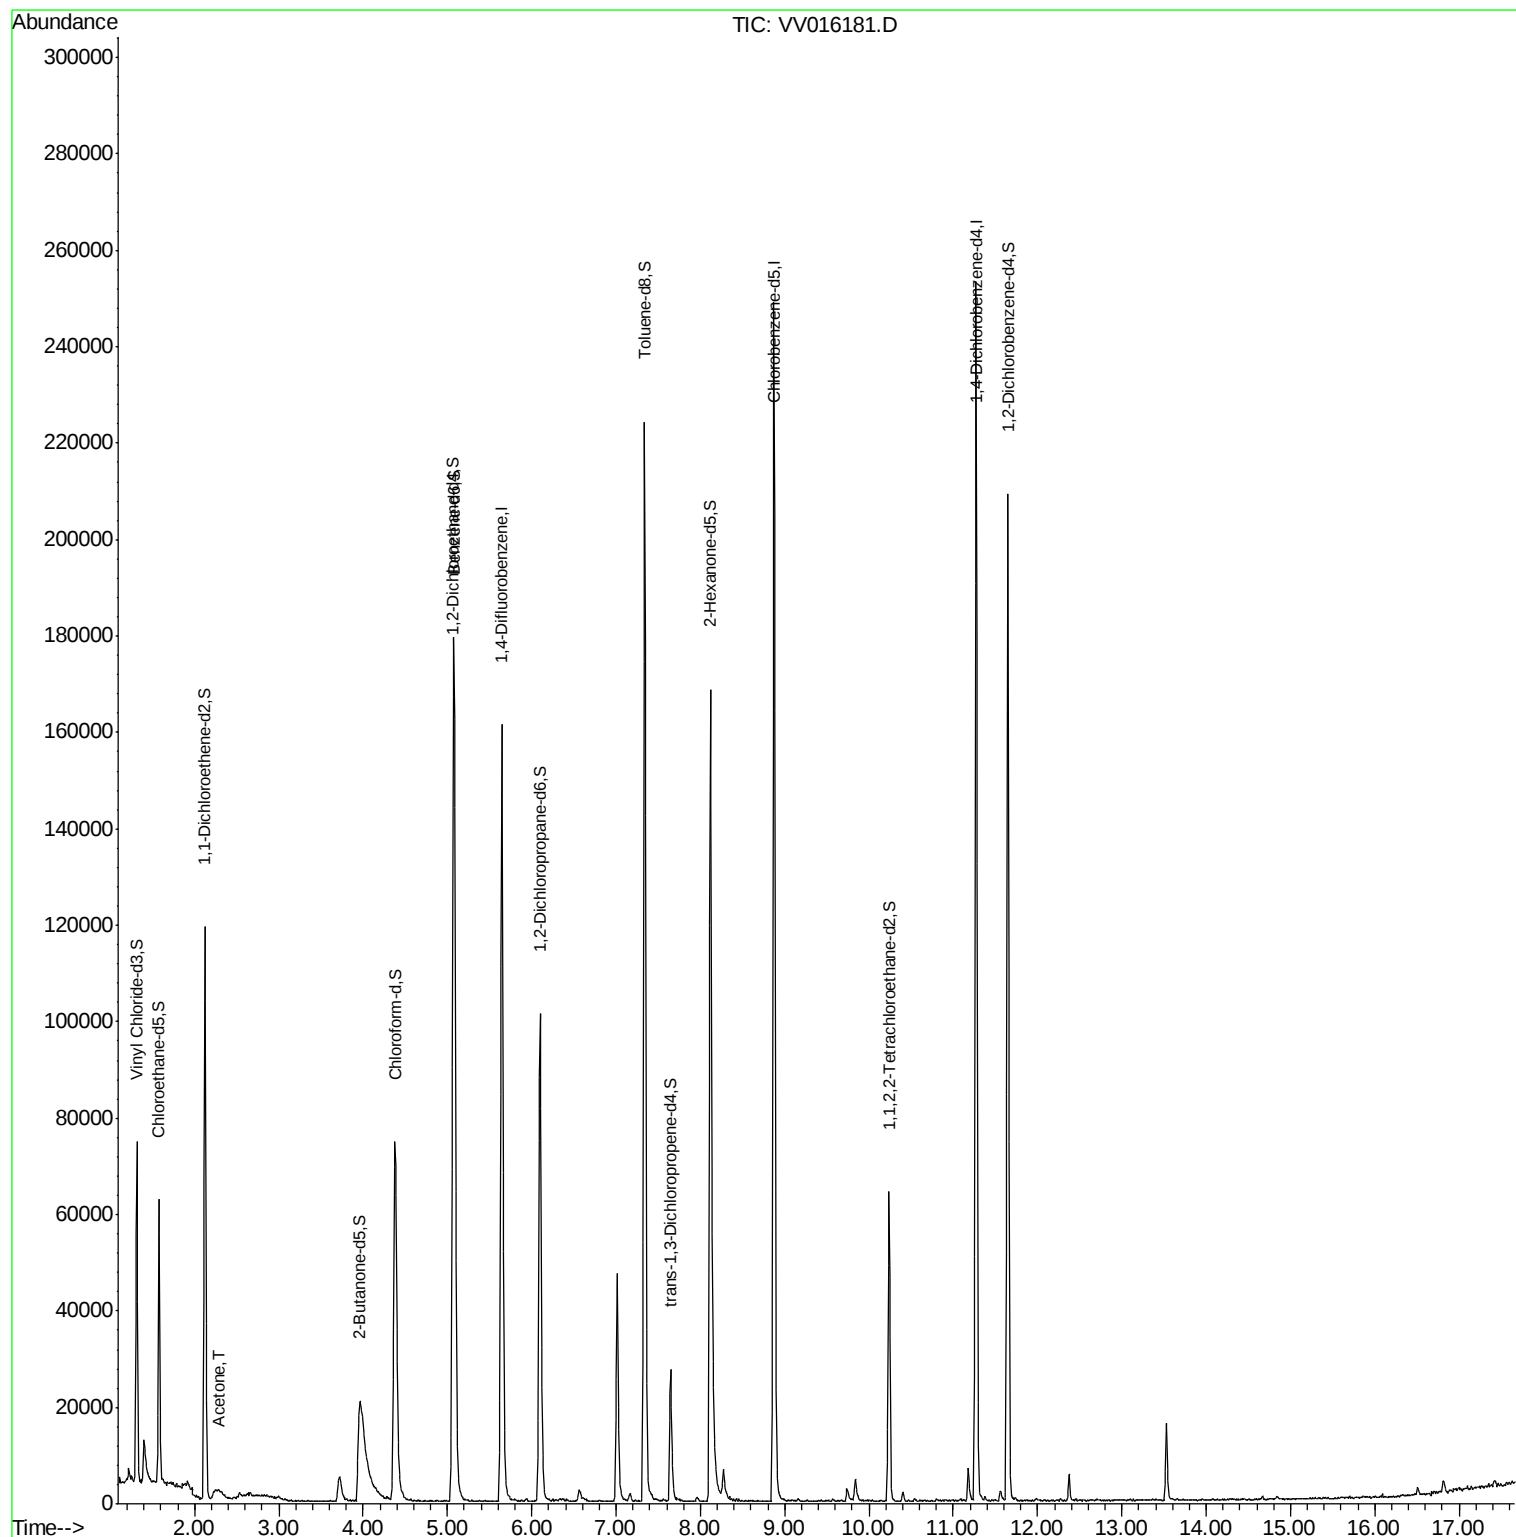

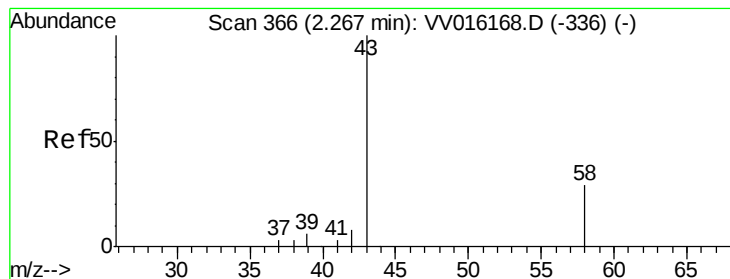

#13

Acetone

Concen: 8.161 ug/L m

RT: 2.28 min Scan# 370

Delta R.T. 0.01 min

Lab File: VV016181.D

Acq: 22 May 2020 19:19

Tot Ion: 43 Resp: 10815

Ion Ratio Lower Upper

43 100

58 5.7 0.0 30.8

Instrument :

MSVOA_V

ClientSampleId :

C0Y33

Manual Integrations

APPROVED

MMDadoda

5/26/2020 9:35:15 AM

