


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052220\
 Data File : VV016167.D
 Acq On : 22 May 2020 12:03
 Operator : SY/MD
 Sample : BFB62
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat May 23 05:08:14 2020

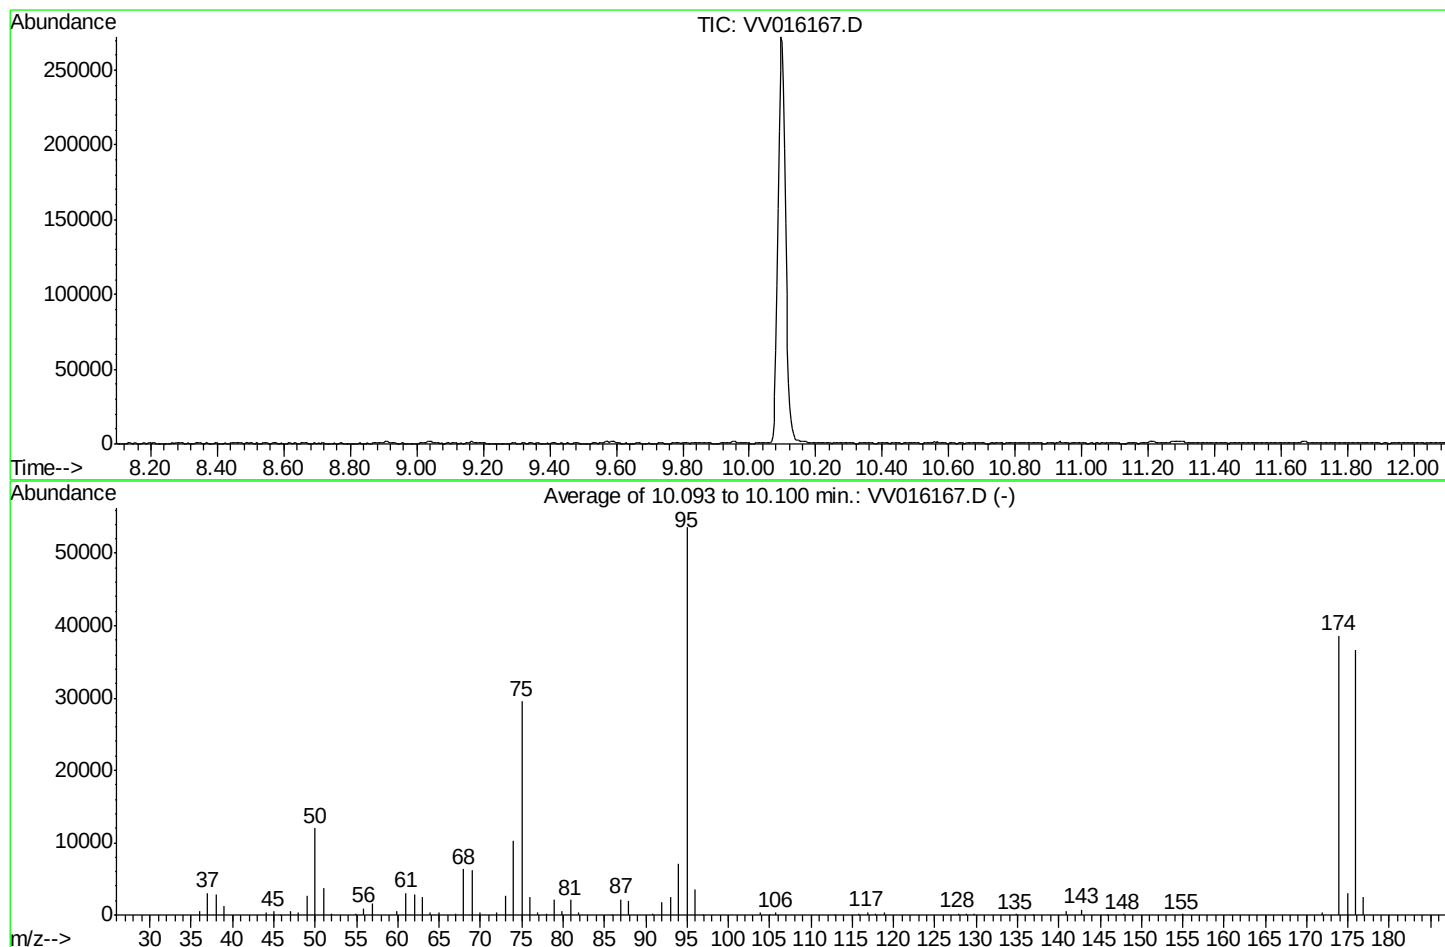

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	11955	PASS
75	95	30	80	55.1	29549	PASS
95	95	100	100	100.0	53594	PASS
96	95	5	9	6.6	3561	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	38634	PASS
175	174	5	9	7.8	3031	PASS
176	174	95	101	95.0	36714	PASS
177	176	5	9	6.7	2469	PASS

m/z	Abundance
36.00	605.0
37.00	2935.0
38.00	2630.0
39.00	1121.0
39.90	279.0
44.00	513.0
45.00	548.0
46.90	636.0
47.90	377.0
49.00	2634.0
50.00	11674.0
51.00	3434.0
51.90	180.0
55.00	165.0
55.90	933.0
57.00	1709.0
59.90	567.0
61.00	2977.0
62.00	2800.0
63.00	2399.0
63.90	306.0
65.00	251.0
67.00	226.0
68.00	5948.0
69.00	5964.0
70.00	396.0
71.90	279.0
73.00	2597.0
74.00	9741.0
75.00	28424.0
76.00	2429.0
76.90	296.0
78.00	210.0
78.90	2037.0
79.90	602.0
80.90	2032.0
81.80	414.0
87.00	2013.0
87.90	1786.0
90.80	252.0
92.00	1684.0
92.90	2451.0
94.00	6709.0
95.00	50816.0
96.00	3472.0
103.80	286.0
105.80	311.0
115.80	244.0
116.80	356.0
117.80	242.0
118.90	253.0
127.80	233.0
128.80	110.0
129.80	175.0
134.80	119.0
136.80	122.0
140.90	586.0
142.80	696.0
147.80	120.0
155.00	154.0
171.90	369.0
173.90	36104.0
175.00	2839.0
175.90	34296.0
176.90	2294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	593.0
37.00	3090.0
38.00	2892.0
39.00	1233.0
39.90	265.0
44.00	567.0
45.00	535.0
45.90	116.0
46.90	645.0
47.90	393.0
49.00	2803.0
50.00	12364.0
51.00	3834.0
52.00	185.0
55.00	184.0
55.90	983.0
57.00	1722.0
59.90	636.0
61.00	3162.0
62.00	2864.0
63.00	2552.0
63.90	346.0
65.00	291.0
67.00	230.0
68.00	6545.0
69.00	6330.0
70.00	435.0
71.90	336.0
73.00	2828.0
74.00	10590.0
75.00	30536.0
76.00	2597.0
76.90	301.0
78.10	212.0
78.90	2170.0
79.90	623.0
80.90	2203.0
81.90	450.0
85.90	101.0
87.00	2272.0
87.90	2018.0
90.80	283.0
92.00	1822.0
92.90	2629.0
94.00	7267.0
95.00	55280.0
96.00	3661.0
96.90	104.0
103.90	342.0
104.90	105.0
105.80	356.0
112.80	109.0
115.90	267.0
116.80	367.0
117.80	241.0
118.90	278.0
127.80	228.0
128.80	123.0
129.80	188.0
134.80	135.0
136.80	111.0
140.90	568.0
142.80	749.0
147.80	123.0
154.90	144.0
171.90	412.0
173.90	39816.0
175.00	3111.0
175.90	37760.0
176.90	2573.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	539.0
37.00	3057.0
38.00	2824.0
39.00	1228.0
39.90	265.0
44.00	602.0
45.00	461.0
45.80	105.0
47.00	580.0
47.90	378.0
49.00	2656.0
50.00	11828.0
51.00	3870.0
52.00	172.0
54.90	192.0
55.90	971.0
57.00	1552.0
59.90	646.0
61.00	3019.0
62.00	2735.0
63.00	2458.0
63.90	338.0
65.00	301.0
67.00	220.0
68.00	6395.0
69.00	6210.0
70.00	465.0
71.90	350.0
73.00	2814.0
74.00	10476.0
75.00	29688.0
76.00	2550.0
76.90	295.0
78.10	205.0
78.90	2090.0
79.90	599.0
80.90	2116.0
81.90	475.0
85.90	102.0
87.00	2305.0
87.90	2098.0
90.80	275.0
92.00	1717.0
93.00	2564.0
94.00	7037.0
95.00	54688.0
96.00	3552.0
96.90	110.0
103.90	328.0
105.80	353.0
112.80	102.0
115.90	254.0
116.80	354.0
117.80	263.0
118.90	326.0
127.80	220.0
128.80	114.0
129.80	191.0
134.80	136.0
140.90	525.0
142.80	759.0
145.90	114.0
147.90	110.0
154.90	144.0
171.90	400.0
173.90	39984.0
175.00	3144.0
175.90	38088.0
176.90	2540.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Scan 2788 (10.055 min): VV016167.D
BFB62

m/z	Abundance
40.00	295.0
44.00	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62