




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Manual IntegrationsAPPROVED

Quant Time: May 23 04:49:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 23 04:42:12 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

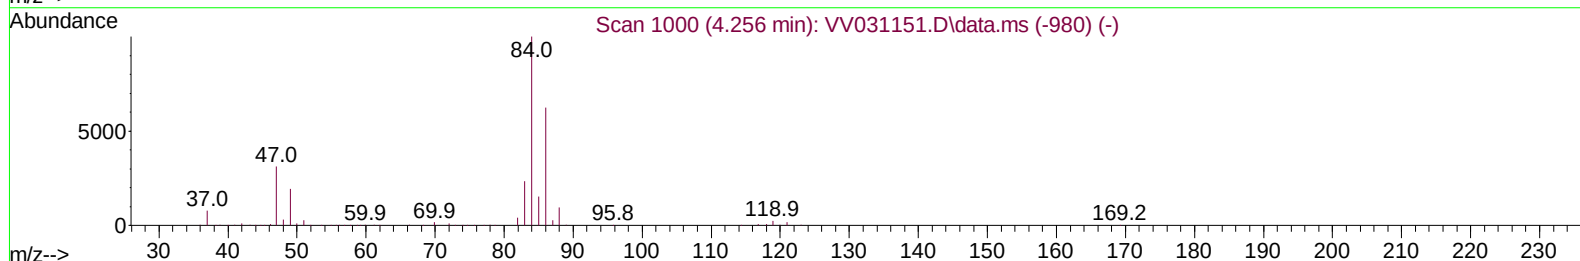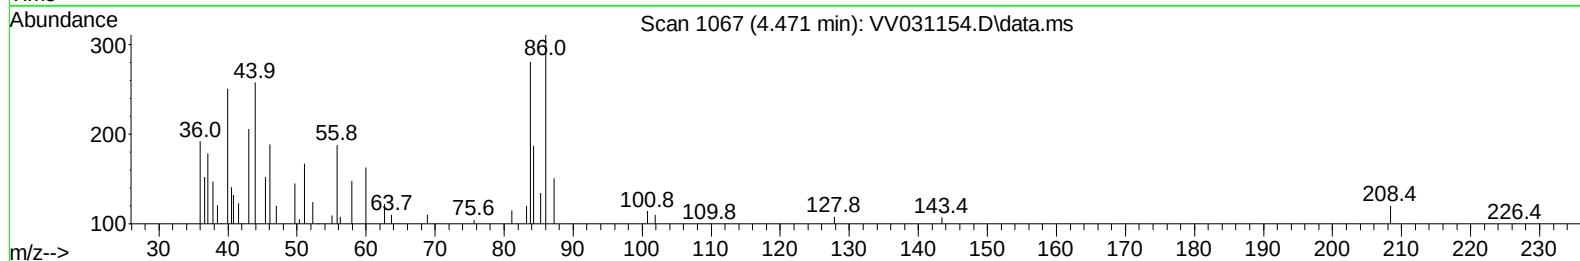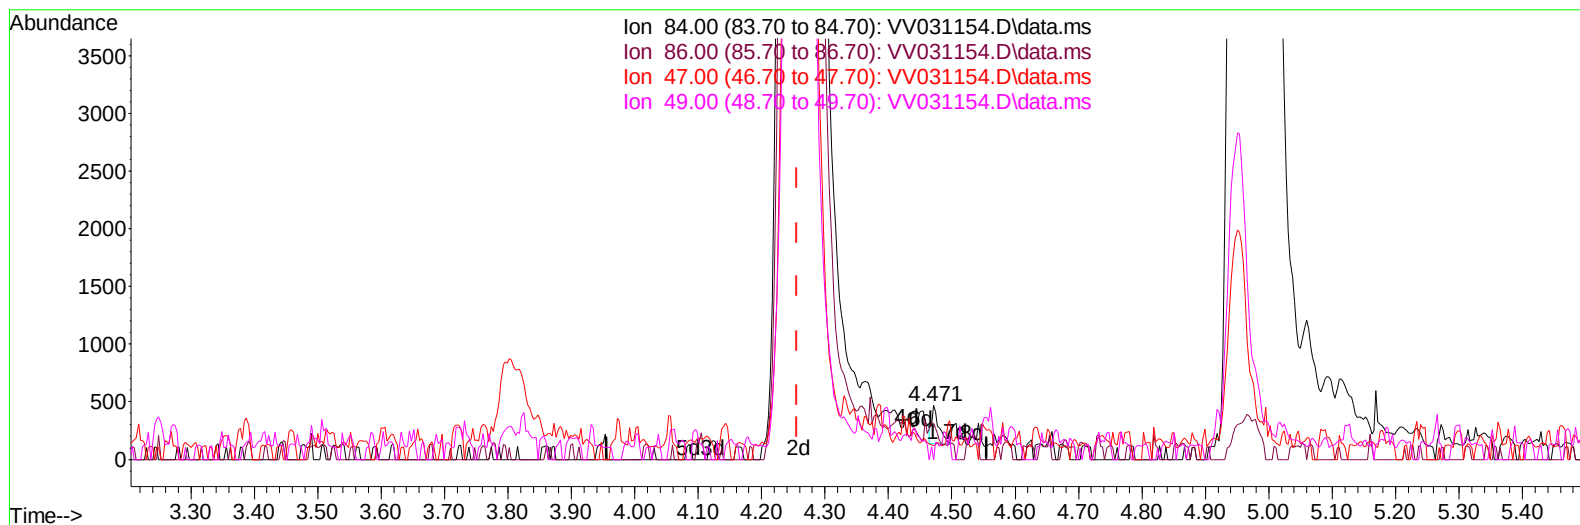

TIC: VV031154.D\data.ms

(24) Chloroform-d (S)

4.471min (+ 0.216) 0.07 ug/L

response 247

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	62.75
47.00	49.40	41.70
49.00	30.30	31.58




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Manual IntegrationsAPPROVED

Quant Time: May 23 04:49:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 23 04:42:12 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

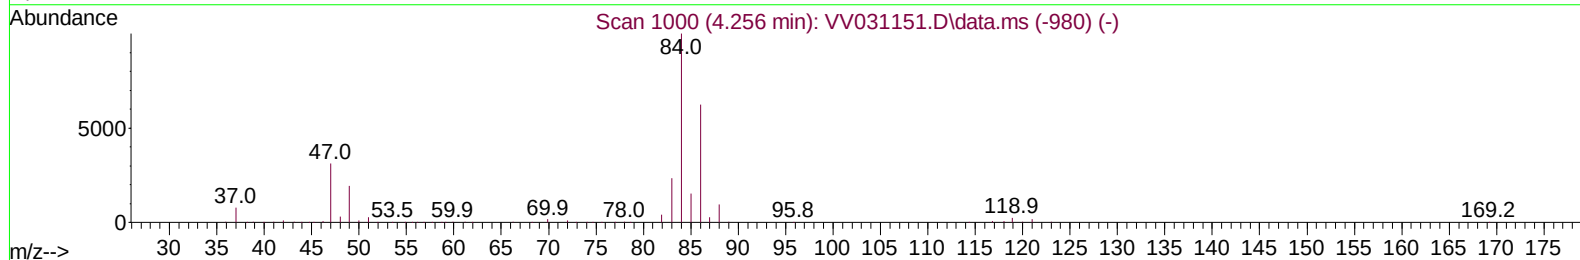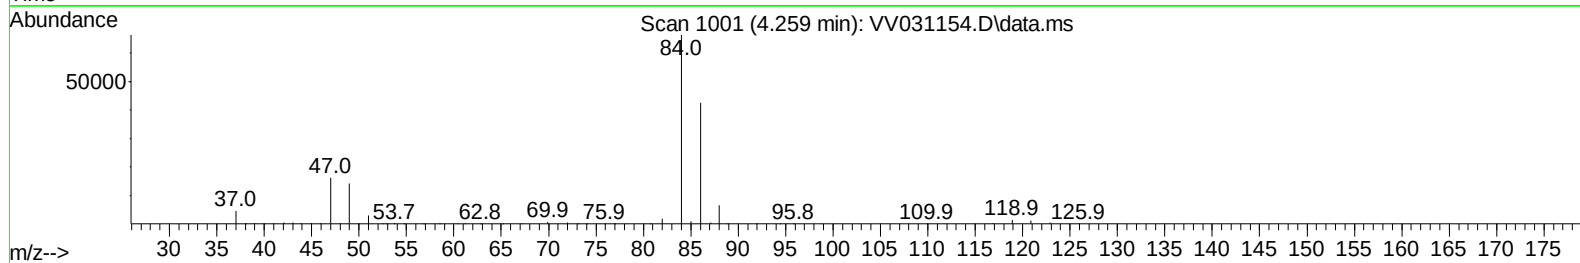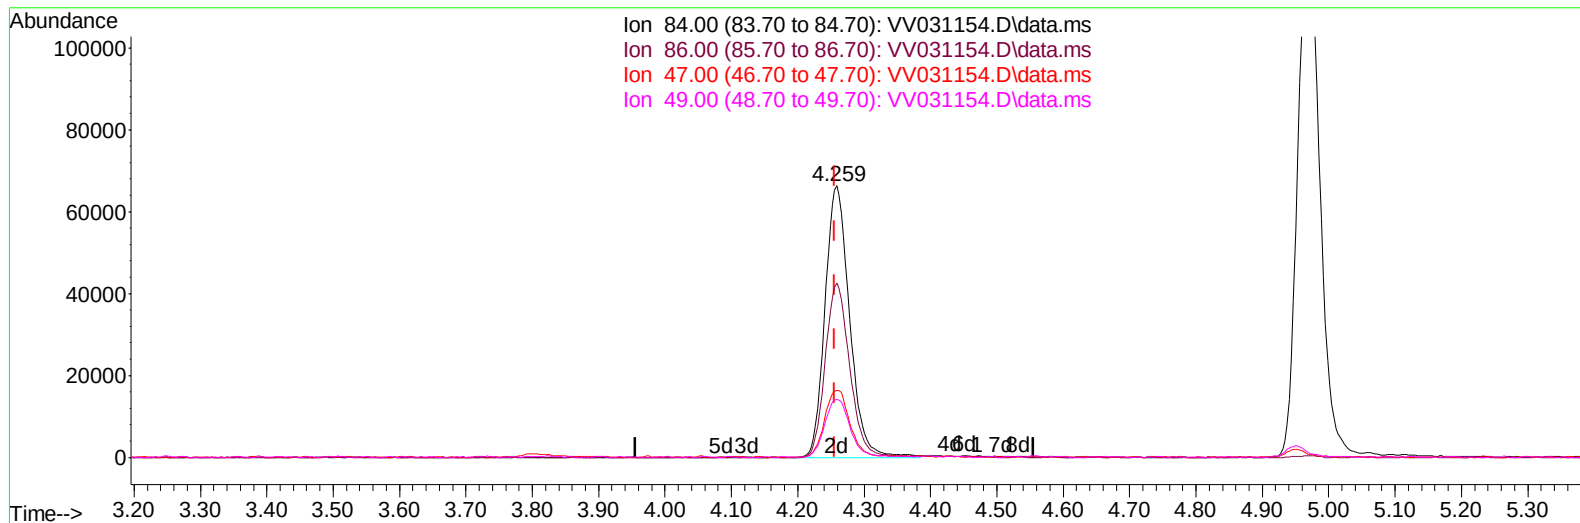

TIC: VV031154.D\data.ms

(24) Chloroform-d (S)

4.259min (+ 0.003) 46.00 ug/L m

response 170409

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.09#
47.00	49.40	0.06#
49.00	30.30	0.05#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Manual IntegrationsAPPROVED

Quant Time: May 23 04:49:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 23 04:42:12 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	245016	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	214082	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	114048	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	82785	39.535	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	79.080%	
7) Chloroethane-d5	1.536	69	73502	45.565	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	91.140%	
11) 1,1-Dichloroethene-d2	2.066	65	41355	42.116	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	84.240%	
21) 2-Butanone-d5	3.799	46	105293	94.369	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	94.370%	
24) Chloroform-d	4.259	84	170409m	46.002	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	4.950	65	121800	48.658	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.320%	
32) Benzene-d6	4.970	84	300183	51.724	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.440%	
36) 1,2-Dichloropropane-d6	5.995	67	92420	53.222	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.440%	
41) Toluene-d8	7.249	98	236686	43.696	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...	7.558	79	40667	46.679	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	93.360%	
47) 2-Hexanone-d5	8.034	63	57893	85.508	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	85.510%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	112277	43.109	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	86.220%	
66) 1,2-Dichlorobenzene-d4	11.567	152	104004	50.748	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	101.500%	
Target Compounds						
20) cis-1,2-Dichloroethene	3.828	96	2285	1.473	ug/L	88
34) Trichloroethene	5.841	95	119195	86.735	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031154.D
Acq On : 22 May 2023 10:37
Operator : SY/MD
Sample : 02866-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81DL

Manual IntegrationsAPPROVED

Quant Time: May 23 04:49:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 23 04:42:12 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

