

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031153.D
 Acq On : 22 May 2023 10:13
 Operator : SY/MD
 Sample : 02866-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	130511	141591	14.43%	1.738%
2	1.535	148	154	167	rVB	122664	146662	14.95%	1.800%
3	2.066	310	319	332	rVB	248380	361103	36.80%	4.433%
4	2.259	377	379	380	rBV2	1378	551	0.06%	0.007%
5	2.349	402	407	408	rBV5	1981	1289	0.13%	0.016%
6	2.596	482	484	488	rVB5	1777	730	0.07%	0.009%
7	2.667	503	506	509	rBV4	1427	984	0.10%	0.012%
8	2.796	542	546	553	rBV10	1467	2063	0.21%	0.025%
9	2.969	596	600	601	rBV4	2178	1249	0.13%	0.015%
10	3.075	629	633	634	rBV4	1455	1092	0.11%	0.013%
11	3.137	647	652	659	rVB10	2275	3492	0.36%	0.043%
12	3.162	659	660	664	rBV3	1329	848	0.09%	0.010%
13	3.239	679	684	686	rBV6	2081	1910	0.19%	0.023%
14	3.291	697	700	703	rBV4	1894	933	0.10%	0.011%
15	3.313	704	707	709	rVV4	1954	1097	0.11%	0.013%
16	3.330	710	712	715	rVB4	2004	1119	0.11%	0.014%
17	3.349	715	718	719	rBV3	992	605	0.06%	0.007%
18	3.400	732	734	738	rVB5	1892	1203	0.12%	0.015%
19	3.445	746	748	751	rBV4	1143	636	0.06%	0.008%
20	3.500	763	765	767	rBV3	1194	523	0.05%	0.006%
21	3.577	785	789	793	rVB8	2217	2011	0.20%	0.025%
22	3.603	793	797	803	rBV7	2802	3383	0.34%	0.042%
23	3.632	803	806	809	rVV5	1726	1327	0.14%	0.016%
24	3.648	809	811	815	rBV5	1033	711	0.07%	0.009%
25	3.754	842	844	848	rBV5	816	470	0.05%	0.006%
26	3.802	848	859	881	rBV2	61529	183384	18.69%	2.251%
27	4.172	968	974	975	rBV5	1363	1425	0.15%	0.017%
28	4.256	987	1000	1024	rVB	166102	413714	42.16%	5.078%
29	4.571	1093	1098	1099	rBV5	1660	1468	0.15%	0.018%
30	4.674	1126	1130	1132	rBV5	1521	1191	0.12%	0.015%
31	4.796	1165	1168	1169	rBV3	1447	714	0.07%	0.009%
32	4.902	1197	1201	1203	rBV5	2028	1630	0.17%	0.020%
33	4.966	1203	1221	1245	rVV2	367644	981227	100.00%	12.045%
34	5.542	1388	1400	1425	rBV	305629	635454	64.76%	7.800%
35	5.841	1482	1493	1514	rVB	295118	580450	59.16%	7.125%
36	5.995	1530	1541	1563	rVB2	224494	455057	46.38%	5.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031153.D
 Acq On : 22 May 2023 10:13
 Operator : SY/MD
 Sample : 02866-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.702	1759	1761	1763	rBV4	1779	879	0.09%	0.011%
38	6.754	1774	1777	1779	rBV4	2030	1314	0.13%	0.016%
39	6.767	1779	1781	1785	rVB5	1680	1000	0.10%	0.012%
40	6.786	1785	1787	1788	rBV2	1298	458	0.05%	0.006%
41	6.857	1806	1809	1812	rVB5	1589	861	0.09%	0.011%
42	6.870	1812	1813	1815	rBV2	1013	250	0.03%	0.003%
43	6.918	1818	1828	1848	rVV	108067	205139	20.91%	2.518%
44	7.185	1910	1911	1913	rBV2	1356	420	0.04%	0.005%
45	7.249	1921	1931	1956	rBV	410477	724432	73.83%	8.892%
46	7.558	2019	2027	2044	rBV	80484	141700	14.44%	1.739%
47	7.812	2104	2106	2109	rBV4	1401	818	0.08%	0.010%
48	7.847	2113	2117	2119	rBV5	2751	2033	0.21%	0.025%
49	8.001	2161	2165	2166	rBV4	1602	1109	0.11%	0.014%
50	8.033	2166	2175	2204	rVV	189315	403105	41.08%	4.948%
51	8.464	2305	2309	2312	rBV6	2071	2049	0.21%	0.025%
52	8.612	2353	2355	2356	rBV2	814	365	0.04%	0.004%
53	8.792	2397	2411	2436	rBV	473118	805437	82.08%	9.887%
54	9.191	2532	2535	2536	rBV3	1303	791	0.08%	0.010%
55	9.242	2550	2551	2553	rBV2	770	293	0.03%	0.004%
56	9.477	2620	2624	2625	rBV3	1657	1133	0.12%	0.014%
57	9.496	2628	2630	2633	rVV4	2308	1322	0.13%	0.016%
58	9.673	2681	2685	2691	rBV9	2151	2801	0.29%	0.034%
59	9.779	2716	2718	2721	rBV4	2041	1475	0.15%	0.018%
60	9.857	2740	2742	2746	rBV5	1214	911	0.09%	0.011%
61	10.069	2806	2808	2809	rBV2	1216	532	0.05%	0.007%
62	10.159	2824	2836	2855	rBV	305983	492369	50.18%	6.044%
63	10.323	2884	2887	2889	rBV3	2975	2260	0.23%	0.028%
64	10.397	2908	2910	2917	rVB7	2974	1882	0.19%	0.023%
65	10.429	2917	2920	2925	rVB6	1983	2043	0.21%	0.025%
66	10.458	2925	2929	2930	rBV4	2077	1381	0.14%	0.017%
67	10.577	2965	2966	2967	rBV	1292	423	0.04%	0.005%
68	10.606	2974	2975	2978	rVB3	2042	622	0.06%	0.008%
69	10.619	2978	2979	2981	rBV2	1445	513	0.05%	0.006%
70	10.754	3020	3021	3024	rBV3	1372	553	0.06%	0.007%
71	11.017	3101	3103	3105	rBV2	1685	947	0.10%	0.012%
72	11.078	3116	3122	3125	rBV8	2297	2623	0.27%	0.032%
73	11.127	3136	3137	3141	rVB3	1633	800	0.08%	0.010%
74	11.143	3141	3142	3145	rBV3	1351	589	0.06%	0.007%
75	11.191	3145	3157	3175	rBV	442753	716162	72.99%	8.791%
76	11.435	3231	3233	3235	rBV2	1573	1048	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031153.D
 Acq On : 22 May 2023 10:13
 Operator : SY/MD
 Sample : 02866-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX80DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	11.490	3248	3250	3251	rBV2	1360	505	0.05%	0.006%
78	11.567	3264	3274	3291	rBV	417598	674403	68.73%	8.278%
79	12.098	3437	3439	3441	rBV3	1632	635	0.06%	0.008%
80	12.130	3447	3449	3451	rBV3	2002	974	0.10%	0.012%
81	12.963	3704	3708	3709	rBV4	1514	1009	0.10%	0.012%
82	13.149	3763	3766	3768	rBV4	1457	903	0.09%	0.011%
83	13.242	3793	3795	3797	rVB3	1287	358	0.04%	0.004%
84	13.255	3797	3799	3800	rBV2	1293	413	0.04%	0.005%
85	13.319	3814	3819	3821	rBV5	1815	1923	0.20%	0.024%
86	13.570	3893	3897	3900	rBV5	1605	1273	0.13%	0.016%
87	13.673	3924	3929	3930	rBV5	1824	1408	0.14%	0.017%
88	13.876	3989	3992	3995	rVB4	2153	1512	0.15%	0.019%
89	14.413	4156	4159	4161	rBV4	1687	1161	0.12%	0.014%
90	14.525	4192	4194	4196	rBV3	2072	786	0.08%	0.010%
91	15.548	4510	4512	4515	rBV4	2397	1263	0.13%	0.016%




Sum of corrected areas: 8146664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031153.D
Acq On : 22 May 2023 10:13
Operator : SY/MD
Sample : 02866-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

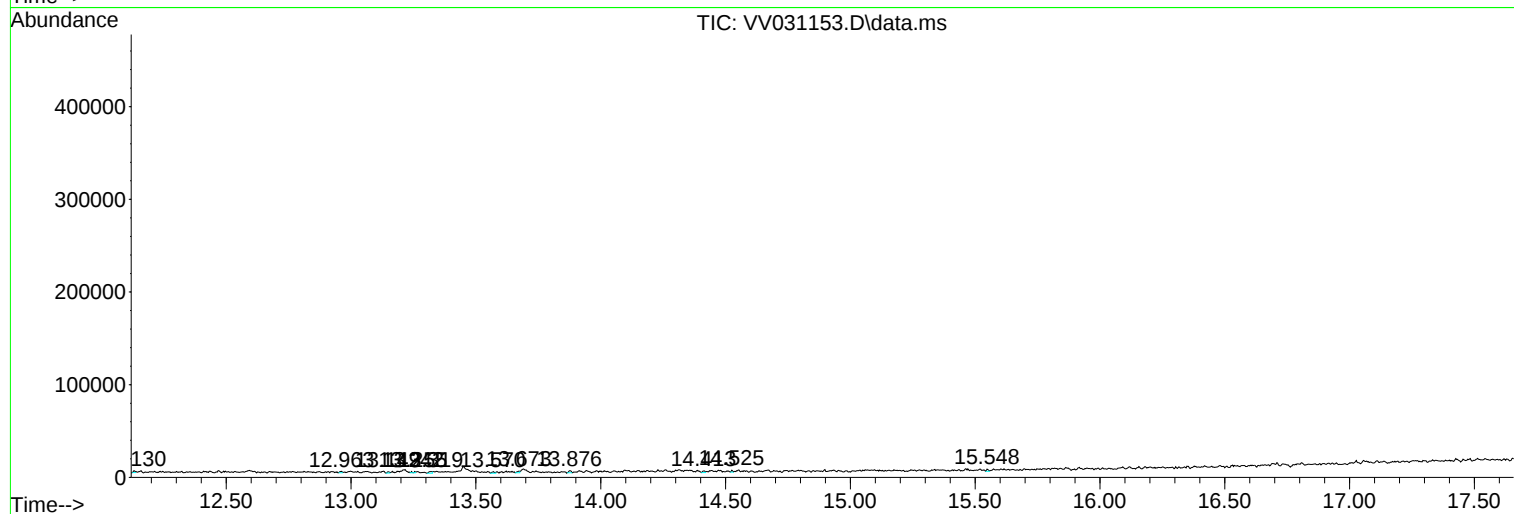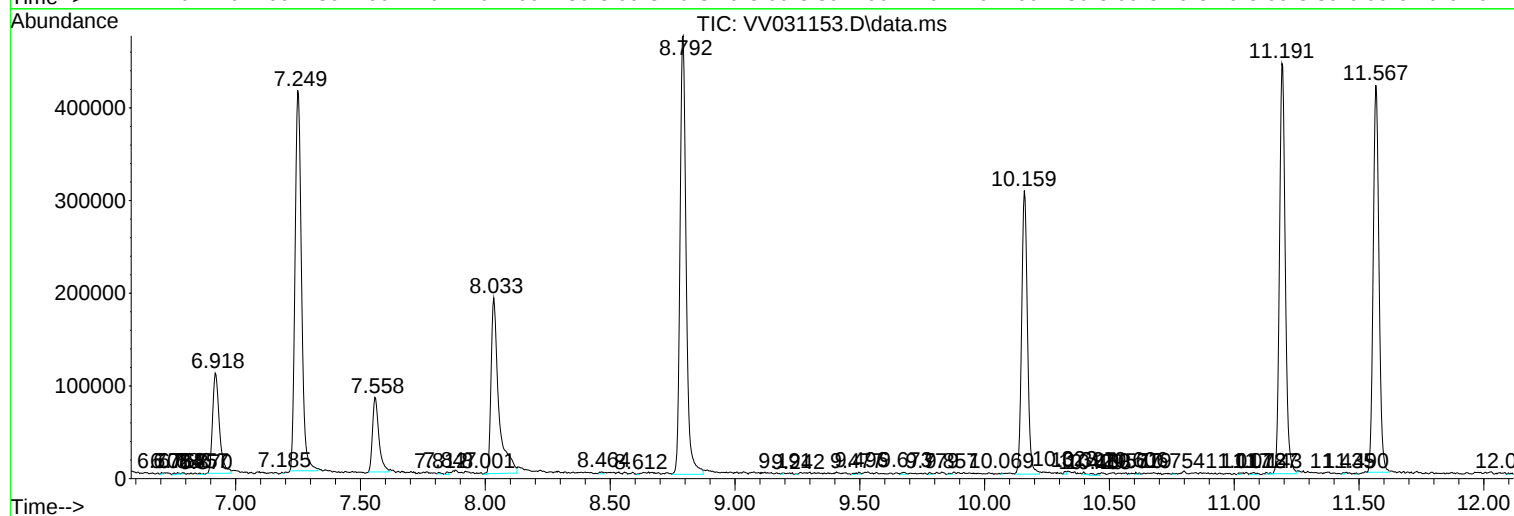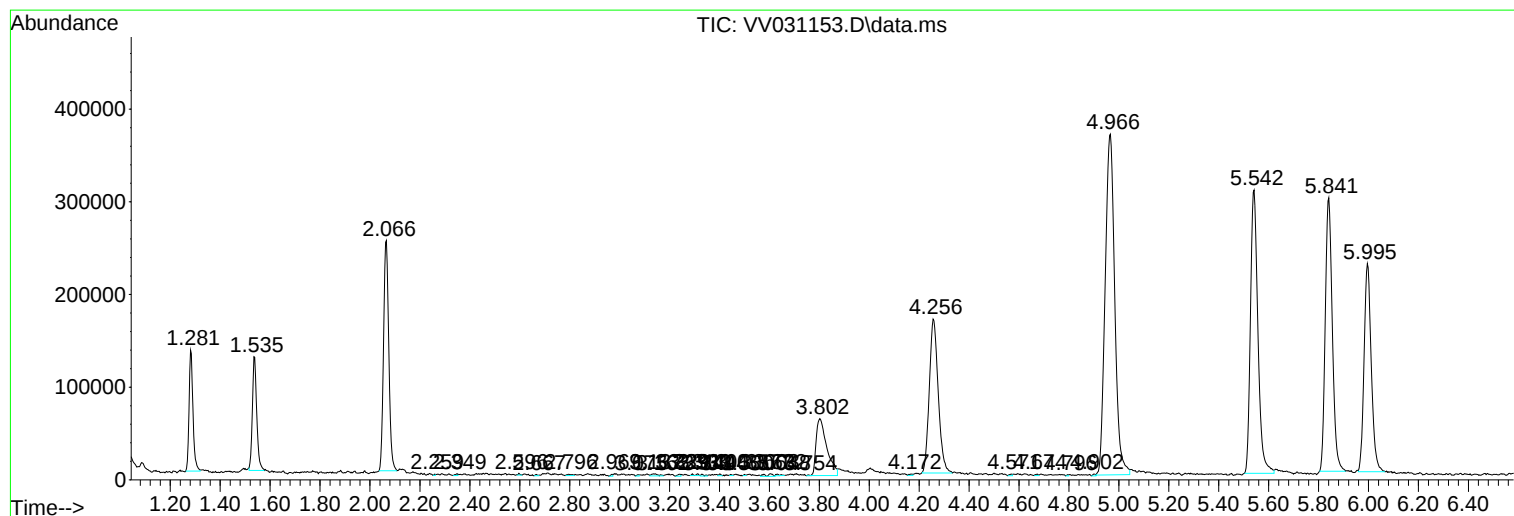

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031153.D
Acq On : 22 May 2023 10:13
Operator : SY/MD
Sample : 02866-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031153.D
Acq On : 22 May 2023 10:13
Operator : SY/MD
Sample : 02866-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------