

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rBV	121731	137626	14.20%	1.761%
2	1.536	148	154	165	rVB	109919	133404	13.76%	1.707%
3	2.066	309	319	334	rBV	246440	365139	37.67%	4.672%
4	2.581	477	479	480	rBV3	1500	408	0.04%	0.005%
5	2.764	532	536	540	rBV6	1876	1623	0.17%	0.021%
6	2.835	556	558	561	rVB3	2211	1098	0.11%	0.014%
7	2.944	590	592	593	rBV2	1217	505	0.05%	0.006%
8	3.143	651	654	657	rBV5	2217	1738	0.18%	0.022%
9	3.169	659	662	665	rVV4	1204	823	0.08%	0.011%
10	3.185	665	667	669	rBV4	1376	636	0.07%	0.008%
11	3.259	688	690	691	rBV3	1550	626	0.06%	0.008%
12	3.632	804	806	809	rBV3	1475	960	0.10%	0.012%
13	3.757	842	845	849	rBV6	2638	1676	0.17%	0.021%
14	3.799	849	858	886	rBV	58502	179942	18.56%	2.302%
15	4.259	987	1001	1019	rBV2	160408	404119	41.69%	5.171%
16	4.738	1145	1150	1152	rBV6	2161	1888	0.19%	0.024%
17	4.767	1157	1159	1160	rBV2	1278	403	0.04%	0.005%
18	4.825	1174	1177	1179	rBV3	1791	1051	0.11%	0.013%
19	4.879	1192	1194	1196	rBV3	1583	780	0.08%	0.010%
20	4.966	1204	1221	1243	rBV2	363530	969437	100.00%	12.404%
21	5.497	1384	1386	1387	rBV2	1401	479	0.05%	0.006%
22	5.542	1388	1400	1421	rVV	290665	603880	62.29%	7.727%
23	5.841	1481	1493	1516	rBV	357865	714896	73.74%	9.147%
24	5.995	1530	1541	1560	rBV	221599	446179	46.02%	5.709%
25	6.397	1664	1666	1667	rBV2	1827	794	0.08%	0.010%
26	6.506	1694	1700	1707	rBV10	1663	2590	0.27%	0.033%
27	6.535	1707	1709	1711	rBV3	2096	1194	0.12%	0.015%
28	6.648	1743	1744	1747	rBV3	1234	567	0.06%	0.007%
29	6.690	1753	1757	1760	rBV4	1747	1515	0.16%	0.019%
30	6.841	1802	1804	1805	rBV2	1128	438	0.05%	0.006%
31	6.850	1805	1807	1810	rVV5	1526	847	0.09%	0.011%
32	6.918	1818	1828	1842	rBV	101794	187317	19.32%	2.397%
33	7.182	1907	1910	1913	rBV4	1291	1096	0.11%	0.014%
34	7.249	1920	1931	1953	rBV	368824	660655	68.15%	8.453%
35	7.558	2019	2027	2049	rBV2	72915	128071	13.21%	1.639%
36	7.773	2092	2094	2095	rBV2	1235	649	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.847	2115	2117	2118	rBV2	1342	517	0.05%	0.007%
38	7.953	2148	2150	2151	rBV2	1757	603	0.06%	0.008%
39	8.034	2166	2175	2207	rBV	171644	364275	37.58%	4.661%
40	8.461	2305	2308	2313	rBV7	1527	1587	0.16%	0.020%
41	8.487	2313	2316	2318	rBV5	1298	862	0.09%	0.011%
42	8.587	2344	2347	2348	rBV3	1814	999	0.10%	0.013%
43	8.625	2356	2359	2361	rBV3	1323	839	0.09%	0.011%
44	8.680	2373	2376	2380	rBV6	1042	572	0.06%	0.007%
45	8.722	2388	2389	2392	rBV2	1302	675	0.07%	0.009%
46	8.747	2394	2397	2398	rBV2	1210	767	0.08%	0.010%
47	8.793	2400	2411	2429	rVV	405604	672768	69.40%	8.608%
48	9.079	2497	2500	2503	rBV4	1888	1562	0.16%	0.020%
49	9.281	2561	2563	2567	rVB5	735	394	0.04%	0.005%
50	9.349	2582	2584	2588	rBV5	1148	891	0.09%	0.011%
51	9.426	2605	2608	2611	rBV5	1246	866	0.09%	0.011%
52	9.448	2613	2615	2617	rVV3	1200	665	0.07%	0.009%
53	9.461	2617	2619	2624	rVV6	1380	1170	0.12%	0.015%
54	9.484	2624	2626	2631	rVB6	1447	1105	0.11%	0.014%
55	9.513	2631	2635	2638	rBV5	1175	852	0.09%	0.011%
56	9.558	2646	2649	2652	rVB5	804	536	0.06%	0.007%
57	9.574	2652	2654	2656	rBV3	1087	629	0.06%	0.008%
58	9.686	2687	2689	2693	rVB5	1239	681	0.07%	0.009%
59	9.738	2703	2705	2706	rBV2	1159	587	0.06%	0.008%
60	9.789	2719	2721	2722	rBV2	1099	449	0.05%	0.006%
61	9.799	2722	2724	2727	rVB5	1395	753	0.08%	0.010%
62	9.854	2739	2741	2745	rVB4	1196	615	0.06%	0.008%
63	9.873	2745	2747	2748	rBV2	1008	424	0.04%	0.005%
64	9.918	2759	2761	2767	rVB5	1313	1086	0.11%	0.014%
65	9.947	2767	2770	2773	rBV4	1399	897	0.09%	0.011%
66	9.966	2773	2776	2779	rBV5	2149	1557	0.16%	0.020%
67	9.985	2779	2782	2785	rVB4	1332	814	0.08%	0.010%
68	10.001	2785	2787	2789	rVB2	1191	528	0.05%	0.007%
69	10.018	2789	2792	2796	rVB5	1570	1261	0.13%	0.016%
70	10.050	2799	2802	2803	rBV2	2117	1267	0.13%	0.016%
71	10.091	2813	2815	2816	rBV2	1456	584	0.06%	0.007%
72	10.159	2823	2836	2859	rBV2	269397	433069	44.67%	5.541%
73	10.243	2861	2862	2863	rBV	1532	366	0.04%	0.005%
74	10.275	2868	2872	2873	rBV3	1094	737	0.08%	0.009%
75	10.378	2903	2904	2909	rBV5	1566	939	0.10%	0.012%
76	10.464	2929	2931	2935	rBV4	1704	1349	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031154.D
 Acq On : 22 May 2023 10:37
 Operator : SY/MD
 Sample : 02866-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX81DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	10.593	2969	2971	2972	rBV2	1576	622	0.06%	0.008%
78	10.619	2977	2979	2982	rVB4	1530	705	0.07%	0.009%
79	10.702	3004	3005	3009	rBV3	1171	544	0.06%	0.007%
80	10.770	3018	3026	3030	rBV9	1714	2688	0.28%	0.034%
81	10.789	3030	3032	3033	rBV2	987	473	0.05%	0.006%
82	10.854	3049	3052	3053	rBV3	1196	752	0.08%	0.010%
83	10.905	3066	3068	3070	rBV3	1792	915	0.09%	0.012%
84	10.950	3078	3082	3085	rBV5	1293	1198	0.12%	0.015%
85	10.969	3085	3088	3092	rVB5	1358	989	0.10%	0.013%
86	10.995	3092	3096	3103	rVB8	2329	2970	0.31%	0.038%
87	11.040	3107	3110	3111	rBV3	1285	504	0.05%	0.006%
88	11.056	3113	3115	3119	rBV4	1536	832	0.09%	0.011%
89	11.085	3122	3124	3126	rBV3	1513	843	0.09%	0.011%
90	11.191	3146	3157	3178	rBV	425515	677276	69.86%	8.666%
91	11.567	3263	3274	3290	rBV	403452	657036	67.78%	8.407%
92	12.034	3417	3419	3423	rVB4	2723	1460	0.15%	0.019%
93	12.564	3583	3584	3587	rBV3	1564	998	0.10%	0.013%
94	12.651	3608	3611	3612	rBV3	1892	890	0.09%	0.011%
95	12.706	3626	3628	3630	rBV3	1325	617	0.06%	0.008%
96	12.812	3659	3661	3663	rBV3	2089	1020	0.11%	0.013%
97	13.017	3722	3725	3730	rBV7	2321	2032	0.21%	0.026%
98	13.911	3998	4003	4005	rBV5	1819	1643	0.17%	0.021%
99	13.998	4028	4030	4033	rBV4	1369	954	0.10%	0.012%
100	14.448	4168	4170	4172	rBV3	1970	1212	0.13%	0.016%




Sum of corrected areas: 7815319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031154.D
Acq On : 22 May 2023 10:37
Operator : SY/MD
Sample : 02866-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

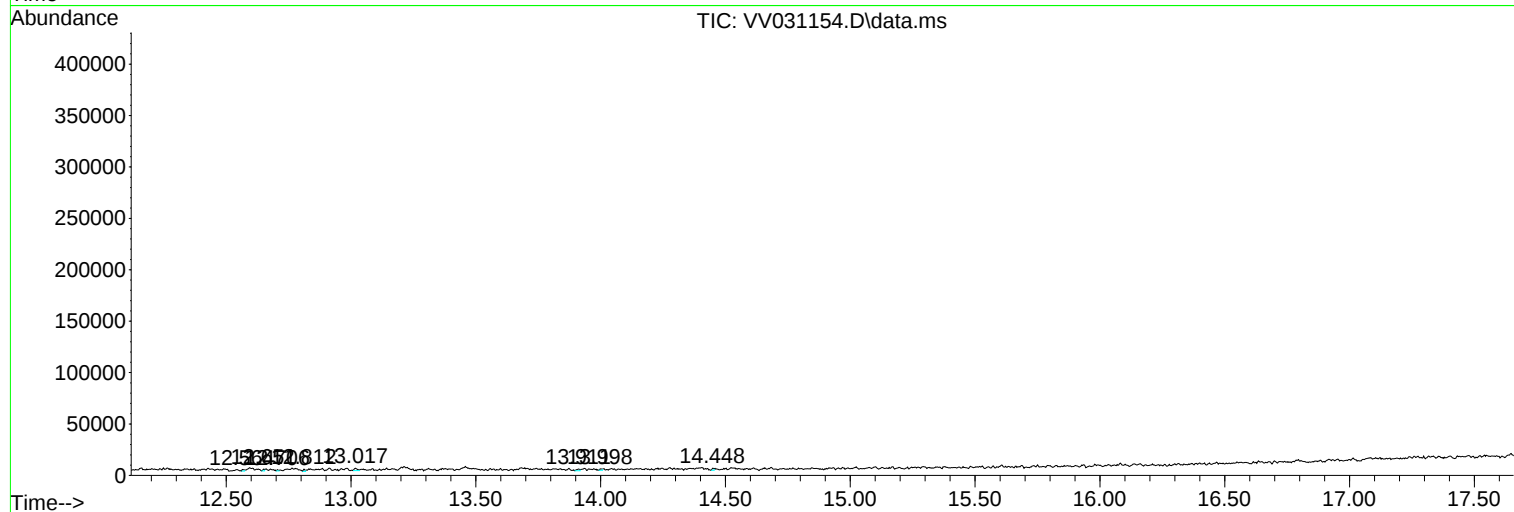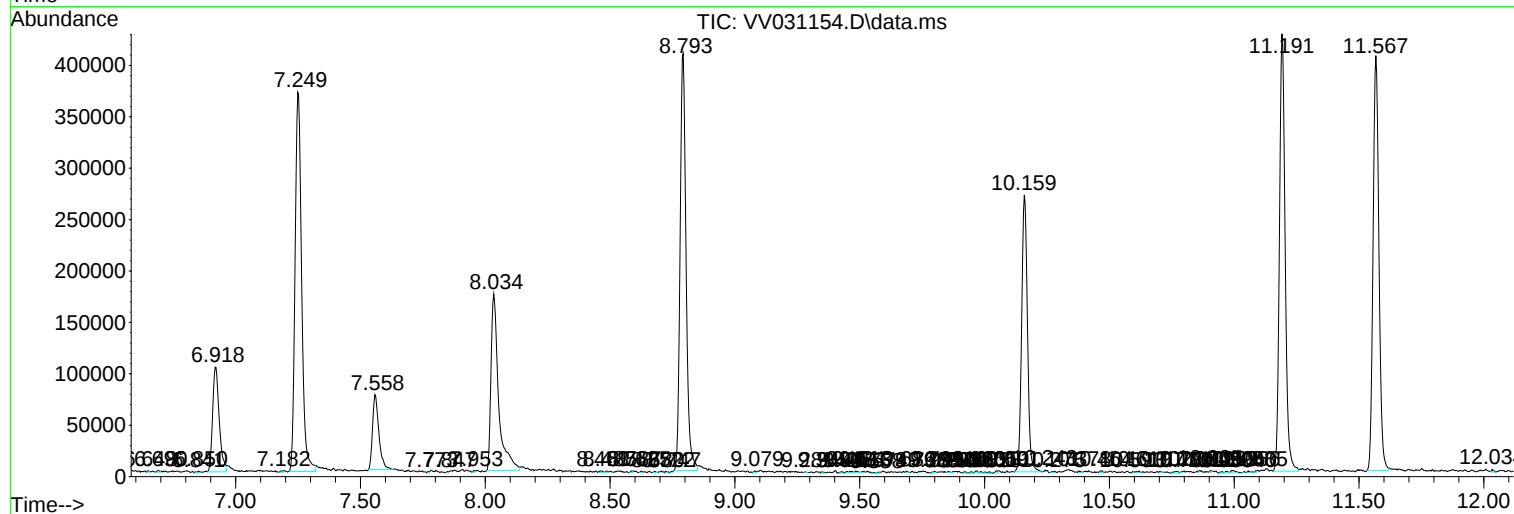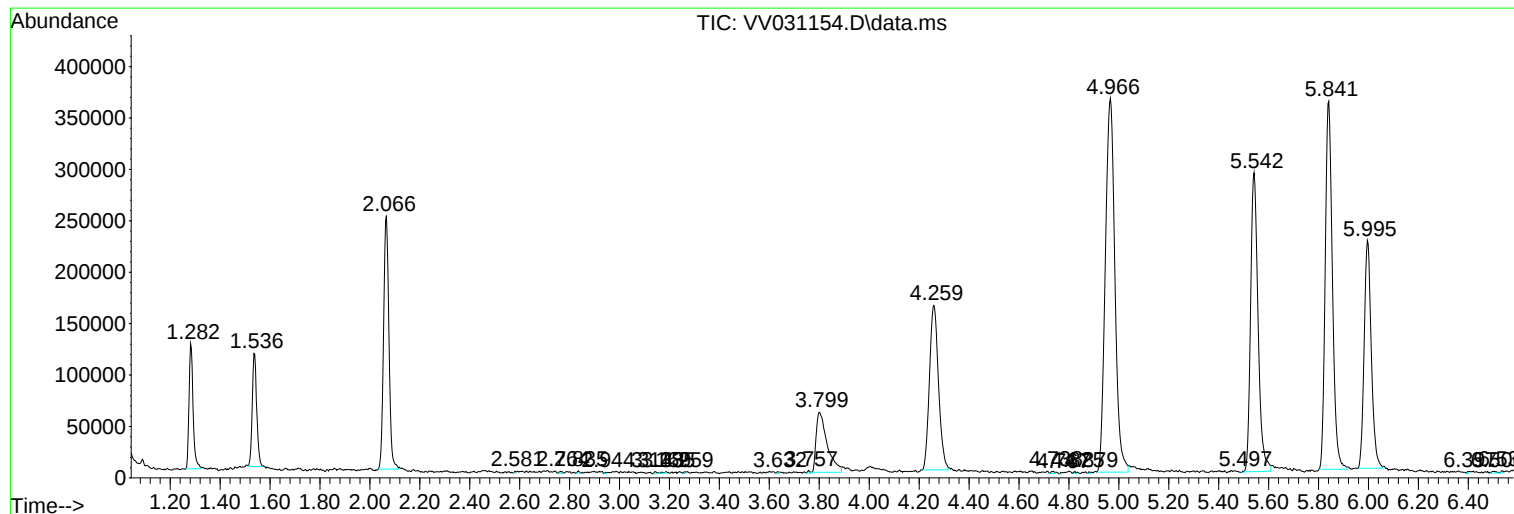

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031154.D
Acq On : 22 May 2023 10:37
Operator : SY/MD
Sample : 02866-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031154.D
Acq On : 22 May 2023 10:37
Operator : SY/MD
Sample : 02866-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------