

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031155.D
 Acq On : 22 May 2023 11:01
 Operator : SY/MD
 Sample : 02866-07DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX82DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	96	rVB	123086	142543	14.50%	1.786%
2	1.535	148	154	173	rVB	123591	151167	15.38%	1.894%
3	2.066	310	319	334	rVB	251197	361590	36.78%	4.529%
4	2.529	462	463	464	rBV	1355	478	0.05%	0.006%
5	2.834	555	558	562	rBV6	1797	1334	0.14%	0.017%
6	2.992	603	607	610	rBV6	1854	1665	0.17%	0.021%
7	3.056	625	627	630	rBV4	1521	900	0.09%	0.011%
8	3.227	678	680	681	rBV	1140	375	0.04%	0.005%
9	3.413	737	738	739	rBV	1303	469	0.05%	0.006%
10	3.461	749	753	758	rBV7	1868	1966	0.20%	0.025%
11	3.574	786	788	791	rBV4	1552	1146	0.12%	0.014%
12	3.693	822	825	827	rBV4	2348	1395	0.14%	0.017%
13	3.802	849	859	884	rBV	65954	208193	21.18%	2.608%
14	4.259	988	1001	1024	rVB2	177361	418804	42.60%	5.246%
15	4.529	1083	1085	1089	rBV6	1507	807	0.08%	0.010%
16	4.760	1154	1157	1160	rBV4	1638	1358	0.14%	0.017%
17	4.966	1205	1221	1244	rBV3	373940	983006	100.00%	12.313%
18	5.436	1365	1367	1370	rBV4	1767	913	0.09%	0.011%
19	5.542	1386	1400	1425	rBV	301586	633076	64.40%	7.930%
20	5.841	1482	1493	1511	rBV	218437	435403	44.29%	5.454%
21	5.995	1530	1541	1560	rBV	224180	451691	45.95%	5.658%
22	6.680	1752	1754	1755	rBV	2073	812	0.08%	0.010%
23	6.918	1819	1828	1848	rBV	111229	209002	21.26%	2.618%
24	7.088	1879	1881	1882	rBV2	1526	461	0.05%	0.006%
25	7.249	1920	1931	1948	rBV	413721	731000	74.36%	9.157%
26	7.558	2018	2027	2040	rBV2	83161	147172	14.97%	1.844%
27	7.953	2148	2150	2156	rBV6	2518	2452	0.25%	0.031%
28	8.034	2164	2175	2207	rBV	191797	423679	43.10%	5.307%
29	8.516	2322	2325	2331	rBV8	2409	2826	0.29%	0.035%
30	8.792	2400	2411	2429	rBV	465982	765822	77.91%	9.593%
31	9.406	2600	2602	2604	rBV3	1559	657	0.07%	0.008%
32	9.966	2772	2776	2778	rBV5	1476	1235	0.13%	0.015%
33	10.008	2787	2789	2790	rBV2	889	358	0.04%	0.004%
34	10.098	2815	2817	2818	rBV3	1527	652	0.07%	0.008%
35	10.159	2825	2836	2852	rBV	311361	496314	50.49%	6.217%
36	10.410	2911	2914	2916	rBV3	1816	1000	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031155.D
 Acq On : 22 May 2023 11:01
 Operator : SY/MD
 Sample : 02866-07DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX82DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.628	2978	2982	2984	rBV5	1849	1307	0.13%	0.016%
38	10.747	3017	3019	3022	rBV3	1429	914	0.09%	0.011%
39	10.847	3048	3050	3051	rBV	1595	642	0.07%	0.008%
40	10.908	3067	3069	3071	rBV3	1049	634	0.06%	0.008%
41	11.085	3122	3124	3127	rBV4	1811	1326	0.13%	0.017%
42	11.191	3147	3157	3176	rVB	427960	688399	70.03%	8.623%
43	11.567	3264	3274	3292	rVB	419657	673145	68.48%	8.432%
44	11.866	3363	3367	3370	rBV6	2709	2519	0.26%	0.032%
45	12.139	3448	3452	3453	rBV4	2039	1362	0.14%	0.017%
46	12.400	3531	3533	3534	rBV2	1508	686	0.07%	0.009%
47	12.500	3562	3564	3565	rBV2	1352	525	0.05%	0.007%
48	12.644	3605	3609	3612	rBV5	1937	1477	0.15%	0.019%
49	12.660	3612	3614	3618	rVB5	1793	1197	0.12%	0.015%
50	12.689	3621	3623	3626	rBV4	1404	1026	0.10%	0.013%
51	12.831	3665	3667	3672	rBV6	1699	1124	0.11%	0.014%
52	12.879	3679	3682	3683	rBV2	1395	928	0.09%	0.012%
53	12.927	3695	3697	3699	rBV3	1250	559	0.06%	0.007%
54	12.972	3709	3711	3712	rBV2	2497	953	0.10%	0.012%
55	13.001	3718	3720	3722	rBV3	853	315	0.03%	0.004%
56	13.049	3733	3735	3736	rBV2	888	361	0.04%	0.005%
57	13.075	3740	3743	3744	rBV3	807	324	0.03%	0.004%
58	13.136	3760	3762	3763	rBV2	888	236	0.02%	0.003%
59	13.156	3766	3768	3769	rBV2	1319	479	0.05%	0.006%
60	13.233	3790	3792	3794	rBV3	900	634	0.06%	0.008%
61	13.258	3798	3800	3802	rBV2	1318	624	0.06%	0.008%
62	13.352	3826	3829	3832	rBV4	1465	1137	0.12%	0.014%
63	13.429	3851	3853	3856	rVB3	1121	540	0.05%	0.007%
64	13.522	3880	3882	3884	rBV2	871	491	0.05%	0.006%
65	13.561	3892	3894	3895	rBV2	1985	883	0.09%	0.011%
66	13.686	3931	3933	3934	rBV2	1277	698	0.07%	0.009%
67	13.725	3942	3945	3946	rBV3	949	445	0.05%	0.006%
68	13.734	3946	3948	3950	rBV3	1226	656	0.07%	0.008%
69	13.831	3977	3978	3979	rBV	965	252	0.03%	0.003%
70	13.927	4005	4008	4011	rBV4	2366	1321	0.13%	0.017%
71	13.946	4011	4014	4016	rVV3	1403	806	0.08%	0.010%
72	14.130	4069	4071	4074	rBV4	1500	1046	0.11%	0.013%
73	14.226	4099	4101	4102	rBV2	1067	376	0.04%	0.005%
74	14.268	4110	4114	4116	rBV5	1891	1419	0.14%	0.018%
75	14.371	4144	4146	4149	rBV3	1385	774	0.08%	0.010%
76	14.480	4177	4180	4182	rBV4	1494	877	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031155.D
Acq On : 22 May 2023 11:01
Operator : SY/MD
Sample : 02866-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis

77	14.561	4202	4205	4208	rBV5	1682	1284	0.13%	0.016%
78	14.612	4215	4221	4223	rBV6	2152	2202	0.22%	0.028%
79	14.667	4235	4238	4244	rVB7	2434	2121	0.22%	0.027%
80	14.696	4244	4247	4249	rBV4	2076	1286	0.13%	0.016%
81	14.779	4271	4273	4275	rBV3	2231	1220	0.12%	0.015%


Sum of corrected areas: 7983251

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031155.D
Acq On : 22 May 2023 11:01
Operator : SY/MD
Sample : 02866-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

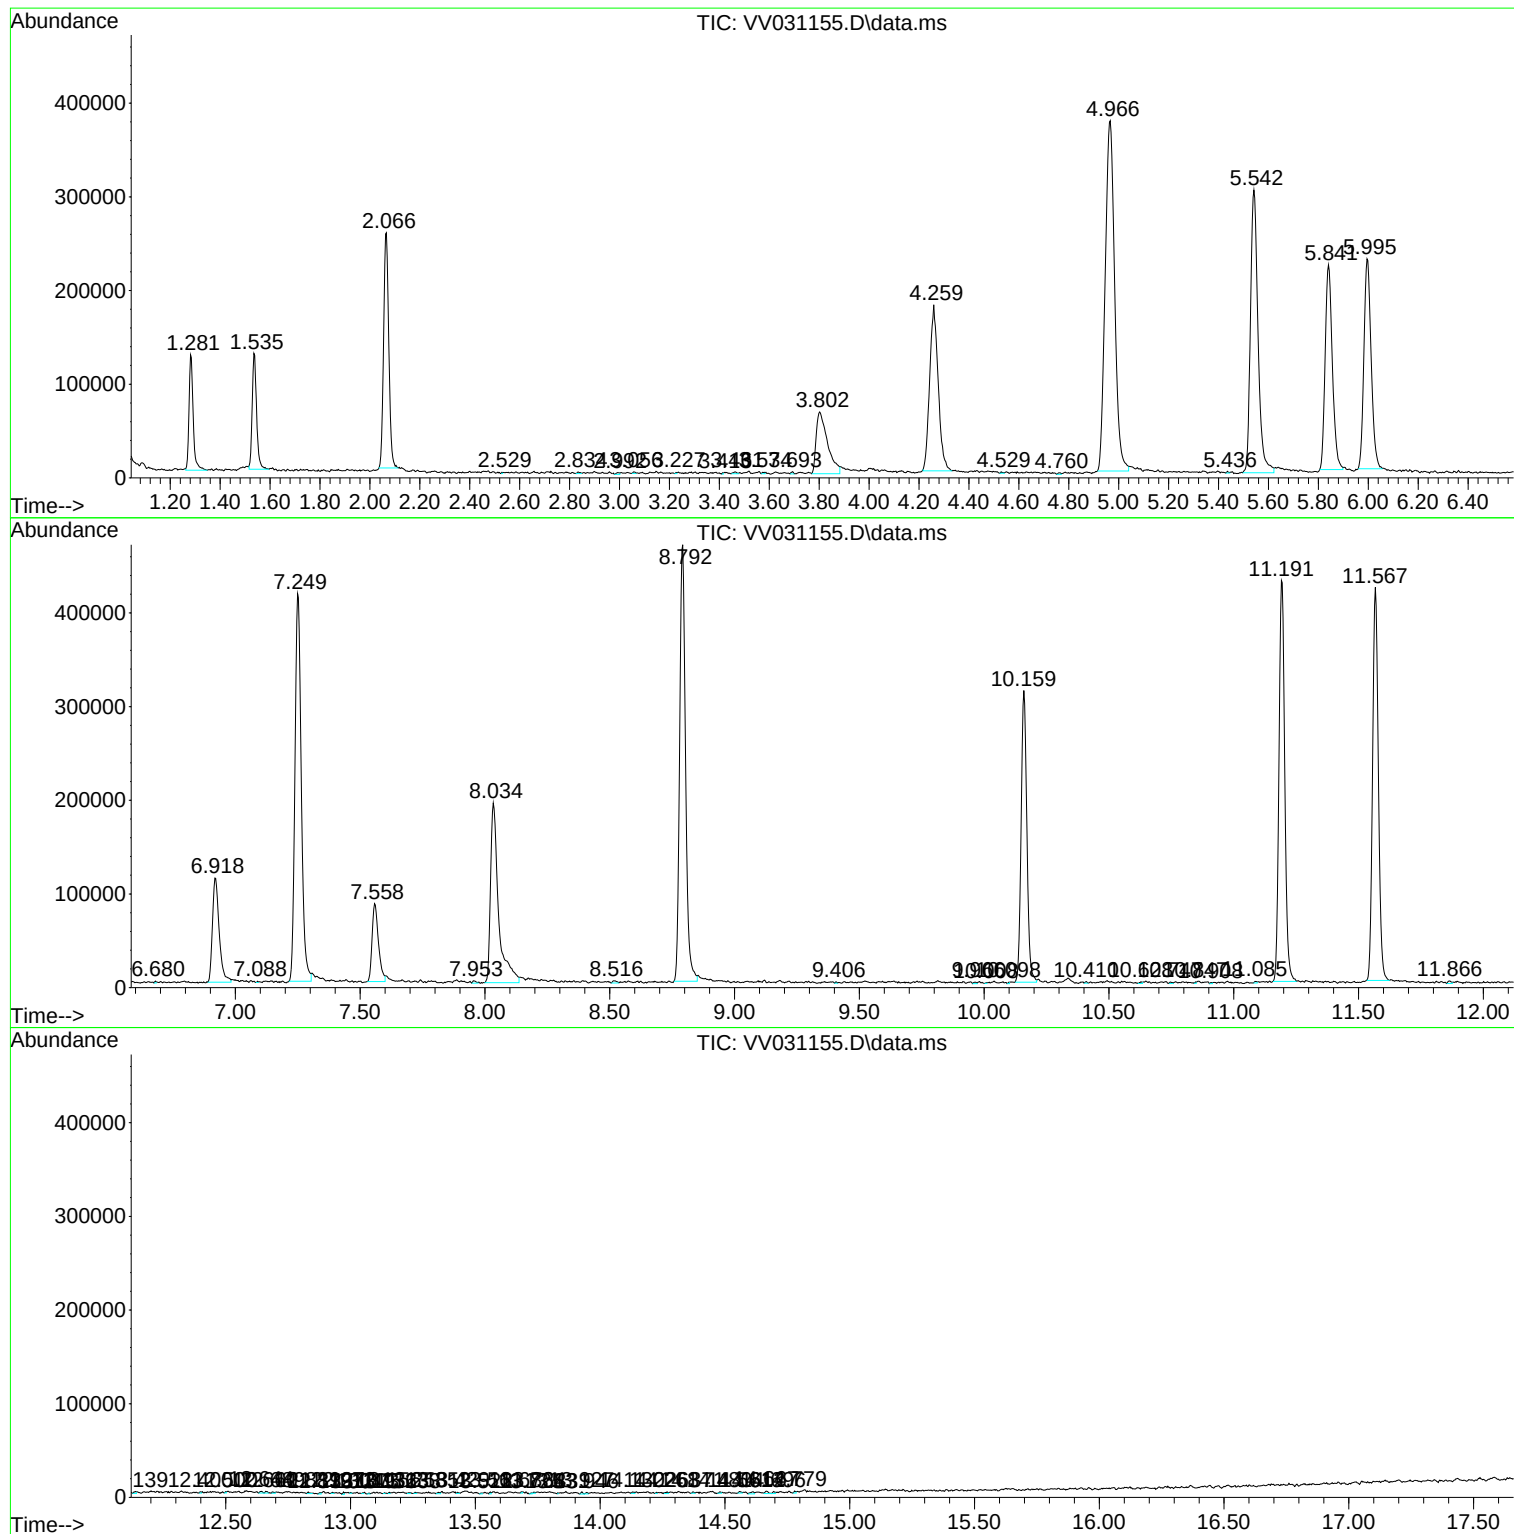

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031155.D
Acq On : 22 May 2023 11:01
Operator : SY/MD
Sample : 02866-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031155.D
Acq On : 22 May 2023 11:01
Operator : SY/MD
Sample : 02866-07DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc