

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031157.D
 Acq On : 22 May 2023 11:48
 Operator : SY/MD
 Sample : 02866-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rBV	121714	132700	13.39%	1.643%
2	1.535	148	154	166	rVB	117839	137884	13.92%	1.707%
3	2.066	309	319	333	rBV	248690	369401	37.28%	4.574%
4	2.262	378	380	387	rBV6	1512	1156	0.12%	0.014%
5	2.513	455	458	461	rBV4	1373	1024	0.10%	0.013%
6	2.696	510	515	517	rBV6	2120	2047	0.21%	0.025%
7	2.719	520	522	527	rVB6	1757	1345	0.14%	0.017%
8	2.770	536	538	541	rBV4	1634	887	0.09%	0.011%
9	2.828	549	556	558	rBV7	1520	1648	0.17%	0.020%
10	2.863	563	567	572	rVB8	1941	1951	0.20%	0.024%
11	2.889	572	575	578	rBV5	1561	1229	0.12%	0.015%
12	2.915	579	583	587	rVB6	1440	1290	0.13%	0.016%
13	2.953	592	595	598	rVB6	1876	1265	0.13%	0.016%
14	2.989	604	606	607	rBV2	2017	860	0.09%	0.011%
15	3.095	635	639	641	rBV5	2055	1275	0.13%	0.016%
16	3.182	662	666	669	rBV5	1479	1162	0.12%	0.014%
17	3.220	673	678	680	rBV6	2476	2340	0.24%	0.029%
18	3.268	690	693	695	rBV4	1786	1080	0.11%	0.013%
19	3.285	695	698	701	rVV5	1423	836	0.08%	0.010%
20	3.410	729	737	741	rBV10	2612	3575	0.36%	0.044%
21	3.503	763	766	767	rBV3	2004	1202	0.12%	0.015%
22	3.532	772	775	778	rBV4	1777	1398	0.14%	0.017%
23	3.622	800	803	805	rBV4	1472	869	0.09%	0.011%
24	3.664	815	816	822	rBV6	1701	1631	0.16%	0.020%
25	3.712	829	831	833	rBV3	1541	890	0.09%	0.011%
26	3.799	848	858	885	rBV	65578	210193	21.21%	2.603%
27	4.207	980	985	986	rBV4	2298	2013	0.20%	0.025%
28	4.259	989	1001	1024	rVB	165312	421362	42.52%	5.217%
29	4.387	1038	1041	1044	rBV4	2363	1761	0.18%	0.022%
30	4.645	1119	1121	1124	rBV4	1528	1011	0.10%	0.013%
31	4.719	1142	1144	1148	rBV4	1454	855	0.09%	0.011%
32	4.802	1168	1170	1176	rBV7	1434	1056	0.11%	0.013%
33	4.966	1203	1221	1247	rBV2	368638	990887	100.00%	12.270%
34	5.207	1294	1296	1299	rBV4	2167	1044	0.11%	0.013%
35	5.497	1384	1386	1388	rBV3	1613	1027	0.10%	0.013%
36	5.542	1388	1400	1427	rVV	310014	645685	65.16%	7.995%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031157.D
 Acq On : 22 May 2023 11:48
 Operator : SY/MD
 Sample : 02866-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.841	1482	1493	1512	rVB	217374	431587	43.56%	5.344%
38	5.995	1531	1541	1564	rVB2	218832	451603	45.58%	5.592%
39	6.297	1633	1635	1641	rVB7	1170	1042	0.11%	0.013%
40	6.339	1641	1648	1650	rBV8	2118	2249	0.23%	0.028%
41	6.468	1686	1688	1689	rBV2	1854	840	0.08%	0.010%
42	6.561	1714	1717	1719	rBV4	1804	1242	0.13%	0.015%
43	6.718	1764	1766	1768	rBV3	1508	868	0.09%	0.011%
44	6.747	1772	1775	1778	rBV5	2819	1861	0.19%	0.023%
45	6.837	1800	1803	1804	rBV3	1681	840	0.08%	0.010%
46	6.876	1811	1815	1816	rBV4	1119	882	0.09%	0.011%
47	6.921	1819	1829	1848	rBV	112414	209241	21.12%	2.591%
48	7.249	1920	1931	1952	rBV	406746	729901	73.66%	9.038%
49	7.452	1992	1994	1997	rBV4	2194	1425	0.14%	0.018%
50	7.561	2018	2028	2045	rBV	79643	147212	14.86%	1.823%
51	7.876	2120	2126	2127	rBV5	2713	2354	0.24%	0.029%
52	7.915	2136	2138	2145	rVB7	1933	1918	0.19%	0.024%
53	8.034	2164	2175	2190	rBV	195458	379604	38.31%	4.700%
54	8.455	2303	2306	2310	rBV5	1570	1424	0.14%	0.018%
55	8.516	2322	2325	2330	rBV7	2642	2510	0.25%	0.031%
56	8.622	2352	2358	2360	rBV6	1422	1514	0.15%	0.019%
57	8.792	2397	2411	2441	rBV	473230	802989	81.04%	9.943%
58	9.197	2535	2537	2538	rBV2	2772	1018	0.10%	0.013%
59	9.233	2544	2548	2550	rBV5	1614	1214	0.12%	0.015%
60	9.255	2552	2555	2557	rBV3	1381	867	0.09%	0.011%
61	9.304	2567	2570	2571	rBV3	2304	1252	0.13%	0.016%
62	9.487	2625	2627	2630	rBV3	1574	839	0.08%	0.010%
63	9.535	2639	2642	2644	rBV3	2033	1217	0.12%	0.015%
64	9.548	2644	2646	2651	rVV6	1661	1094	0.11%	0.014%
65	9.715	2695	2698	2700	rBV3	2130	1525	0.15%	0.019%
66	9.853	2738	2741	2743	rBV4	1914	1425	0.14%	0.018%
67	9.924	2761	2763	2766	rVB4	2006	952	0.10%	0.012%
68	10.159	2825	2836	2852	rBV	307310	493969	49.85%	6.117%
69	10.332	2880	2890	2893	rBV10	4941	8007	0.81%	0.099%
70	10.451	2925	2927	2932	rVB6	1717	1387	0.14%	0.017%
71	10.490	2937	2939	2941	rBV3	1744	898	0.09%	0.011%
72	10.532	2949	2952	2957	rVB7	1812	1414	0.14%	0.018%
73	10.638	2983	2985	2988	rBV3	1457	1065	0.11%	0.013%
74	10.892	3062	3064	3067	rBV4	1464	909	0.09%	0.011%
75	11.130	3134	3138	3140	rBV5	2686	2248	0.23%	0.028%
76	11.191	3146	3157	3180	rBV	442359	711566	71.81%	8.811%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031157.D
 Acq On : 22 May 2023 11:48
 Operator : SY/MD
 Sample : 02866-09DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX84DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.435	3231	3233	3236	rVB4	2779	1411	0.14%	0.017%
78	11.567	3261	3274	3294	rBV	437501	687809	69.41%	8.517%
79	11.892	3370	3375	3377	rBV5	1733	1620	0.16%	0.020%
80	11.953	3390	3394	3395	rBV3	1879	847	0.09%	0.010%
81	11.966	3395	3398	3401	rBV5	2037	1364	0.14%	0.017%
82	12.400	3529	3533	3535	rBV5	1468	1286	0.13%	0.016%
83	12.583	3587	3590	3592	rBV3	1479	891	0.09%	0.011%
84	12.635	3603	3606	3609	rBV5	1709	1309	0.13%	0.016%
85	12.660	3612	3614	3616	rBV3	1549	951	0.10%	0.012%
86	12.699	3624	3626	3628	rBV3	2163	1268	0.13%	0.016%
87	12.770	3645	3648	3653	rBV7	2279	2213	0.22%	0.027%
88	12.795	3653	3656	3662	rVB8	1814	1616	0.16%	0.020%
89	13.284	3804	3808	3812	rBV6	1879	1586	0.16%	0.020%
90	13.638	3916	3918	3923	rVV4	2025	1248	0.13%	0.015%
91	13.783	3960	3963	3967	rVB6	1924	1304	0.13%	0.016%
92	13.808	3967	3971	3974	rBV5	2166	1886	0.19%	0.023%
93	13.885	3991	3995	3996	rBV4	1568	1153	0.12%	0.014%
94	13.943	4008	4013	4014	rBV5	1595	1345	0.14%	0.017%
95	14.072	4051	4053	4060	rVB7	2801	2036	0.21%	0.025%
96	14.152	4075	4078	4081	rBV5	1953	1674	0.17%	0.021%
97	14.432	4162	4165	4167	rBV4	2472	1317	0.13%	0.016%
98	14.725	4253	4256	4261	rBV6	2184	1943	0.20%	0.024%
99	14.805	4278	4281	4285	rBV6	3038	2185	0.22%	0.027%
100	14.824	4285	4287	4291	rBV4	2408	1864	0.19%	0.023%




Sum of corrected areas: 8075937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031157.D
Acq On : 22 May 2023 11:48
Operator : SY/MD
Sample : 02866-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

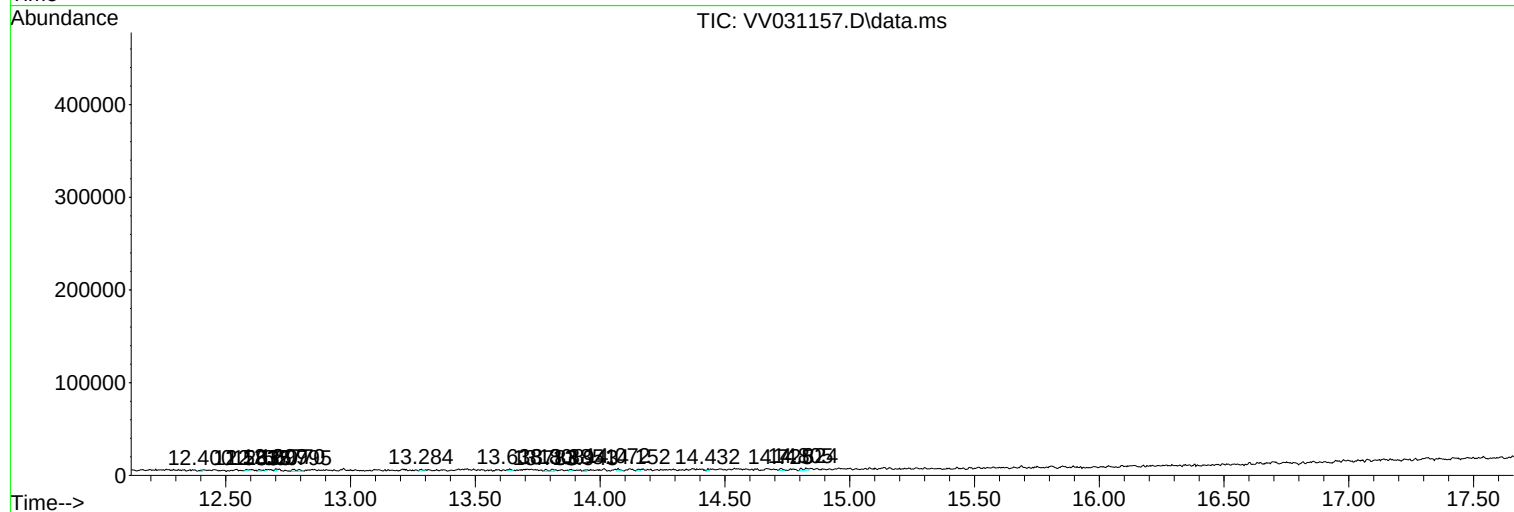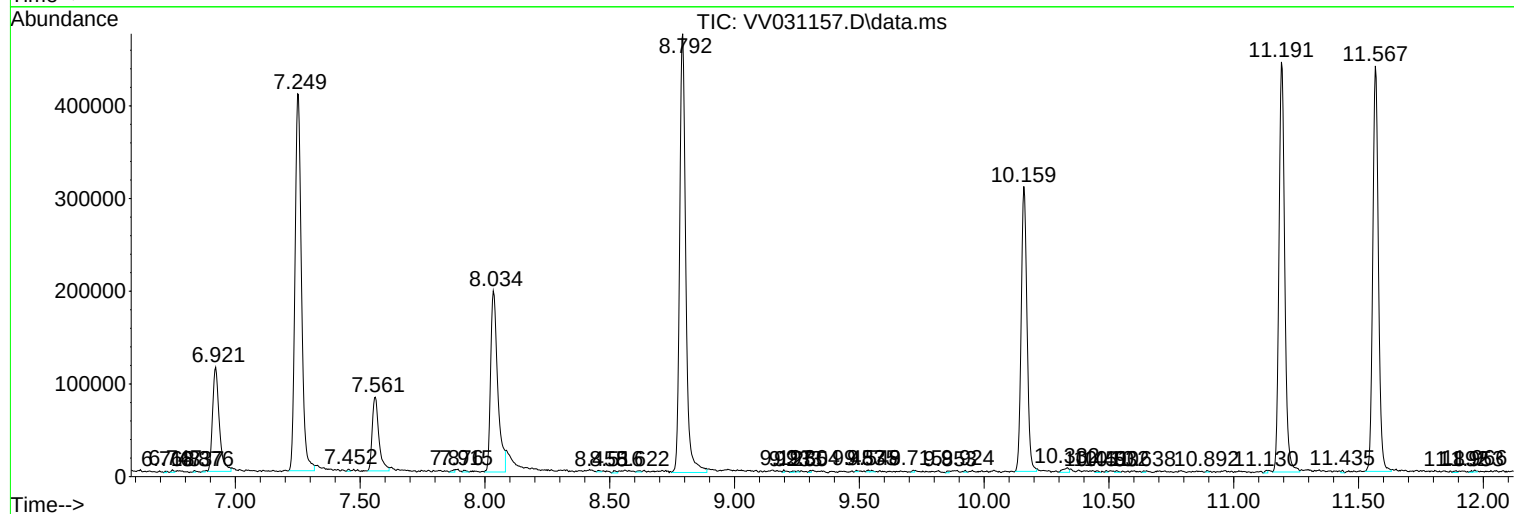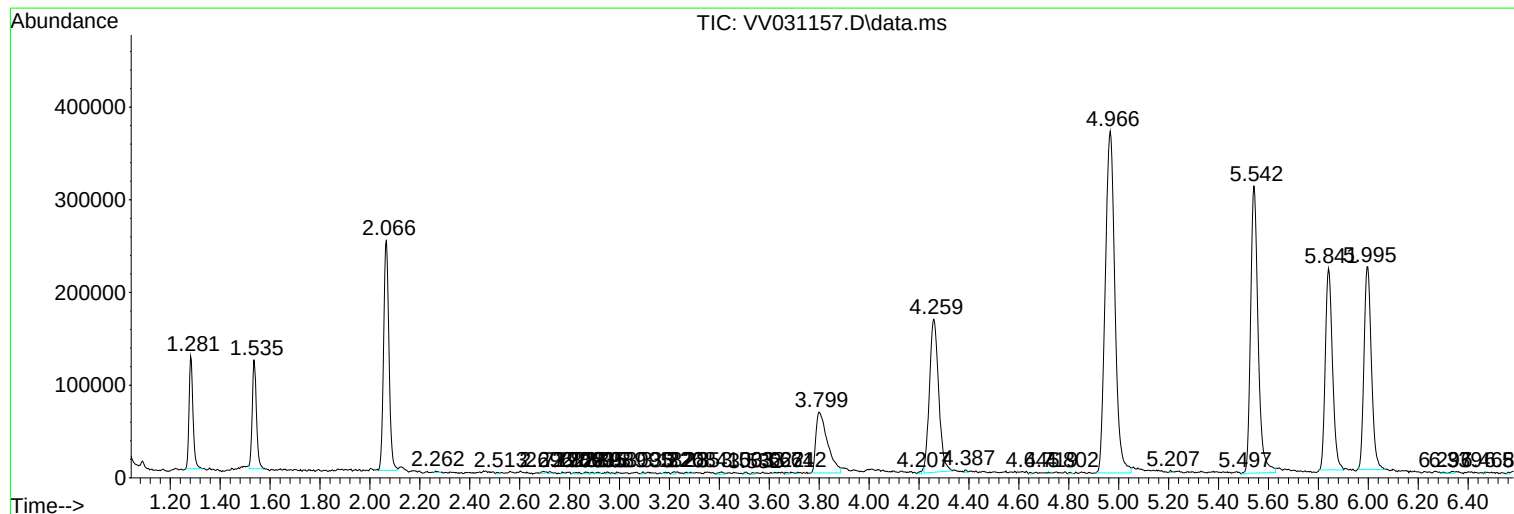

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031157.D
Acq On : 22 May 2023 11:48
Operator : SY/MD
Sample : 02866-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031157.D
Acq On : 22 May 2023 11:48
Operator : SY/MD
Sample : 02866-09DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX84DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------