

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031158.D
 Acq On : 22 May 2023 12:12
 Operator : SY/MD
 Sample : 02866-10DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX85DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	93	rVB	112714	131823	14.61%	1.801%
2	1.539	148	155	169	rVB	114248	136899	15.17%	1.871%
3	2.066	309	319	334	rBV	232873	346331	38.37%	4.732%
4	2.648	498	500	502	rBV3	1373	776	0.09%	0.011%
5	2.770	534	538	541	rBV5	1361	1138	0.13%	0.016%
6	2.870	565	569	572	rBV5	1278	823	0.09%	0.011%
7	2.937	588	590	592	rBV3	1595	1034	0.11%	0.014%
8	3.031	616	619	621	rBV4	2101	1549	0.17%	0.021%
9	3.339	714	715	716	rBV2	1323	407	0.05%	0.006%
10	3.368	721	724	728	rVV7	1467	1325	0.15%	0.018%
11	3.449	745	749	750	rBV3	1996	1360	0.15%	0.019%
12	3.545	778	779	781	rBV3	1083	449	0.05%	0.006%
13	3.593	791	794	795	rBV3	1743	1080	0.12%	0.015%
14	3.699	824	827	829	rBV4	1448	762	0.08%	0.010%
15	3.767	845	848	850	rBV3	2218	1881	0.21%	0.026%
16	3.802	850	859	884	rVV	55892	162636	18.02%	2.222%
17	4.166	970	972	973	rBV2	1795	816	0.09%	0.011%
18	4.259	987	1001	1026	rBV	154143	384099	42.56%	5.248%
19	4.587	1099	1103	1107	rBV5	2401	2246	0.25%	0.031%
20	4.870	1188	1191	1195	rBV7	1923	1662	0.18%	0.023%
21	4.966	1206	1221	1244	rBV2	342149	902497	100.00%	12.332%
22	5.166	1280	1283	1286	rBV5	1833	1597	0.18%	0.022%
23	5.477	1378	1380	1382	rBV4	1433	763	0.08%	0.010%
24	5.542	1388	1400	1421	rBV	290164	600760	66.57%	8.209%
25	5.841	1483	1493	1511	rBV	182846	355889	39.43%	4.863%
26	5.998	1531	1542	1561	rVB	208419	414065	45.88%	5.658%
27	6.455	1680	1684	1688	rBV5	2417	2549	0.28%	0.035%
28	6.522	1701	1705	1706	rBV4	1525	981	0.11%	0.013%
29	6.648	1740	1744	1746	rBV5	2314	1357	0.15%	0.019%
30	6.690	1755	1757	1761	rVB4	1732	1108	0.12%	0.015%
31	6.821	1795	1798	1799	rBV2	1040	596	0.07%	0.008%
32	6.838	1799	1803	1808	rBV7	1426	1432	0.16%	0.020%
33	6.921	1819	1829	1850	rBV	102788	191640	21.23%	2.619%
34	7.188	1907	1912	1915	rVB6	2012	1517	0.17%	0.021%
35	7.249	1915	1931	1955	rBV	350667	644350	71.40%	8.804%
36	7.493	2004	2007	2009	rBV4	1547	967	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031158.D
 Acq On : 22 May 2023 12:12
 Operator : SY/MD
 Sample : 02866-10DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX85DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.558	2019	2027	2040	rBV	69595	122678	13.59%	1.676%
38	7.728	2077	2080	2082	rBV3	986	668	0.07%	0.009%
39	7.741	2082	2084	2086	rBV3	1379	659	0.07%	0.009%
40	7.821	2107	2109	2111	rBV3	1186	636	0.07%	0.009%
41	7.860	2118	2121	2123	rBV4	1523	1092	0.12%	0.015%
42	7.979	2157	2158	2164	rVB6	1729	1477	0.16%	0.020%
43	8.034	2165	2175	2207	rBV	170028	371585	41.17%	5.077%
44	8.278	2249	2251	2253	rBV3	2086	1008	0.11%	0.014%
45	8.506	2319	2322	2325	rBV5	1362	1083	0.12%	0.015%
46	8.583	2341	2346	2347	rBV5	1676	1359	0.15%	0.019%
47	8.635	2360	2362	2365	rBV4	950	613	0.07%	0.008%
48	8.792	2399	2411	2430	rBV	401957	678411	75.17%	9.270%
49	8.992	2468	2473	2480	rBV	2140	2571	0.28%	0.035%
50	9.050	2489	2491	2493	rBV4	1036	599	0.07%	0.008%
51	9.117	2509	2512	2514	rBV4	1711	1097	0.12%	0.015%
52	9.136	2514	2518	2520	rVV5	1912	1240	0.14%	0.017%
53	9.175	2528	2530	2533	rBV4	1974	1190	0.13%	0.016%
54	9.249	2549	2553	2558	rVB7	1817	1372	0.15%	0.019%
55	9.297	2566	2568	2570	rVB4	1519	613	0.07%	0.008%
56	9.342	2580	2582	2584	rBV3	1260	633	0.07%	0.009%
57	9.368	2588	2590	2592	rBV3	1780	834	0.09%	0.011%
58	9.407	2599	2602	2605	rVB5	1389	737	0.08%	0.010%
59	9.436	2606	2611	2614	rBV6	1196	1125	0.12%	0.015%
60	9.481	2618	2625	2626	rBV6	1791	1440	0.16%	0.020%
61	9.519	2632	2637	2639	rBV6	1299	829	0.09%	0.011%
62	9.532	2639	2641	2643	rBV3	958	410	0.05%	0.006%
63	9.593	2655	2660	2662	rBV6	1739	1578	0.17%	0.022%
64	9.673	2682	2685	2688	rBV5	1564	1181	0.13%	0.016%
65	9.722	2697	2700	2705	rVB6	1717	1429	0.16%	0.020%
66	9.754	2708	2710	2713	rBV4	1662	787	0.09%	0.011%
67	9.789	2718	2721	2725	rVB6	1721	1210	0.13%	0.017%
68	9.821	2728	2731	2734	rBV5	1387	1062	0.12%	0.015%
69	9.866	2740	2745	2746	rBV4	1168	833	0.09%	0.011%
70	9.905	2755	2757	2761	rVB4	1444	933	0.10%	0.013%
71	9.924	2761	2763	2765	rBV3	1011	437	0.05%	0.006%
72	10.050	2799	2802	2805	rBV6	1289	997	0.11%	0.014%
73	10.159	2824	2836	2852	rBV	290552	469404	52.01%	6.414%
74	10.307	2876	2882	2884	rBV7	2034	1800	0.20%	0.025%
75	10.378	2901	2904	2910	rBV7	1281	1165	0.13%	0.016%
76	10.435	2920	2922	2926	rVB4	1668	812	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031158.D
 Acq On : 22 May 2023 12:12
 Operator : SY/MD
 Sample : 02866-10DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX85DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	10.574	2963	2965	2967	rBV3	1608	562	0.06%	0.008%
78	11.005	3098	3099	3104	rBV4	1446	1239	0.14%	0.017%
79	11.191	3145	3157	3179	rBV	420923	681613	75.53%	9.313%
80	11.439	3230	3234	3241	rBV9	2049	2274	0.25%	0.031%
81	11.490	3246	3250	3252	rBV4	2097	1459	0.16%	0.020%
82	11.567	3263	3274	3291	rBV	392430	631445	69.97%	8.628%
83	12.352	3514	3518	3519	rBV4	1335	916	0.10%	0.013%
84	12.506	3562	3566	3570	rBV8	2013	2201	0.24%	0.030%
85	12.570	3583	3586	3587	rBV3	1498	731	0.08%	0.010%
86	12.802	3656	3658	3659	rBV2	2459	1025	0.11%	0.014%
87	12.837	3664	3669	3670	rBV5	1627	1371	0.15%	0.019%
88	12.905	3688	3690	3692	rBV3	2170	1001	0.11%	0.014%
89	12.969	3707	3710	3713	rBV5	1781	1424	0.16%	0.019%
90	13.365	3831	3833	3835	rBV3	1439	630	0.07%	0.009%
91	13.406	3843	3846	3848	rBV3	2115	905	0.10%	0.012%
92	13.596	3903	3905	3907	rBV3	1158	553	0.06%	0.008%
93	13.641	3915	3919	3921	rBV5	1284	1155	0.13%	0.016%
94	13.680	3930	3931	3934	rBV3	1309	810	0.09%	0.011%
95	13.821	3973	3975	3979	rBV5	1269	888	0.10%	0.012%
96	13.924	4005	4007	4010	rVB4	2123	1087	0.12%	0.015%
97	14.043	4041	4044	4049	rBV8	1752	2132	0.24%	0.029%
98	14.127	4068	4070	4071	rBV2	1924	627	0.07%	0.009%
99	14.178	4084	4086	4087	rBV2	1311	387	0.04%	0.005%
100	14.371	4143	4146	4147	rBV3	2155	1405	0.16%	0.019%




Sum of corrected areas: 7318591

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031158.D
Acq On : 22 May 2023 12:12
Operator : SY/MD
Sample : 02866-10DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

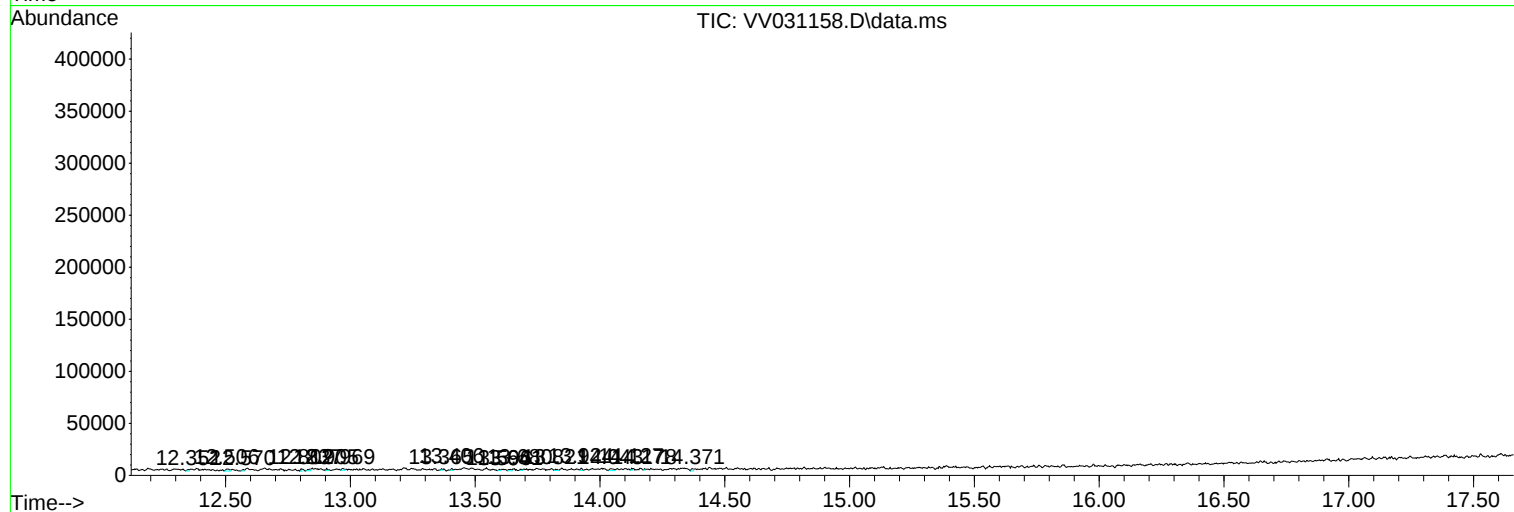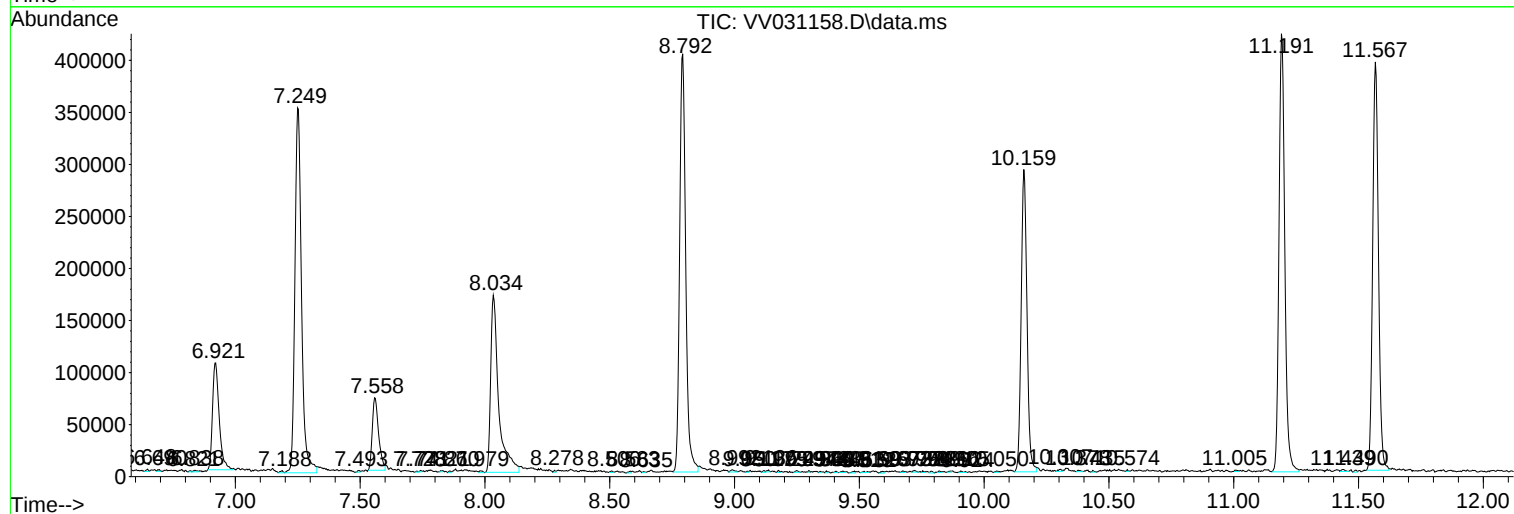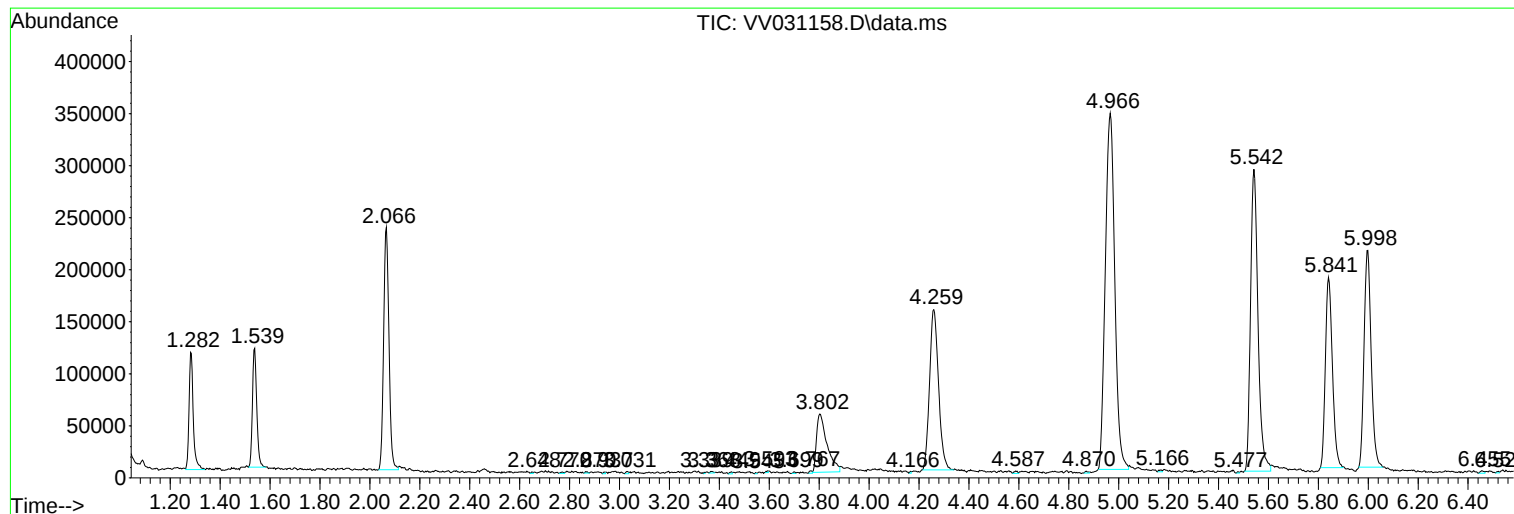

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031158.D
Acq On : 22 May 2023 12:12
Operator : SY/MD
Sample : 02866-10DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031158.D
Acq On : 22 May 2023 12:12
Operator : SY/MD
Sample : 02866-10DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------