

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031159.D
 Acq On : 22 May 2023 12:35
 Operator : SY/MD
 Sample : 02866-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	112795	125997	13.98%	1.633%
2	1.539	148	155	170	rVB	113723	142430	15.81%	1.846%
3	2.066	310	319	333	rVB	227838	332780	36.93%	4.314%
4	2.674	505	508	515	rVB8	2288	2250	0.25%	0.029%
5	2.709	518	519	521	rBV2	1398	664	0.07%	0.009%
6	2.754	530	533	537	rBV5	1892	1546	0.17%	0.020%
7	2.841	558	560	563	rVB4	1505	704	0.08%	0.009%
8	3.178	661	665	668	rBV6	1973	2042	0.23%	0.026%
9	3.304	700	704	708	rBV7	1894	1914	0.21%	0.025%
10	3.349	715	718	721	rBV4	1944	1934	0.21%	0.025%
11	3.448	746	749	755	rVB6	2387	2169	0.24%	0.028%
12	3.481	755	759	760	rBV4	1516	1169	0.13%	0.015%
13	3.609	797	799	802	rBV4	1978	875	0.10%	0.011%
14	3.805	849	860	884	rBV	56403	168153	18.66%	2.180%
15	4.259	989	1001	1020	rVB	149352	366632	40.69%	4.752%
16	4.786	1162	1165	1167	rBV3	2089	1233	0.14%	0.016%
17	4.831	1177	1179	1181	rBV3	1652	981	0.11%	0.013%
18	4.860	1185	1188	1189	rBV3	1754	946	0.10%	0.012%
19	4.966	1205	1221	1248	rBV2	342277	901005	100.00%	11.679%
20	5.256	1305	1311	1314	rBV7	2578	3123	0.35%	0.040%
21	5.500	1385	1387	1388	rBV2	1283	416	0.05%	0.005%
22	5.542	1388	1400	1423	rBV	304319	636711	70.67%	8.253%
23	5.841	1481	1493	1517	rBV	352171	699065	77.59%	9.061%
24	5.998	1530	1542	1560	rBV	207483	422210	46.86%	5.473%
25	6.268	1620	1626	1627	rBV6	2056	1894	0.21%	0.025%
26	6.529	1705	1707	1710	rBV5	1509	911	0.10%	0.012%
27	6.722	1765	1767	1771	rBV4	1401	1034	0.11%	0.013%
28	6.776	1782	1784	1788	rBV4	1526	910	0.10%	0.012%
29	6.918	1820	1828	1851	rVB	98970	183485	20.36%	2.378%
30	7.194	1912	1914	1915	rBV2	1600	807	0.09%	0.010%
31	7.252	1921	1932	1956	rBV	371901	666234	73.94%	8.636%
32	7.561	2020	2028	2046	rBV2	70979	125370	13.91%	1.625%
33	7.985	2158	2160	2161	rBV3	1283	346	0.04%	0.004%
34	8.034	2166	2175	2192	rBV	181215	354530	39.35%	4.595%
35	8.599	2347	2351	2354	rBV6	1873	1711	0.19%	0.022%
36	8.792	2400	2411	2437	rBV	467256	778191	86.37%	10.087%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031159.D
 Acq On : 22 May 2023 12:35
 Operator : SY/MD
 Sample : 02866-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.204	2537	2539	2540	rBV2	1322	575	0.06%	0.007%
38	9.249	2550	2553	2557	rBV6	1382	1403	0.16%	0.018%
39	9.291	2564	2566	2568	rBV3	1397	731	0.08%	0.009%
40	9.570	2649	2653	2655	rBV4	1654	1549	0.17%	0.020%
41	9.628	2667	2671	2675	rBV6	2473	2000	0.22%	0.026%
42	9.705	2693	2695	2698	rBV4	1465	1135	0.13%	0.015%
43	10.001	2785	2787	2790	rVB4	1555	654	0.07%	0.008%
44	10.114	2820	2822	2823	rBV2	1148	530	0.06%	0.007%
45	10.159	2824	2836	2854	rVV	290496	467192	51.85%	6.056%
46	10.406	2911	2913	2915	rVB3	1467	536	0.06%	0.007%
47	10.484	2935	2937	2938	rBV3	1438	490	0.05%	0.006%
48	10.718	3008	3010	3011	rBV2	1810	621	0.07%	0.008%
49	10.760	3021	3023	3025	rBV3	1713	750	0.08%	0.010%
50	10.824	3041	3043	3045	rVB3	2013	676	0.08%	0.009%
51	11.033	3106	3108	3109	rBV2	1198	490	0.05%	0.006%
52	11.046	3110	3112	3114	rVB3	1163	508	0.06%	0.007%
53	11.088	3122	3125	3129	rVB5	2000	1169	0.13%	0.015%
54	11.107	3129	3131	3133	rVB3	1824	895	0.10%	0.012%
55	11.120	3133	3135	3137	rBV3	1281	805	0.09%	0.010%
56	11.191	3145	3157	3177	rBV	431106	683085	75.81%	8.854%
57	11.339	3201	3203	3207	rBV5	1361	1229	0.14%	0.016%
58	11.422	3227	3229	3230	rBV2	1832	831	0.09%	0.011%
59	11.451	3237	3238	3241	rBV3	911	586	0.07%	0.008%
60	11.487	3246	3249	3256	rVB7	2073	1893	0.21%	0.025%
61	11.522	3258	3260	3262	rBV3	1433	812	0.09%	0.011%
62	11.567	3262	3274	3296	rBV	358939	583265	64.73%	7.560%
63	11.712	3317	3319	3323	rBV5	1381	991	0.11%	0.013%
64	11.818	3349	3352	3355	rVB5	2216	922	0.10%	0.012%
65	11.834	3355	3357	3359	rBV3	1347	695	0.08%	0.009%
66	11.866	3365	3367	3369	rBV3	955	543	0.06%	0.007%
67	11.885	3371	3373	3375	rBV3	1128	684	0.08%	0.009%
68	11.914	3380	3382	3385	rBV3	2028	1268	0.14%	0.016%
69	11.972	3397	3400	3402	rBV4	1220	778	0.09%	0.010%
70	11.998	3405	3408	3410	rVB3	1198	651	0.07%	0.008%
71	12.046	3421	3423	3427	rVB5	850	434	0.05%	0.006%
72	12.127	3443	3448	3449	rBV6	1429	1120	0.12%	0.015%
73	12.223	3476	3478	3479	rBV2	995	349	0.04%	0.005%
74	12.265	3489	3491	3493	rVB3	1326	449	0.05%	0.006%
75	12.287	3496	3498	3502	rVV5	1495	839	0.09%	0.011%
76	12.368	3521	3523	3531	rVB9	1548	1254	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031159.D
 Acq On : 22 May 2023 12:35
 Operator : SY/MD
 Sample : 02866-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.413	3535	3537	3540	rVB4	666	406	0.05%	0.005%
78	12.435	3540	3544	3547	rBV4	1811	1527	0.17%	0.020%
79	12.557	3580	3582	3586	rVB5	1454	1112	0.12%	0.014%
80	12.664	3612	3615	3617	rBV3	1573	1063	0.12%	0.014%
81	12.728	3630	3635	3640	rVB7	1771	1355	0.15%	0.018%
82	12.760	3643	3645	3646	rBV2	1362	461	0.05%	0.006%
83	12.853	3673	3674	3677	rBV3	927	499	0.06%	0.006%
84	12.947	3699	3703	3704	rBV3	1434	884	0.10%	0.011%
85	12.969	3708	3710	3713	rVV4	1450	910	0.10%	0.012%
86	13.004	3717	3721	3723	rBV5	1044	637	0.07%	0.008%
87	13.017	3723	3725	3728	rBV4	1265	861	0.10%	0.011%
88	13.056	3735	3737	3740	rBV4	1708	825	0.09%	0.011%
89	13.117	3754	3756	3759	rBV3	1434	505	0.06%	0.007%
90	13.133	3759	3761	3762	rBV2	1188	468	0.05%	0.006%
91	13.178	3773	3775	3777	rVB3	1738	683	0.08%	0.009%
92	13.194	3777	3780	3781	rBV3	1039	628	0.07%	0.008%
93	13.217	3785	3787	3788	rBV2	1338	478	0.05%	0.006%
94	13.316	3816	3818	3819	rVB	1300	351	0.04%	0.005%
95	13.358	3830	3831	3833	rBV2	915	366	0.04%	0.005%
96	13.371	3833	3835	3838	rVV4	1224	615	0.07%	0.008%
97	13.602	3903	3907	3908	rBV4	2217	1477	0.16%	0.019%
98	14.088	4056	4058	4061	rVB4	2234	950	0.11%	0.012%




Sum of corrected areas: 7714820

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031159.D
Acq On : 22 May 2023 12:35
Operator : SY/MD
Sample : 02866-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

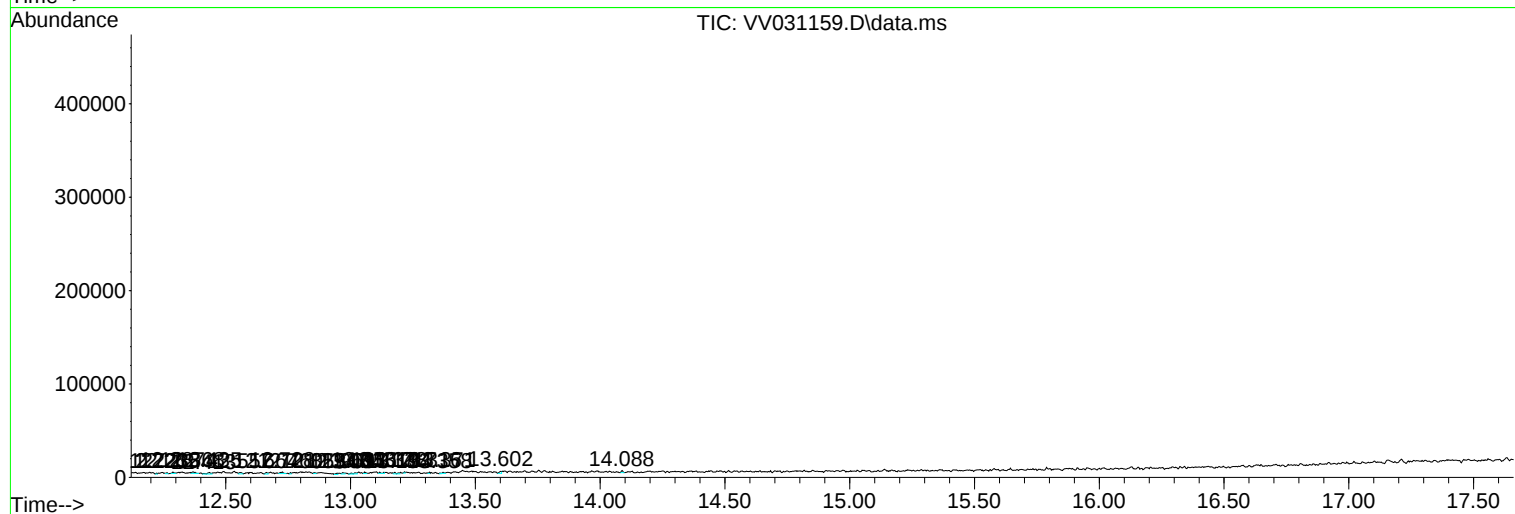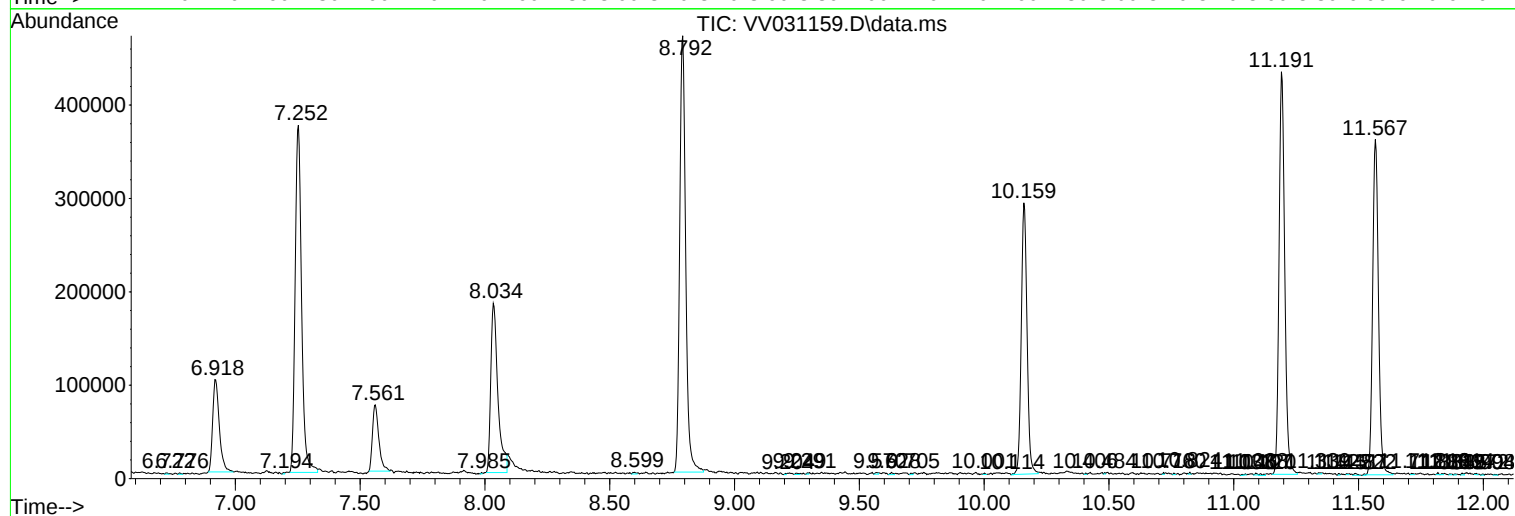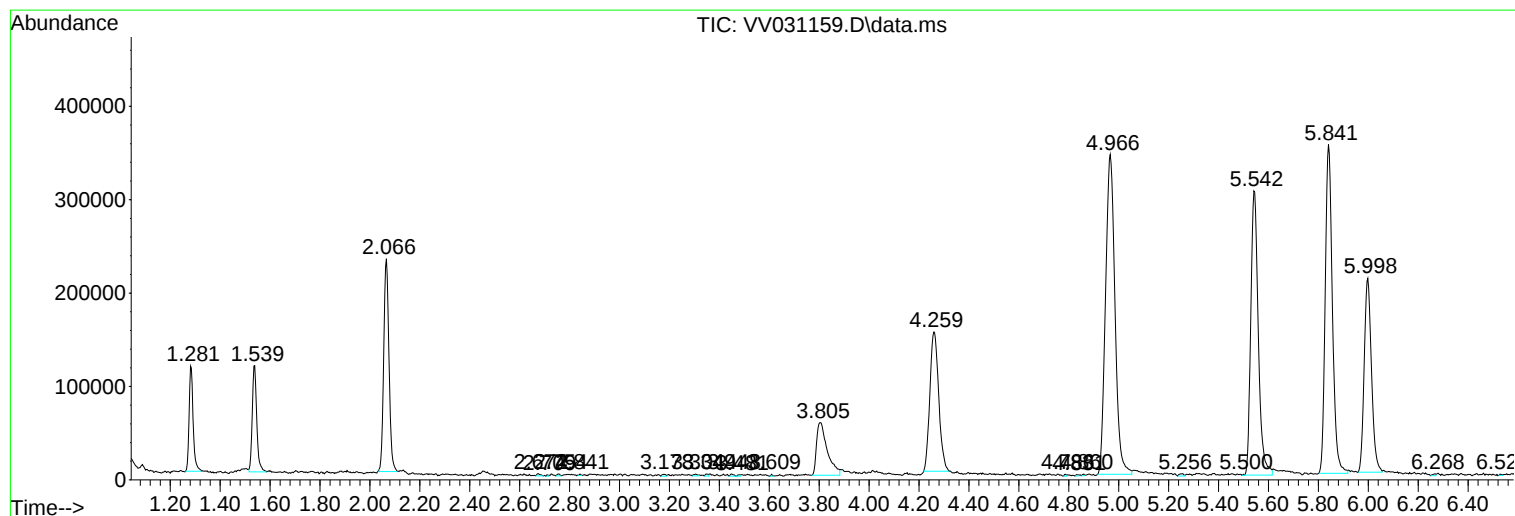

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031159.D
Acq On : 22 May 2023 12:35
Operator : SY/MD
Sample : 02866-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031159.D
Acq On : 22 May 2023 12:35
Operator : SY/MD
Sample : 02866-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------