

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031160.D
 Acq On : 22 May 2023 12:57
 Operator : SY/MD
 Sample : 02866-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	110830	126080	13.50%	1.601%
2	1.536	148	154	167	rVB	113706	136352	14.60%	1.731%
3	2.066	310	319	336	rVB	231155	333421	35.69%	4.233%
4	2.249	374	376	379	rVB4	2250	844	0.09%	0.011%
5	2.320	395	398	400	rBV4	1510	1171	0.13%	0.015%
6	2.458	433	441	456	rBV4	5410	10463	1.12%	0.133%
7	2.574	475	477	480	rBV4	1143	874	0.09%	0.011%
8	2.693	512	514	516	rBV3	1792	951	0.10%	0.012%
9	2.767	533	537	539	rBV4	1819	968	0.10%	0.012%
10	2.851	559	563	564	rBV4	1832	1349	0.14%	0.017%
11	2.925	583	586	588	rBV4	2226	1331	0.14%	0.017%
12	2.947	591	593	598	rBV5	896	710	0.08%	0.009%
13	2.970	598	600	601	rBV2	1355	734	0.08%	0.009%
14	3.227	677	680	682	rBV4	2000	1228	0.13%	0.016%
15	3.275	692	695	696	rBV2	1640	783	0.08%	0.010%
16	3.330	711	712	715	rVB3	1515	737	0.08%	0.009%
17	3.368	722	724	728	rVB5	1203	743	0.08%	0.009%
18	3.452	747	750	752	rBV4	1745	1129	0.12%	0.014%
19	3.490	760	762	765	rBV4	1161	748	0.08%	0.009%
20	3.510	765	768	771	rBV5	1536	1234	0.13%	0.016%
21	3.571	785	787	792	rVB6	1990	1679	0.18%	0.021%
22	3.693	823	825	830	rVB6	1456	1109	0.12%	0.014%
23	3.799	850	858	883	rBV	57722	171244	18.33%	2.174%
24	4.262	988	1002	1026	rVB	163313	396287	42.42%	5.031%
25	4.555	1090	1093	1096	rBV5	1669	1181	0.13%	0.015%
26	4.674	1128	1130	1133	rBV4	1648	807	0.09%	0.010%
27	4.699	1136	1138	1140	rBV3	1746	920	0.10%	0.012%
28	4.886	1193	1196	1197	rBV3	1359	890	0.10%	0.011%
29	4.966	1202	1221	1251	rBV2	347608	934214	100.00%	11.859%
30	5.542	1388	1400	1422	rBV	286440	599827	64.21%	7.614%
31	5.841	1481	1493	1515	rBV	366120	729559	78.09%	9.261%
32	5.998	1530	1542	1559	rBV	206478	424781	45.47%	5.392%
33	6.326	1642	1644	1648	rVB4	2032	1160	0.12%	0.015%
34	6.561	1715	1717	1719	rBV3	1356	756	0.08%	0.010%
35	6.738	1770	1772	1779	rBV8	2010	1560	0.17%	0.020%
36	6.921	1817	1829	1850	rBV2	103676	201004	21.52%	2.552%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031160.D
 Acq On : 22 May 2023 12:57
 Operator : SY/MD
 Sample : 02866-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.059	1870	1872	1875	rBV3	1737	760	0.08%	0.010%
38	7.252	1920	1932	1949	rBV	379135	672706	72.01%	8.540%
39	7.506	2009	2011	2014	rVB4	1819	726	0.08%	0.009%
40	7.561	2019	2028	2044	rBV	76777	134816	14.43%	1.711%
41	7.963	2151	2153	2157	rBV5	1536	980	0.10%	0.012%
42	8.034	2166	2175	2208	rBV	180374	390250	41.77%	4.954%
43	8.452	2302	2305	2306	rBV2	1731	942	0.10%	0.012%
44	8.667	2369	2372	2375	rBV4	1596	1301	0.14%	0.017%
45	8.793	2400	2411	2430	rBV	445385	737004	78.89%	9.356%
46	9.130	2511	2516	2519	rBV4	1956	1923	0.21%	0.024%
47	9.272	2558	2560	2565	rVB6	2065	840	0.09%	0.011%
48	9.310	2568	2572	2574	rBV5	1815	1426	0.15%	0.018%
49	9.368	2588	2590	2597	rBV7	2973	2696	0.29%	0.034%
50	9.545	2642	2645	2647	rBV4	1906	1352	0.14%	0.017%
51	9.635	2672	2673	2678	rBV4	1316	895	0.10%	0.011%
52	9.670	2683	2684	2690	rVB5	1550	992	0.11%	0.013%
53	9.841	2735	2737	2740	rVB4	1665	1075	0.12%	0.014%
54	9.870	2742	2746	2747	rBV4	1857	911	0.10%	0.012%
55	10.159	2824	2836	2848	rBV	292653	463946	49.66%	5.890%
56	10.426	2917	2919	2921	rBV3	1831	886	0.09%	0.011%
57	10.506	2941	2944	2947	rVB4	1651	957	0.10%	0.012%
58	10.593	2969	2971	2975	rVB5	1738	1148	0.12%	0.015%
59	10.725	3008	3012	3015	rBV6	2331	2233	0.24%	0.028%
60	10.789	3029	3032	3033	rBV2	1776	990	0.11%	0.013%
61	10.870	3052	3057	3059	rBV6	1585	1676	0.18%	0.021%
62	10.979	3087	3091	3093	rBV4	1634	1368	0.15%	0.017%
63	11.056	3110	3115	3116	rBV5	1875	1702	0.18%	0.022%
64	11.066	3116	3118	3121	rVB4	2639	1272	0.14%	0.016%
65	11.101	3126	3129	3132	rBV5	1711	1322	0.14%	0.017%
66	11.124	3132	3136	3138	rBV5	2241	1406	0.15%	0.018%
67	11.191	3145	3157	3173	rBV	418991	673049	72.04%	8.544%
68	11.500	3250	3253	3256	rBV5	2301	1155	0.12%	0.015%
69	11.522	3256	3260	3261	rBV3	1735	1352	0.14%	0.017%
70	11.567	3262	3274	3292	rVV	399189	640986	68.61%	8.137%
71	11.857	3361	3364	3367	rBV5	1706	1247	0.13%	0.016%
72	12.037	3416	3420	3423	rBV5	1919	1721	0.18%	0.022%
73	12.053	3423	3425	3429	rVB4	3308	2275	0.24%	0.029%
74	12.085	3429	3435	3437	rBV5	2176	2222	0.24%	0.028%
75	12.178	3462	3464	3465	rBV2	1459	790	0.08%	0.010%
76	12.345	3514	3516	3518	rVB3	1669	740	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031160.D
 Acq On : 22 May 2023 12:57
 Operator : SY/MD
 Sample : 02866-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX87DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.397	3530	3532	3534	rBV3	1480	735	0.08%	0.009%
78	12.480	3556	3558	3560	rBV4	1915	831	0.09%	0.011%
79	12.525	3569	3572	3573	rBV3	1882	973	0.10%	0.012%
80	12.844	3665	3671	3673	rBV6	1976	1987	0.21%	0.025%
81	13.133	3758	3761	3764	rBV5	2140	1307	0.14%	0.017%
82	13.210	3778	3785	3787	rBV8	1952	2153	0.23%	0.027%
83	13.307	3812	3815	3819	rVB6	2525	2187	0.23%	0.028%
84	13.333	3819	3823	3825	rBV4	1930	1616	0.17%	0.021%
85	13.355	3827	3830	3835	rBV6	1801	1716	0.18%	0.022%
86	13.455	3857	3861	3864	rBV6	2478	2315	0.25%	0.029%
87	13.551	3888	3891	3893	rBV3	1898	902	0.10%	0.011%
88	13.564	3893	3895	3898	rBV3	1442	998	0.11%	0.013%
89	13.625	3910	3914	3916	rVB4	1590	998	0.11%	0.013%
90	13.660	3922	3925	3929	rBV6	1570	1358	0.15%	0.017%
91	13.686	3931	3933	3937	rVV5	2056	1442	0.15%	0.018%
92	13.857	3984	3986	3990	rVV5	1228	997	0.11%	0.013%
93	13.882	3992	3994	3998	rVB5	2093	1003	0.11%	0.013%
94	13.914	4000	4004	4005	rBV4	1227	923	0.10%	0.012%
95	14.027	4037	4039	4043	rBV5	1525	1150	0.12%	0.015%
96	14.082	4052	4056	4058	rBV5	1594	764	0.08%	0.010%
97	14.178	4084	4086	4088	rBV3	1539	731	0.08%	0.009%
98	14.480	4176	4180	4183	rBV6	1418	1390	0.15%	0.018%
99	15.204	4401	4405	4408	rBV6	2365	2060	0.22%	0.026%
100	15.676	4548	4552	4556	rBV7	2323	2039	0.22%	0.026%




Sum of corrected areas: 7877441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031160.D
Acq On : 22 May 2023 12:57
Operator : SY/MD
Sample : 02866-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

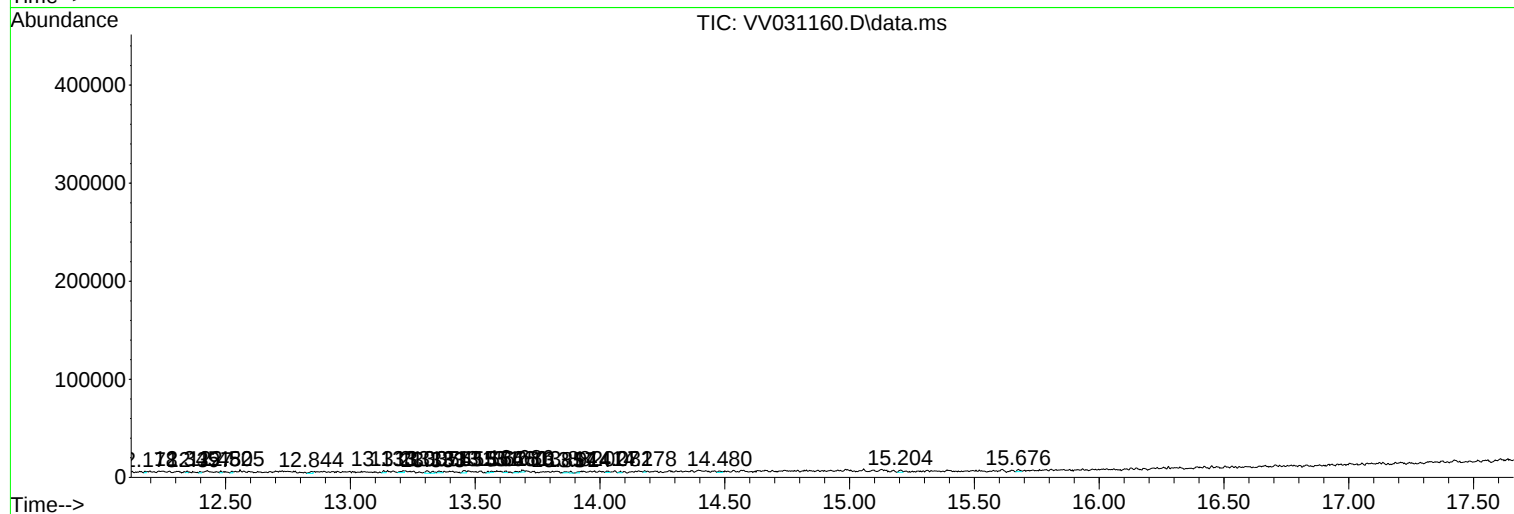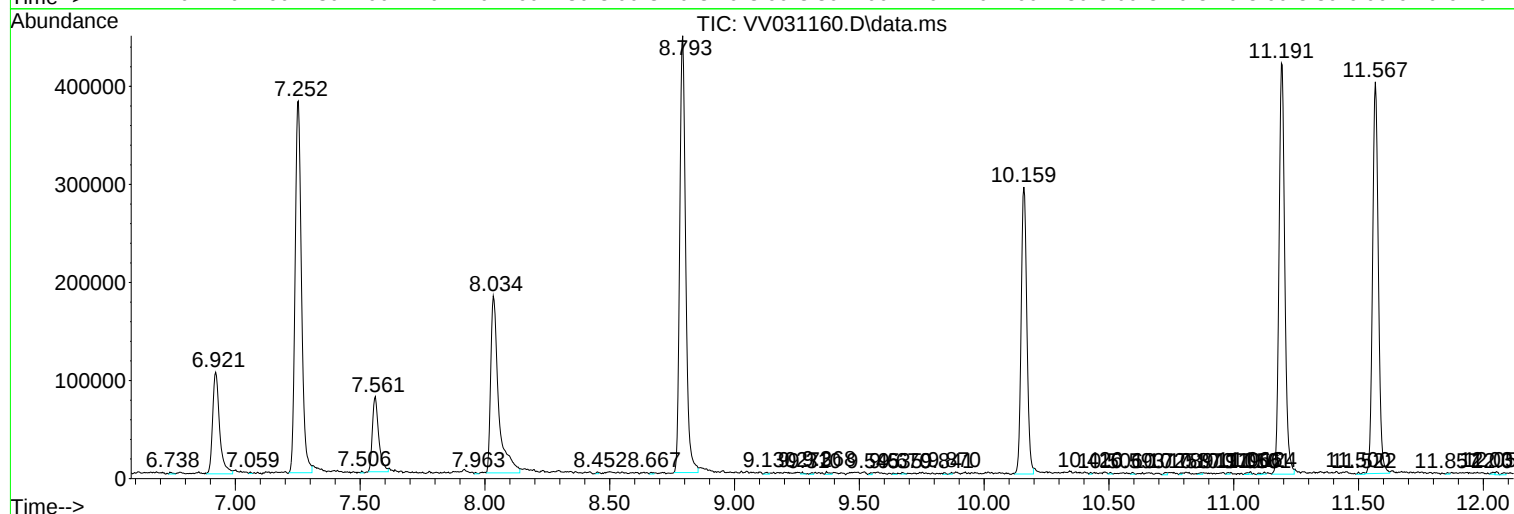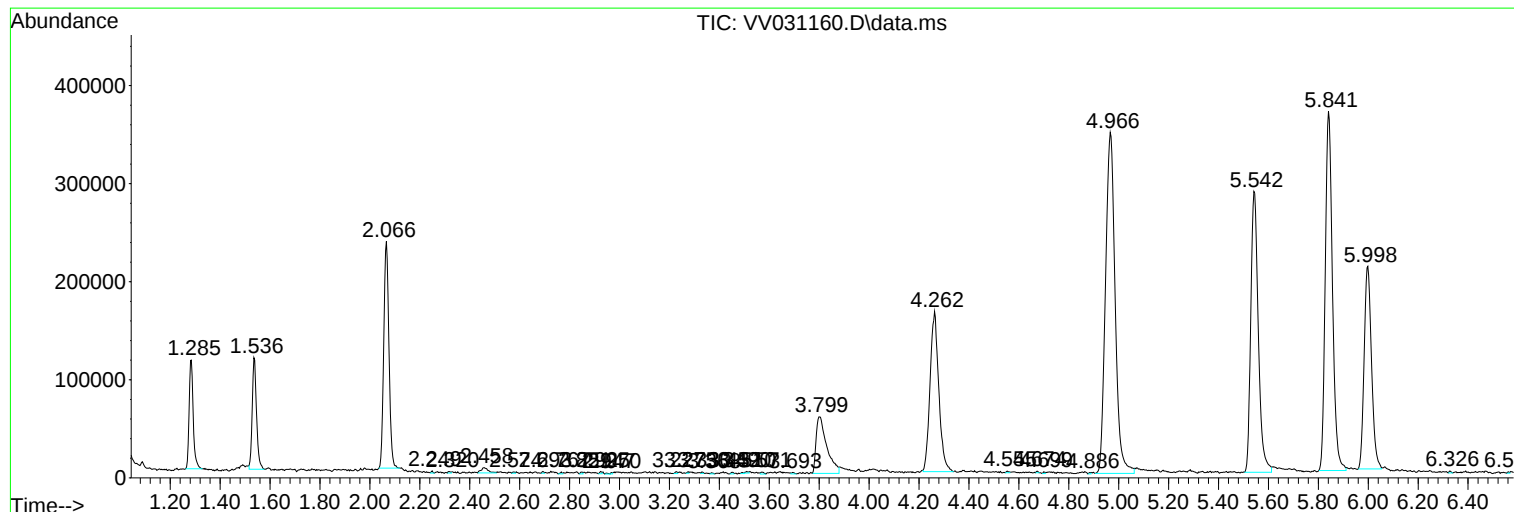

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031160.D
Acq On : 22 May 2023 12:57
Operator : SY/MD
Sample : 02866-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031160.D
Acq On : 22 May 2023 12:57
Operator : SY/MD
Sample : 02866-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------