

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031161.D
 Acq On : 22 May 2023 13:21
 Operator : SY/MD
 Sample : 02866-15DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	88	rVB	80801	89768	10.97%	1.218%
2	1.539	148	155	167	rVB	83285	104609	12.78%	1.420%
3	2.066	310	319	334	rVB	161597	237516	29.03%	3.223%
4	2.410	424	426	429	rVB4	1502	444	0.05%	0.006%
5	2.458	433	441	449	rVV2	11687	20074	2.45%	0.272%
6	2.568	473	475	479	rBV5	1891	1147	0.14%	0.016%
7	2.687	508	512	513	rBV4	1555	1017	0.12%	0.014%
8	2.867	566	568	570	rBV2	920	407	0.05%	0.006%
9	2.879	570	572	573	rVV2	798	241	0.03%	0.003%
10	2.889	573	575	576	rBV2	825	302	0.04%	0.004%
11	3.060	624	628	630	rBV5	1198	786	0.10%	0.011%
12	3.191	666	669	672	rBV4	1249	976	0.12%	0.013%
13	3.278	694	696	699	rBV3	1696	792	0.10%	0.011%
14	3.481	757	759	764	rBV5	1831	1250	0.15%	0.017%
15	3.516	768	770	772	rVV3	1276	673	0.08%	0.009%
16	3.548	776	780	784	rVB6	2120	1582	0.19%	0.021%
17	3.568	784	786	787	rBV2	1019	271	0.03%	0.004%
18	3.603	794	797	798	rBV3	1878	932	0.11%	0.013%
19	3.635	805	807	812	rBV5	1184	988	0.12%	0.013%
20	3.661	812	815	816	rBV3	1274	654	0.08%	0.009%
21	3.712	827	831	833	rBV5	1186	823	0.10%	0.011%
22	3.722	833	834	838	rVB4	1501	605	0.07%	0.008%
23	3.818	847	864	893	rBV3	114079	395963	48.39%	5.373%
24	4.259	988	1001	1023	rBV2	144785	362747	44.33%	4.923%
25	4.497	1073	1075	1080	rBV6	1399	936	0.11%	0.013%
26	4.664	1125	1127	1128	rBV2	918	312	0.04%	0.004%
27	4.754	1153	1155	1161	rBV7	1657	1843	0.23%	0.025%
28	4.783	1162	1164	1165	rBV2	1299	395	0.05%	0.005%
29	4.886	1194	1196	1199	rVB3	1278	769	0.09%	0.010%
30	4.966	1205	1221	1245	rBV2	297599	800000	97.77%	10.856%
31	5.355	1339	1342	1343	rBV3	1133	666	0.08%	0.009%
32	5.542	1385	1400	1426	rBV	317960	664125	81.16%	9.013%
33	5.844	1484	1494	1508	rBV	90072	177397	21.68%	2.407%
34	5.998	1530	1542	1563	rBV	193112	401577	49.08%	5.450%
35	6.284	1628	1631	1634	rVB4	1620	946	0.12%	0.013%
36	6.346	1648	1650	1651	rBV2	1491	610	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031161.D
 Acq On : 22 May 2023 13:21
 Operator : SY/MD
 Sample : 02866-15DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.580	1721	1723	1726	rBV3	1434	1092	0.13%	0.015%
38	6.725	1765	1768	1769	rBV3	1408	632	0.08%	0.009%
39	6.918	1817	1828	1847	rBV	97284	190957	23.34%	2.591%
40	7.149	1898	1900	1904	rVB5	1590	785	0.10%	0.011%
41	7.252	1920	1932	1947	rBV	305716	542244	66.27%	7.359%
42	7.561	2020	2028	2042	rBV	69502	117540	14.36%	1.595%
43	7.960	2150	2152	2154	rBV3	1893	1149	0.14%	0.016%
44	8.034	2164	2175	2204	rBV	201540	434478	53.10%	5.896%
45	8.632	2358	2361	2366	rBV6	1728	1461	0.18%	0.020%
46	8.690	2377	2379	2380	rBV2	1269	641	0.08%	0.009%
47	8.792	2398	2411	2436	rBV	480055	818252	100.00%	11.104%
48	9.091	2502	2504	2506	rBV3	2099	1169	0.14%	0.016%
49	9.181	2530	2532	2534	rBV3	1438	803	0.10%	0.011%
50	9.210	2540	2541	2542	rBV	1654	618	0.08%	0.008%
51	9.452	2613	2616	2619	rBV5	898	591	0.07%	0.008%
52	9.590	2657	2659	2662	rVB4	2213	990	0.12%	0.013%
53	9.670	2680	2684	2689	rBV7	2046	1941	0.24%	0.026%
54	9.693	2689	2691	2693	rBV3	1317	757	0.09%	0.010%
55	9.776	2715	2717	2719	rBV3	984	431	0.05%	0.006%
56	9.895	2752	2754	2757	rBV4	1361	679	0.08%	0.009%
57	9.947	2768	2770	2774	rVB4	1349	710	0.09%	0.010%
58	10.104	2816	2819	2820	rBV3	1747	942	0.12%	0.013%
59	10.159	2823	2836	2856	rVV	316776	512096	62.58%	6.949%
60	10.365	2898	2900	2901	rBV2	1778	597	0.07%	0.008%
61	10.419	2915	2917	2919	rVB3	2002	855	0.10%	0.012%
62	10.439	2919	2923	2925	rBV4	1443	1108	0.14%	0.015%
63	10.660	2989	2992	2993	rBV3	1153	534	0.07%	0.007%
64	10.686	2997	3000	3003	rBV5	1723	1321	0.16%	0.018%
65	10.728	3009	3013	3014	rBV3	1911	1240	0.15%	0.017%
66	10.815	3038	3040	3042	rBV3	1012	436	0.05%	0.006%
67	10.853	3048	3052	3053	rBV4	1573	1217	0.15%	0.017%
68	10.976	3088	3090	3091	rBV2	1788	631	0.08%	0.009%
69	11.005	3097	3099	3100	rBV2	1254	532	0.07%	0.007%
70	11.037	3107	3109	3110	rBV	1125	338	0.04%	0.005%
71	11.078	3120	3122	3124	rBV3	1711	840	0.10%	0.011%
72	11.191	3146	3157	3181	rVB	452391	736228	89.98%	9.991%
73	11.448	3233	3237	3238	rBV4	1740	1323	0.16%	0.018%
74	11.567	3262	3274	3293	rBV	426577	683739	83.56%	9.279%
75	11.831	3354	3356	3359	rBV4	1259	652	0.08%	0.009%
76	11.953	3392	3394	3397	rVB4	2444	1384	0.17%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031161.D
 Acq On : 22 May 2023 13:21
 Operator : SY/MD
 Sample : 02866-15DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX90DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.982	3397	3403	3406	rBV7	2476	2497	0.31%	0.034%
78	12.017	3413	3414	3416	rBV	1163	383	0.05%	0.005%
79	12.046	3419	3423	3427	rBV7	1709	1866	0.23%	0.025%
80	12.091	3435	3437	3438	rBV2	1051	540	0.07%	0.007%
81	12.259	3487	3489	3490	rBV2	1592	610	0.07%	0.008%
82	12.384	3522	3528	3530	rBV7	2644	3029	0.37%	0.041%
83	12.419	3538	3539	3541	rBV2	1178	427	0.05%	0.006%
84	12.432	3541	3543	3545	rBV3	1146	630	0.08%	0.009%
85	12.474	3552	3556	3560	rBV6	1734	1853	0.23%	0.025%
86	12.715	3629	3631	3632	rBV2	1069	320	0.04%	0.004%
87	12.776	3646	3650	3651	rBV4	1191	752	0.09%	0.010%
88	12.853	3672	3674	3675	rBV2	1907	638	0.08%	0.009%
89	12.956	3702	3706	3708	rBV4	1282	886	0.11%	0.012%
90	13.133	3755	3761	3765	rBV9	3323	3545	0.43%	0.048%
91	13.156	3766	3768	3770	rBV2	1690	750	0.09%	0.010%
92	13.210	3781	3785	3787	rBV5	1407	1018	0.12%	0.014%
93	13.551	3887	3891	3895	rBV6	2526	2244	0.27%	0.030%
94	13.631	3914	3916	3918	rBV3	1195	293	0.04%	0.004%
95	13.802	3968	3969	3971	rBV2	1532	653	0.08%	0.009%
96	13.924	4005	4007	4008	rBV2	1431	517	0.06%	0.007%
97	13.995	4022	4029	4031	rBV9	2178	2648	0.32%	0.036%
98	14.136	4069	4073	4075	rVB5	1972	1478	0.18%	0.020%
99	14.156	4075	4079	4083	rBV7	2118	1913	0.23%	0.026%
100	14.545	4195	4200	4201	rBV4	1674	1321	0.16%	0.018%




Sum of corrected areas: 7368887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031161.D
Acq On : 22 May 2023 13:21
Operator : SY/MD
Sample : 02866-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

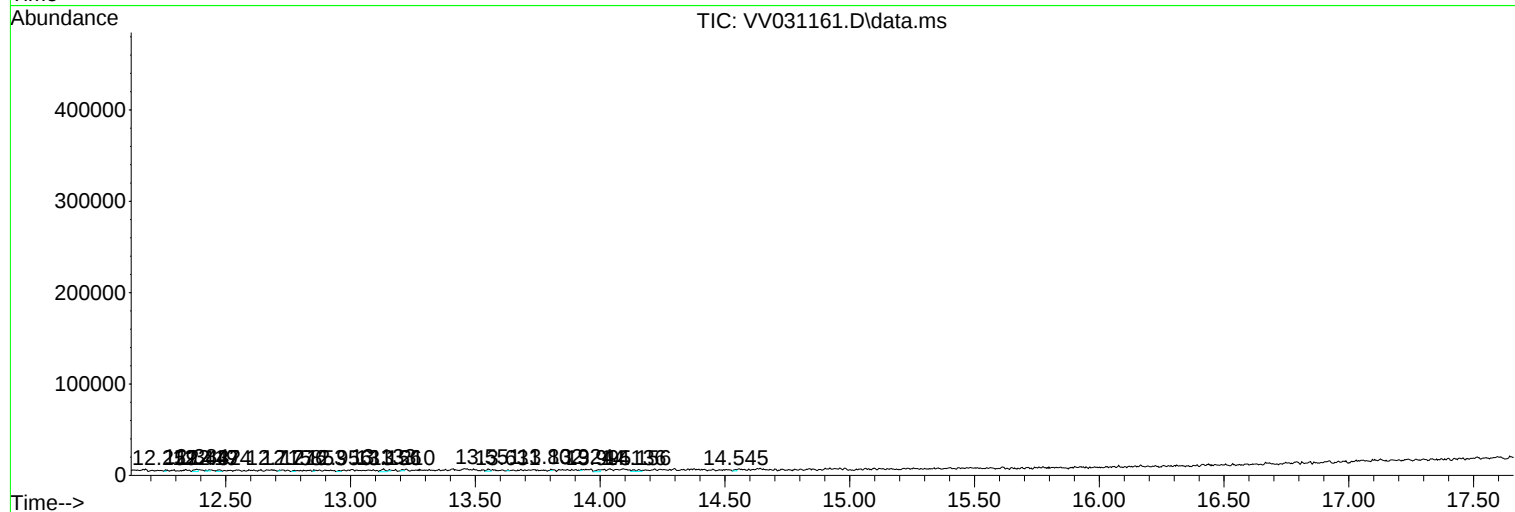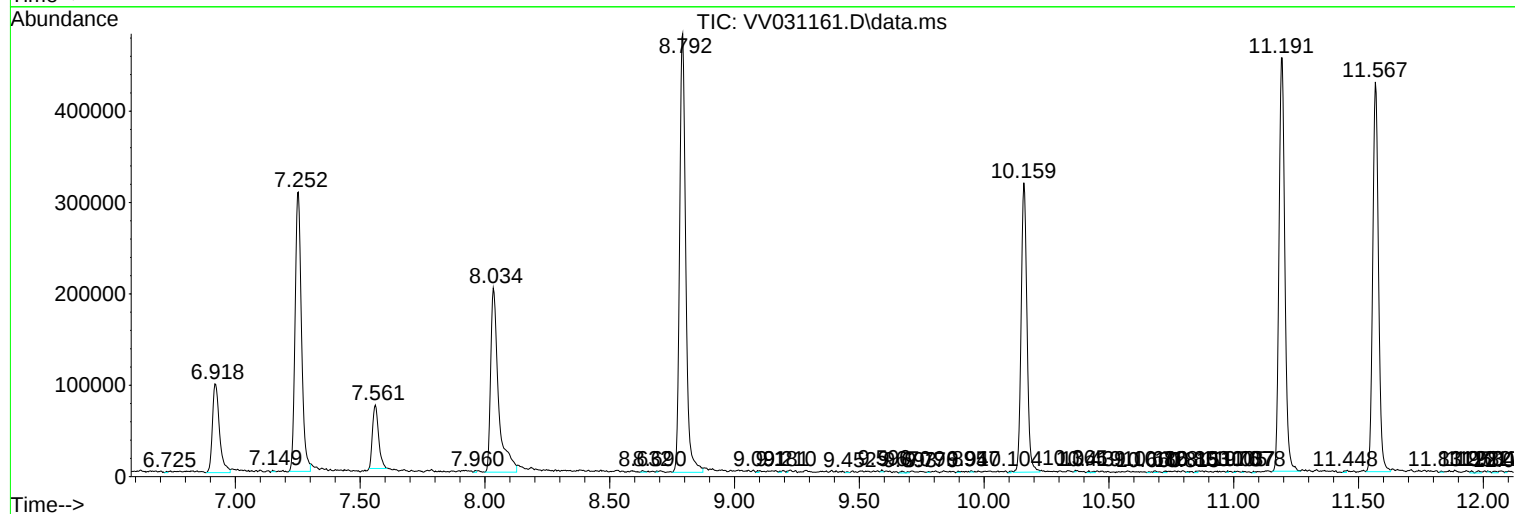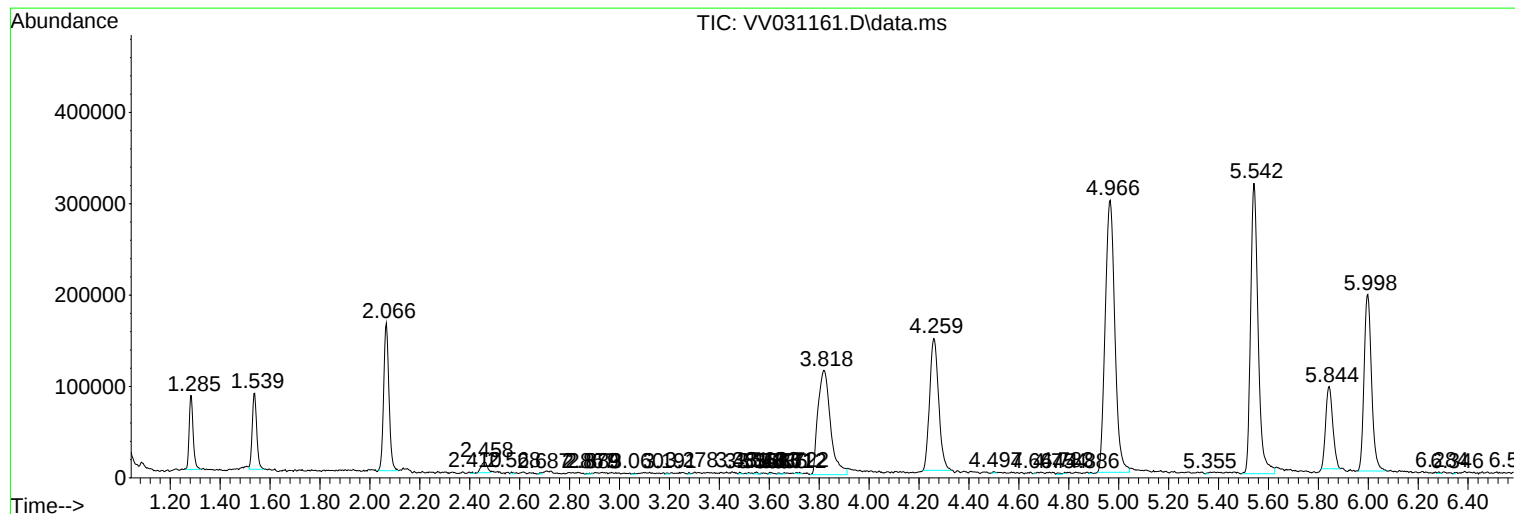

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031161.D
Acq On : 22 May 2023 13:21
Operator : SY/MD
Sample : 02866-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031161.D
Acq On : 22 May 2023 13:21
Operator : SY/MD
Sample : 02866-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------