

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031162.D
 Acq On : 22 May 2023 13:44
 Operator : SY/MD
 Sample : 02866-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	90	rVB	110853	123335	13.96%	1.673%
2	1.539	148	155	171	rVB	113211	140588	15.91%	1.907%
3	2.066	310	319	331	rBV	228818	328989	37.23%	4.462%
4	2.285	384	387	391	rVB6	2353	1924	0.22%	0.026%
5	2.304	391	393	402	rBV9	2055	2067	0.23%	0.028%
6	2.458	435	441	448	rVB4	7849	11150	1.26%	0.151%
7	2.577	476	478	480	rBV3	1100	598	0.07%	0.008%
8	2.658	500	503	504	rBV4	1348	807	0.09%	0.011%
9	3.018	610	615	616	rBV5	1891	1412	0.16%	0.019%
10	3.256	685	689	691	rBV5	2796	2402	0.27%	0.033%
11	3.387	728	730	733	rVB4	2430	1184	0.13%	0.016%
12	3.429	739	743	747	rVB7	1441	1214	0.14%	0.016%
13	3.449	747	749	753	rBV4	1970	1497	0.17%	0.020%
14	3.474	753	757	759	rBV5	1337	1044	0.12%	0.014%
15	3.522	770	772	776	rBV5	1499	778	0.09%	0.011%
16	3.619	800	802	803	rBV2	1163	460	0.05%	0.006%
17	3.693	821	825	830	rBV7	1667	1805	0.20%	0.024%
18	3.715	830	832	834	rVB2	1505	484	0.05%	0.007%
19	3.802	850	859	881	rBV2	59628	167582	18.96%	2.273%
20	4.153	966	968	971	rBV4	1518	1066	0.12%	0.014%
21	4.262	987	1002	1018	rBV	153969	383770	43.43%	5.205%
22	4.526	1082	1084	1087	rBV4	1892	1316	0.15%	0.018%
23	4.706	1136	1140	1142	rBV5	2004	1664	0.19%	0.023%
24	4.966	1206	1221	1243	rBV2	334508	883727	100.00%	11.985%
25	5.374	1345	1348	1355	rBV6	2083	2299	0.26%	0.031%
26	5.542	1388	1400	1423	rBV	292803	616974	69.81%	8.368%
27	5.841	1481	1493	1512	rBV	211766	428960	48.54%	5.818%
28	5.998	1531	1542	1562	rVB	205459	417653	47.26%	5.664%
29	6.738	1769	1772	1774	rBV4	1611	1008	0.11%	0.014%
30	6.918	1820	1828	1848	rBV	97955	182736	20.68%	2.478%
31	7.249	1921	1931	1949	rBV	367493	645921	73.09%	8.760%
32	7.561	2019	2028	2040	rBV2	72641	128369	14.53%	1.741%
33	7.931	2141	2143	2148	rBV5	2017	1543	0.17%	0.021%
34	8.034	2166	2175	2204	rBV	186407	394656	44.66%	5.352%
35	8.792	2400	2411	2432	rBV	458685	747854	84.63%	10.143%
36	9.162	2523	2526	2527	rBV3	2670	1209	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031162.D
 Acq On : 22 May 2023 13:44
 Operator : SY/MD
 Sample : 02866-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.194	2532	2536	2538	rBV5	1937	1583	0.18%	0.021%
38	9.506	2631	2633	2634	rBV2	1533	660	0.07%	0.009%
39	9.554	2645	2648	2653	rBV6	1693	1552	0.18%	0.021%
40	9.619	2666	2668	2670	rBV3	1506	636	0.07%	0.009%
41	9.744	2705	2707	2709	rBV3	1604	652	0.07%	0.009%
42	10.021	2791	2793	2796	rVB4	2366	1302	0.15%	0.018%
43	10.040	2796	2799	2800	rBV3	1642	1059	0.12%	0.014%
44	10.159	2825	2836	2851	rBV	290998	464168	52.52%	6.295%
45	10.545	2951	2956	2961	rBV8	2573	3421	0.39%	0.046%
46	10.612	2975	2977	2980	rVB3	2109	884	0.10%	0.012%
47	10.722	3008	3011	3015	rBV6	1864	1497	0.17%	0.020%
48	10.773	3024	3027	3031	rBV5	1901	1222	0.14%	0.017%
49	10.921	3069	3073	3074	rBV3	1104	810	0.09%	0.011%
50	10.976	3086	3090	3091	rBV4	1404	940	0.11%	0.013%
51	11.111	3130	3132	3133	rBV2	1694	525	0.06%	0.007%
52	11.191	3146	3157	3175	rBV	406682	645525	73.05%	8.755%
53	11.484	3246	3248	3250	rBV3	1092	630	0.07%	0.009%
54	11.567	3263	3274	3293	rBV	363098	583035	65.97%	7.907%
55	11.770	3335	3337	3342	rBV6	1606	1252	0.14%	0.017%
56	11.805	3346	3348	3349	rBV2	831	310	0.04%	0.004%
57	12.033	3415	3419	3420	rBV4	1623	790	0.09%	0.011%
58	12.056	3424	3426	3428	rBV3	1248	680	0.08%	0.009%
59	12.091	3435	3437	3440	rBV4	1312	713	0.08%	0.010%
60	12.107	3440	3442	3443	rVV2	1012	259	0.03%	0.004%
61	12.127	3447	3448	3451	rBV3	1127	652	0.07%	0.009%
62	12.172	3460	3462	3464	rBV3	1250	743	0.08%	0.010%
63	12.226	3476	3479	3484	rBV6	1707	1535	0.17%	0.021%
64	12.246	3484	3485	3486	rVV	1078	257	0.03%	0.003%
65	12.271	3486	3493	3496	rVV8	2093	2281	0.26%	0.031%
66	12.307	3500	3504	3505	rBV4	1622	1178	0.13%	0.016%
67	12.316	3505	3507	3513	rVB6	1857	1013	0.11%	0.014%
68	12.451	3547	3549	3551	rBV3	878	369	0.04%	0.005%
69	12.480	3556	3558	3560	rBV3	1742	1166	0.13%	0.016%
70	12.493	3560	3562	3565	rVB3	2228	1043	0.12%	0.014%
71	12.516	3566	3569	3573	rVB5	1758	1229	0.14%	0.017%
72	12.532	3573	3574	3576	rBV2	819	309	0.03%	0.004%
73	12.551	3576	3580	3581	rBV4	954	751	0.08%	0.010%
74	12.580	3586	3589	3594	rBV7	2517	2670	0.30%	0.036%
75	12.619	3598	3601	3604	rBV5	1885	1437	0.16%	0.019%
76	12.805	3655	3659	3660	rBV5	2241	1465	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031162.D
 Acq On : 22 May 2023 13:44
 Operator : SY/MD
 Sample : 02866-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	12.969	3707	3710	3711	rBV4	1617	956	0.11%	0.013%
78	13.001	3716	3720	3722	rBV4	1924	1290	0.15%	0.017%
79	13.313	3815	3817	3822	rBV6	1708	1433	0.16%	0.019%
80	13.374	3834	3836	3838	rBV3	1661	955	0.11%	0.013%
81	13.400	3843	3844	3846	rBV2	843	431	0.05%	0.006%
82	13.432	3852	3854	3857	rBV3	2064	1175	0.13%	0.016%
83	13.477	3864	3868	3872	rBV6	1955	1762	0.20%	0.024%
84	13.863	3986	3988	3990	rBV3	1699	670	0.08%	0.009%
85	14.117	4065	4067	4068	rBV2	1163	410	0.05%	0.006%
86	14.374	4145	4147	4148	rBV2	1712	810	0.09%	0.011%
87	14.618	4221	4223	4227	rBV5	1862	1213	0.14%	0.016%




Sum of corrected areas: 7373353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031162.D
Acq On : 22 May 2023 13:44
Operator : SY/MD
Sample : 02866-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

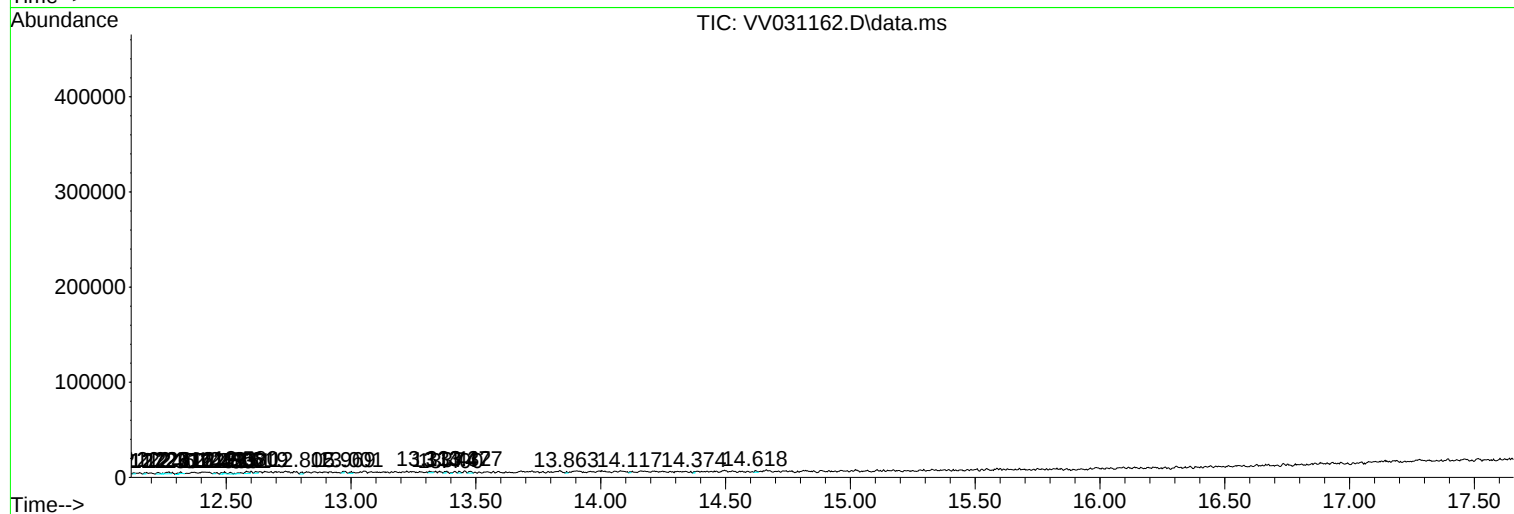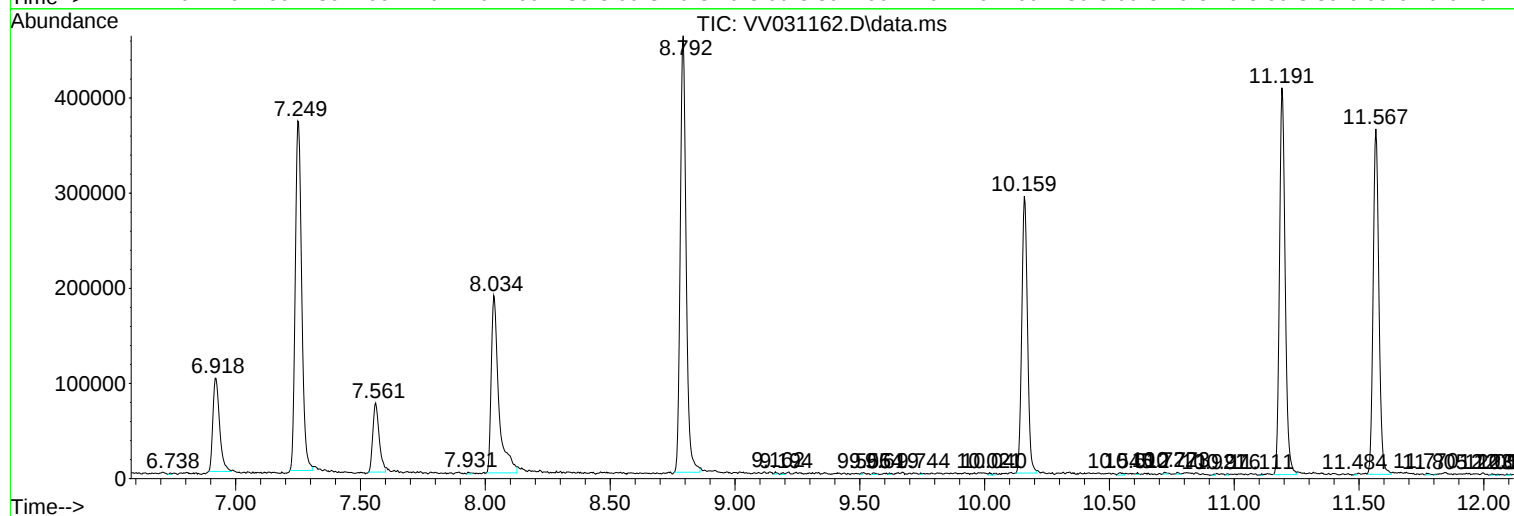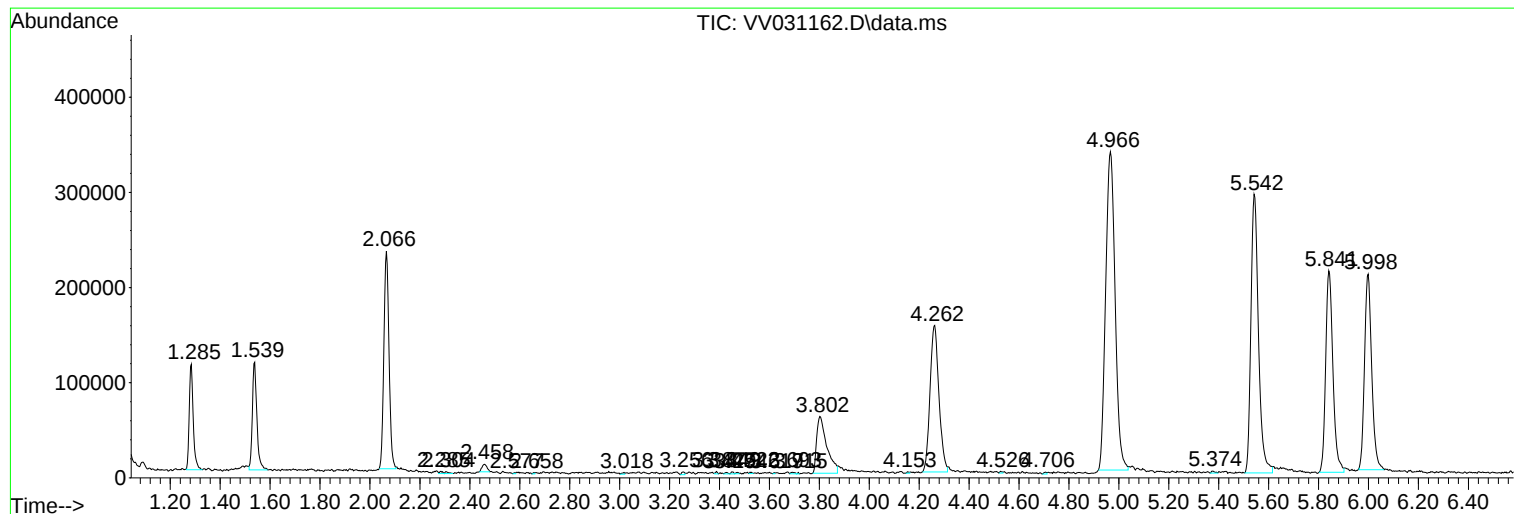

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031162.D
Acq On : 22 May 2023 13:44
Operator : SY/MD
Sample : 02866-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031162.D
Acq On : 22 May 2023 13:44
Operator : SY/MD
Sample : 02866-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------